
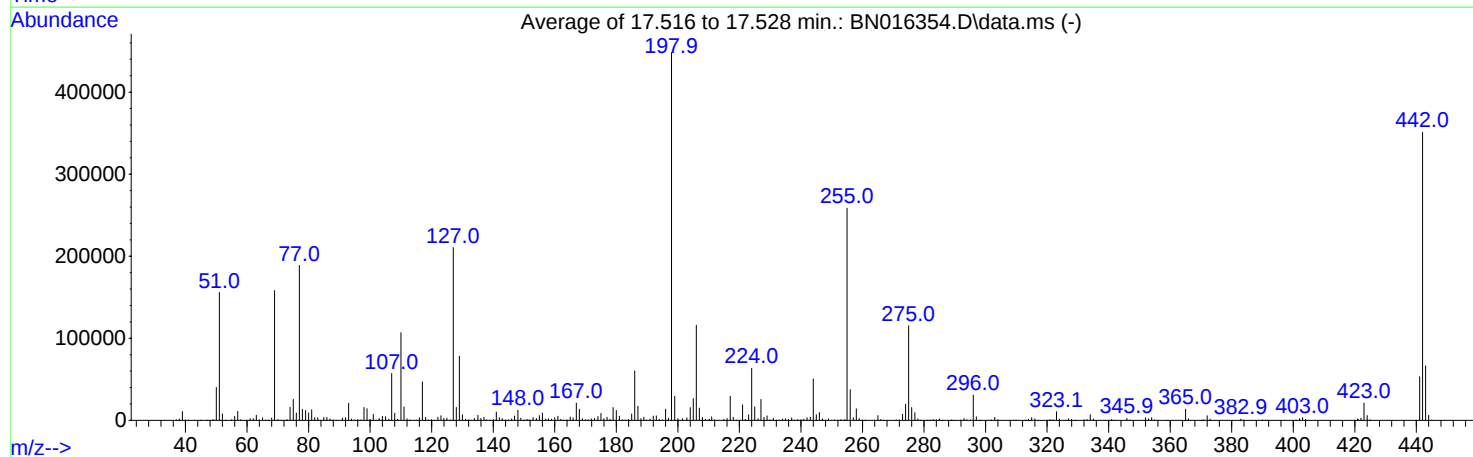


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092021\
 Data File : BN016354.D
 Acq On : 20 Sep 2021 22:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 20 11:09:23 2021

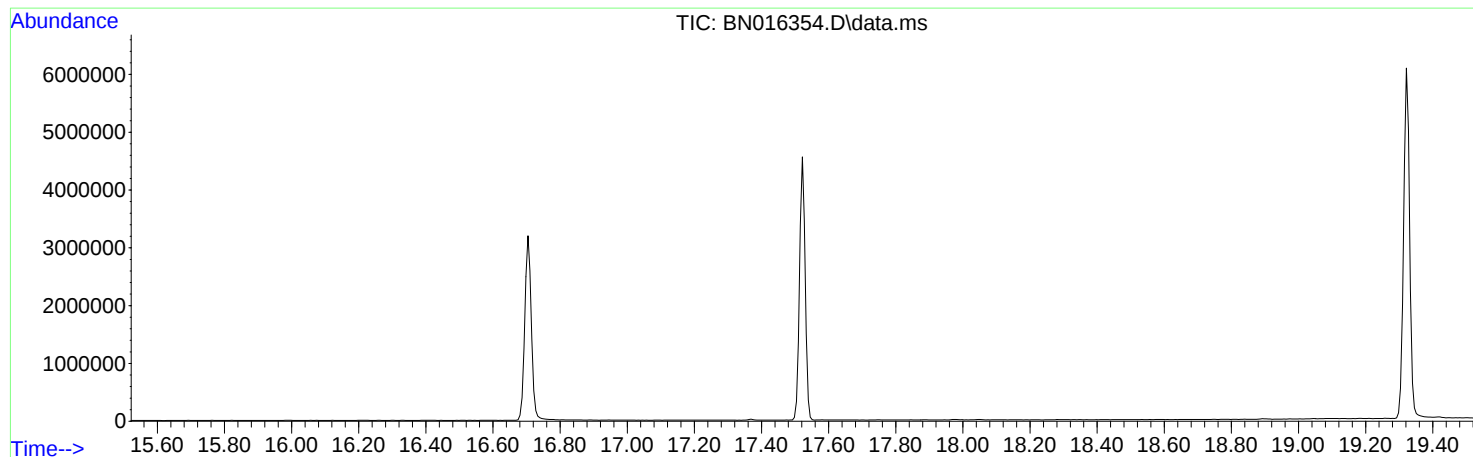




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	155898	PASS
68	69	0.00	2	1.8	2871	PASS
69	198	0.00	100	35.3	158075	PASS
70	69	0.00	2	0.6	978	PASS
127	198	10	80	47.0	210496	PASS
197	198	0.00	2	0.6	2588	PASS
198	198	100	100	100.0	448277	PASS
199	198	5	9	6.6	29544	PASS
275	198	10	60	25.7	115229	PASS
365	198	1	100	3.0	13598	PASS
441	198	0.01	100	11.9	53155	PASS
442	442	50	100	100.0	351189	PASS
443	442	15	24	18.9	66475	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092021\
Data File : BN016354.D
Acq On : 20 Sep 2021 22:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 21 02:16:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 02:16:08 2021
Response via : Initial Calibration

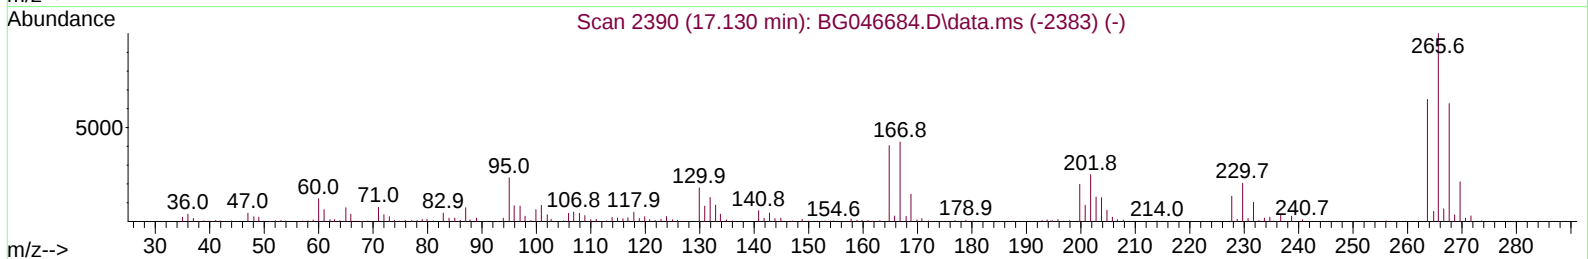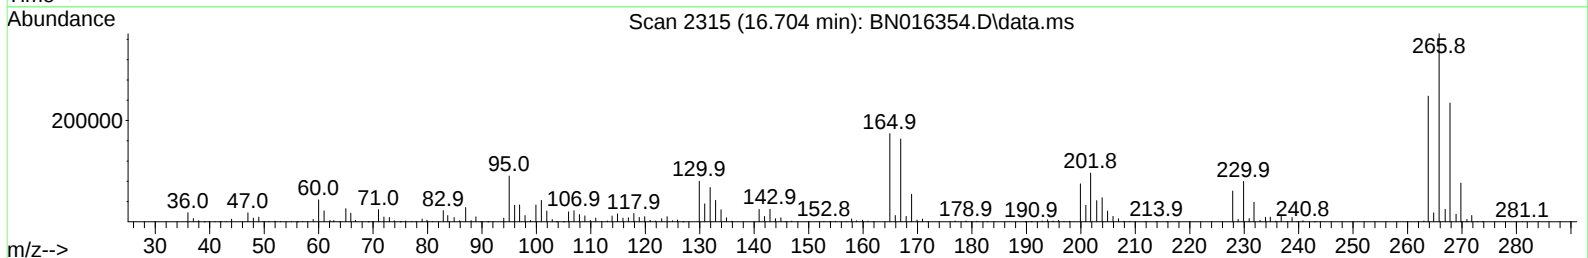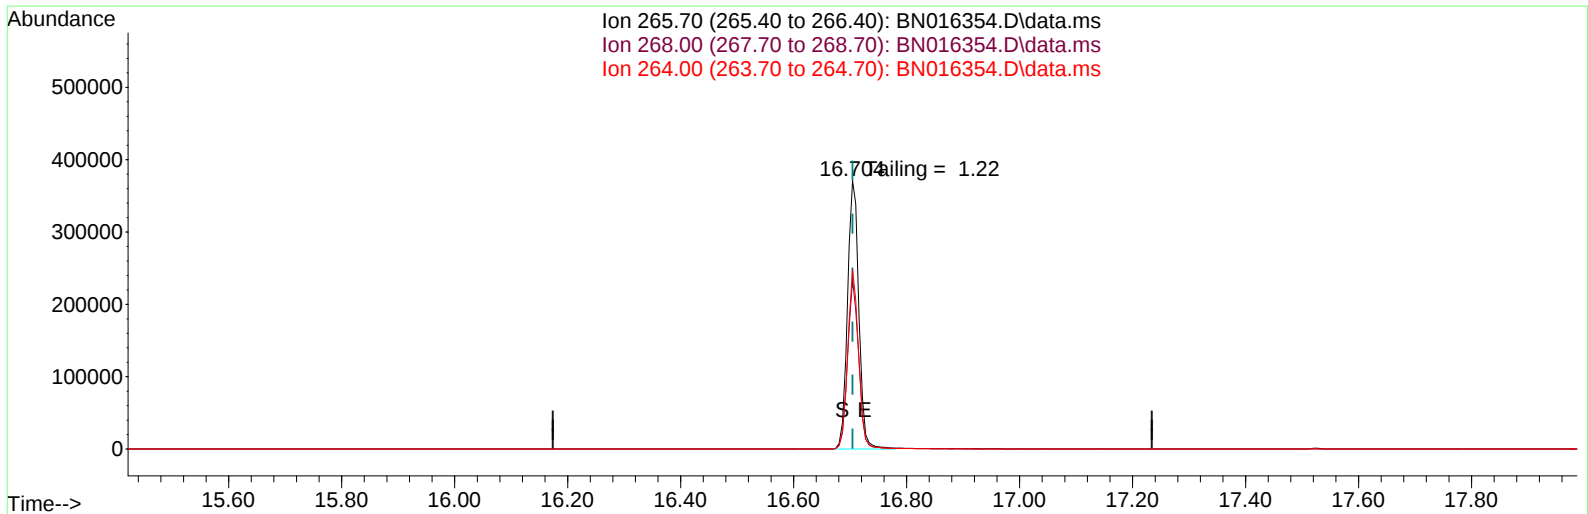

TIC: BN016354.D\data.ms

(70) Pentachlorophenol (C)

16.704min (0.000) 24468.68 ng




response 519233

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.14
264.00	61.60	66.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092021\
Data File : BN016354.D
Acq On : 20 Sep 2021 22:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 21 02:16:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 02:16:08 2021
Response via : Initial Calibration

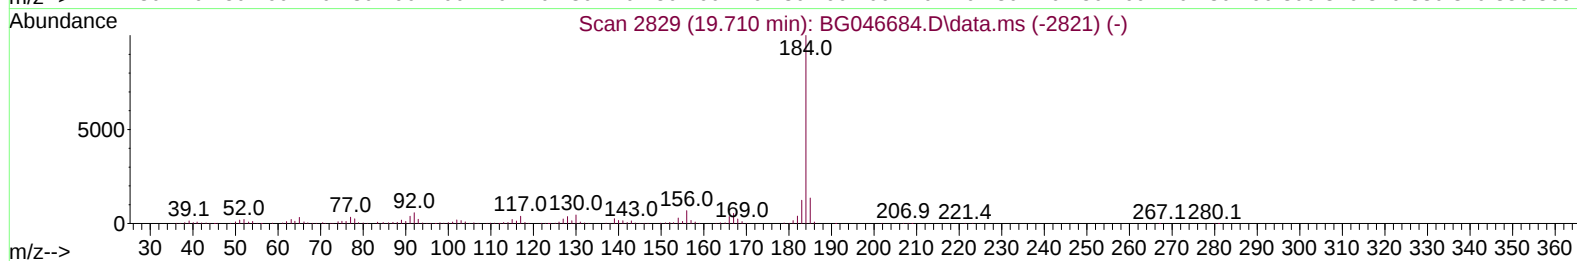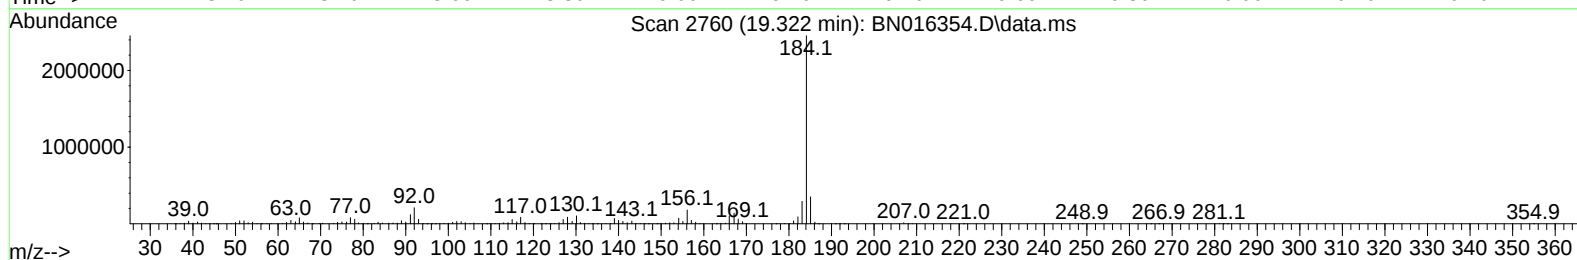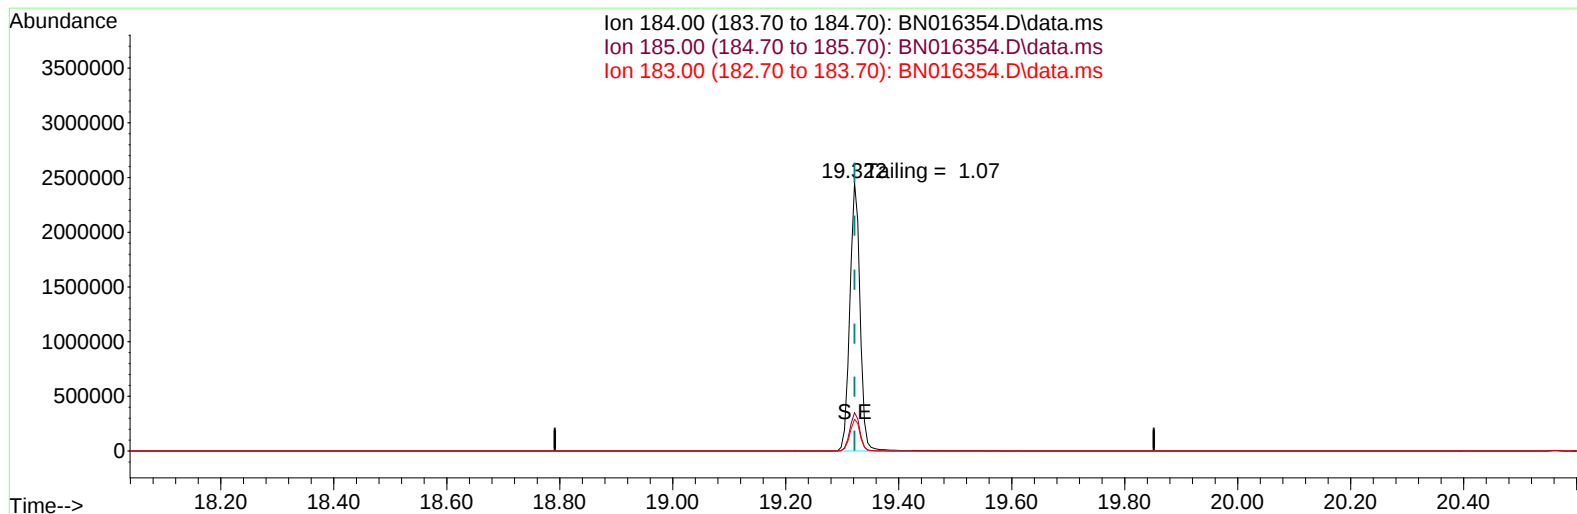

TIC: BN016354.D\data.ms

(77) Benzidine

19.322min (0.000) 0.00 ng

response 3100620

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.32
183.00	13.20	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2021	BNA_N	<u>BN016354.D</u>
Compound Name	Response	Retention Time
DDT	1419543	20.563
DDD	56307	20.122
DDE	3176	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
59483	1479026	4.02

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP