
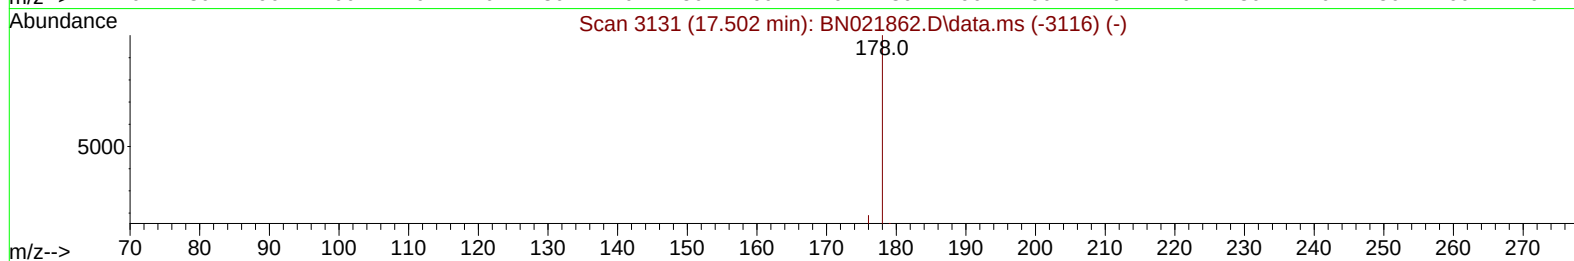
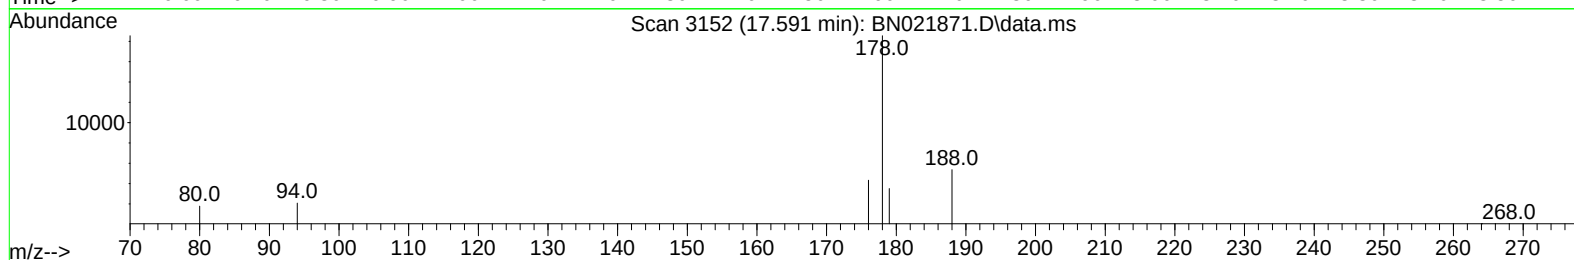


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021871.D
Acq On : 22 Sep 2022 19:15
Operator : CG/JU
Sample : N4706-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Sep 23 02:11:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

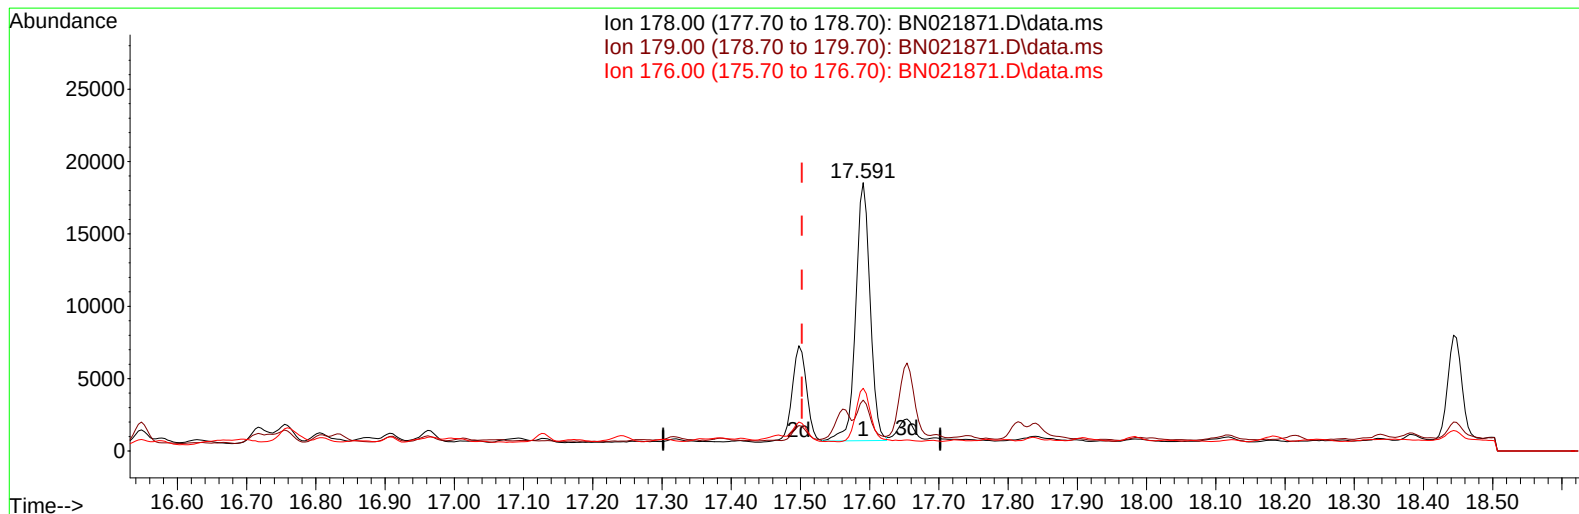

TIC: BN021871.D\data.ms

(15) Phenanthrene

17.591min (+ 0.089) 0.38 ng/u1

response 25695

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.00	18.98
176.00	19.90	23.39
0.00	0.00	0.00