

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021863.D
 Acq On : 22 Sep 2022 10:15
 Operator : CG/JU
 Sample : PB147713BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 23 02:09:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	5111	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	17104	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.707	164	9504	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.455	188	18206	0.400	ng/ul	0.00
17) Chrysene-d12	21.656	240	9612	0.400	ng/ul	# 0.00
23) Perylene-d12	24.158	264	7975	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	36942	5.875	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	8707	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	14307	0.400	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.854	202	1788	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.994	252	2900	0.099	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021863.D
Acq On : 22 Sep 2022 10:15
Operator : CG/JU
Sample : PB147713BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 23 02:09:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




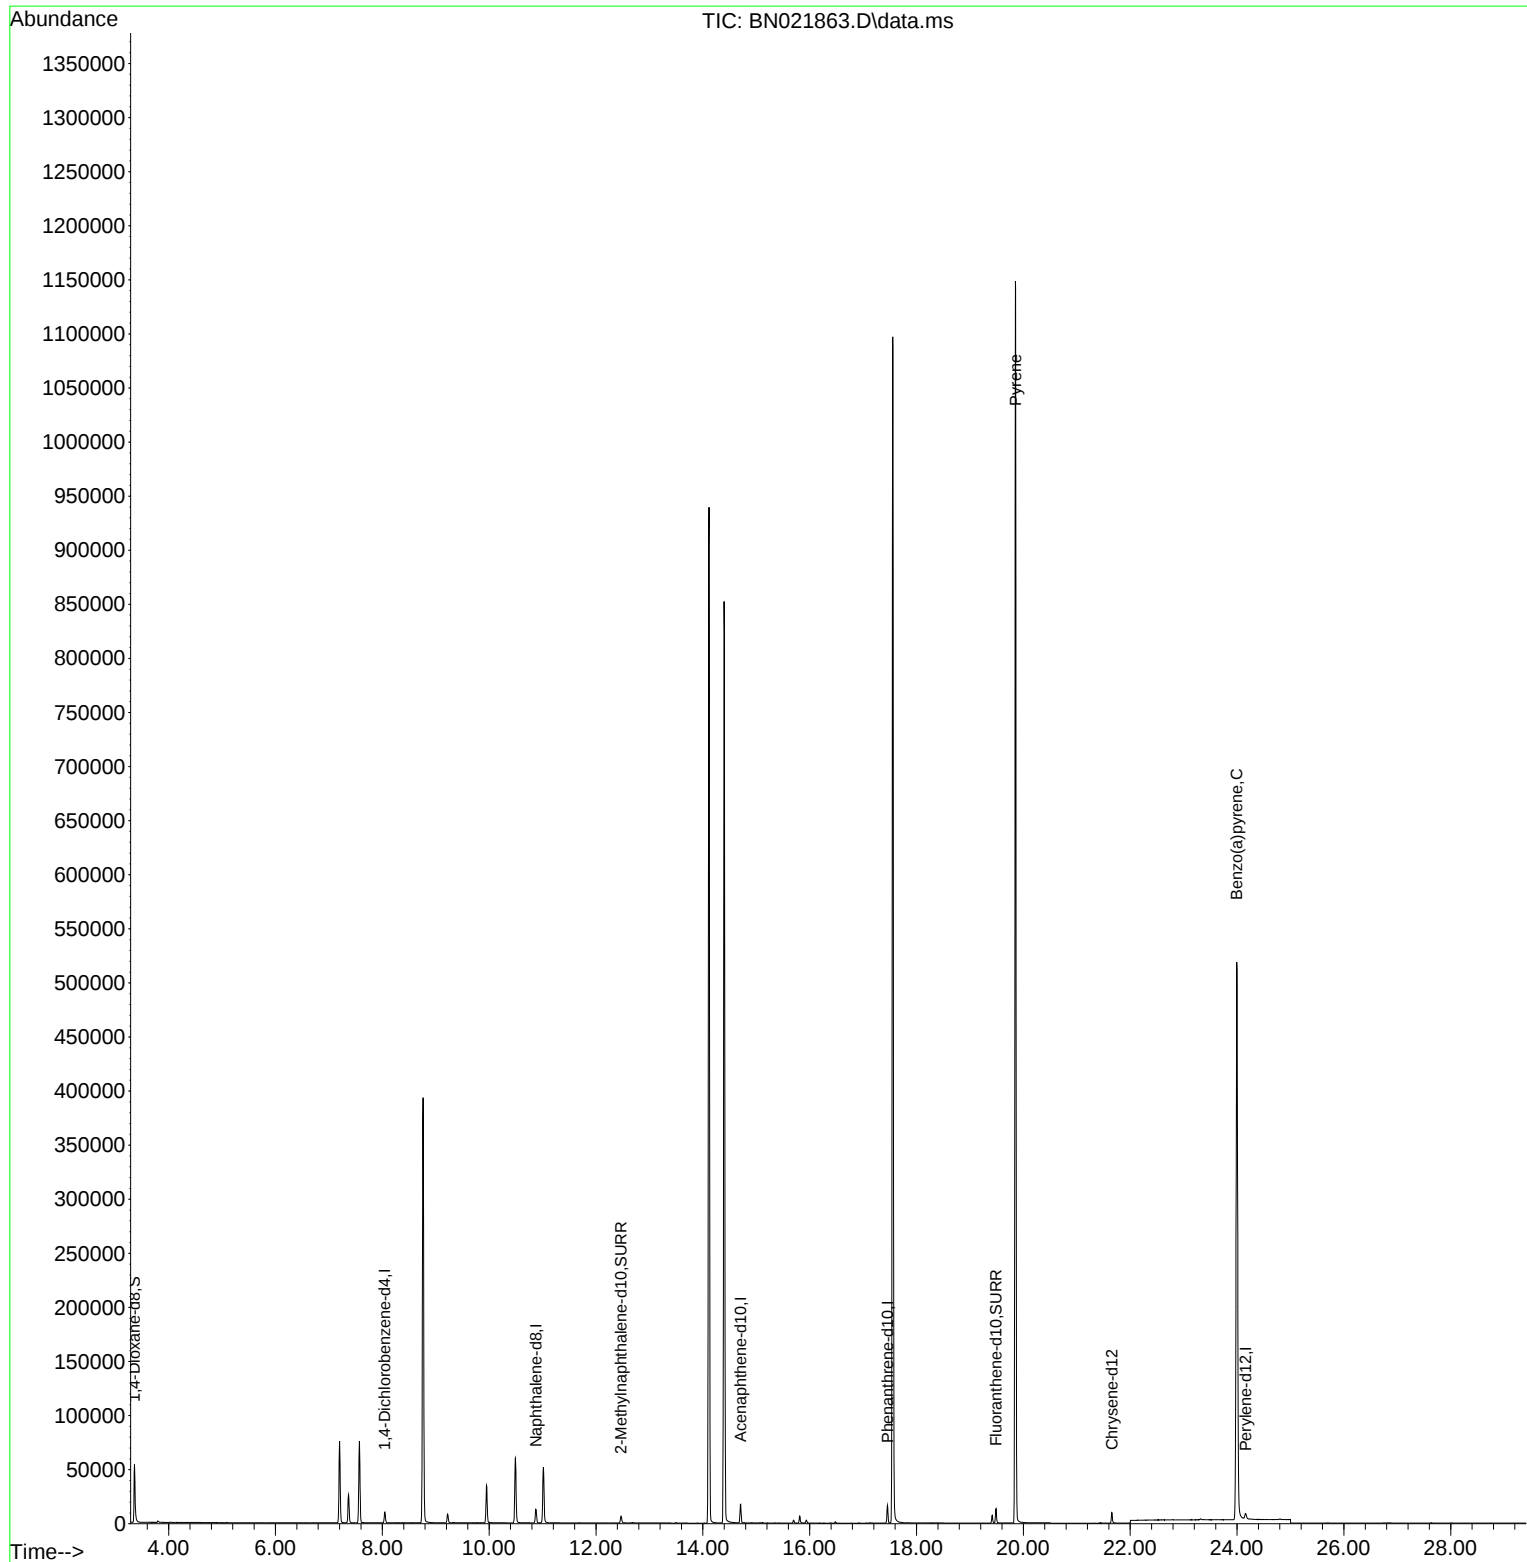


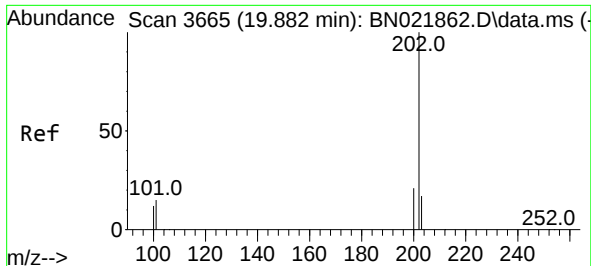

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.854 min Scan# 30
Delta R.T. -0.023 min
Lab File: BN021863.D
Acq: 22 Sep 2022 10:15

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1788
Ion Ratio Lower Upper
202 100
101 163.8 11.3 16.9#
100 1159.6 9.0 13.4#

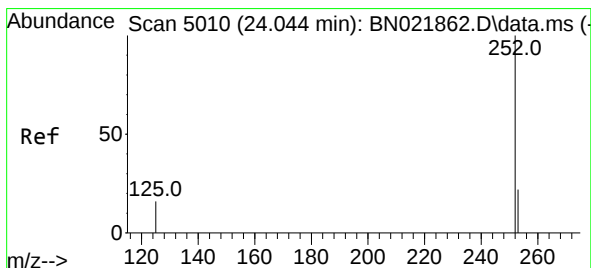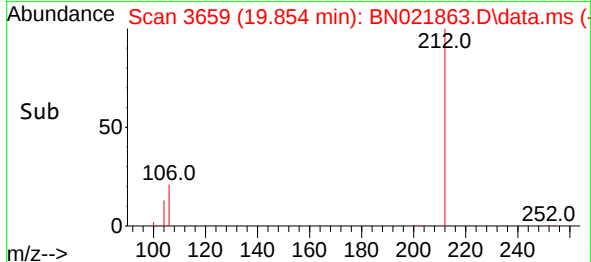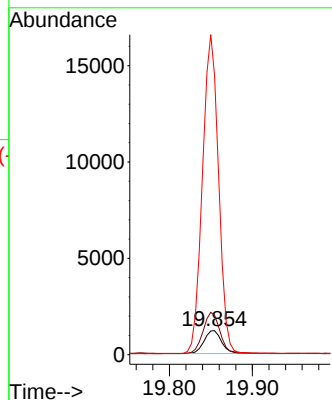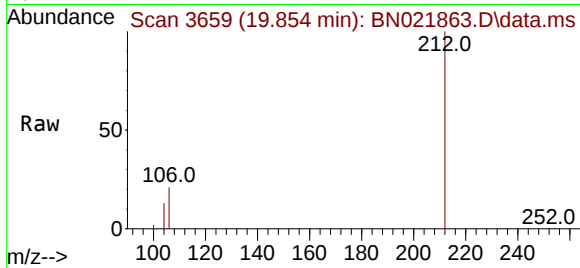

#26
Benzo(a)pyrene
Concen: 0.099 ng/ul
RT: 23.994 min Scan# 4993
Delta R.T. -0.047 min
Lab File: BN021863.D
Acq: 22 Sep 2022 10:15

Tgt Ion:252 Resp: 2900
Ion Ratio Lower Upper
252 100
253 52.2 22.1 33.1#
125 50.7 14.7 22.1#

