




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021904.D
 Acq On : 23 Sep 2022 17:18
 Operator : CG/JU
 Sample : N4706-01DL 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8J8DL

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:02:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/26/2022
 Supervised By :mohammad ahmed 09/26/2022

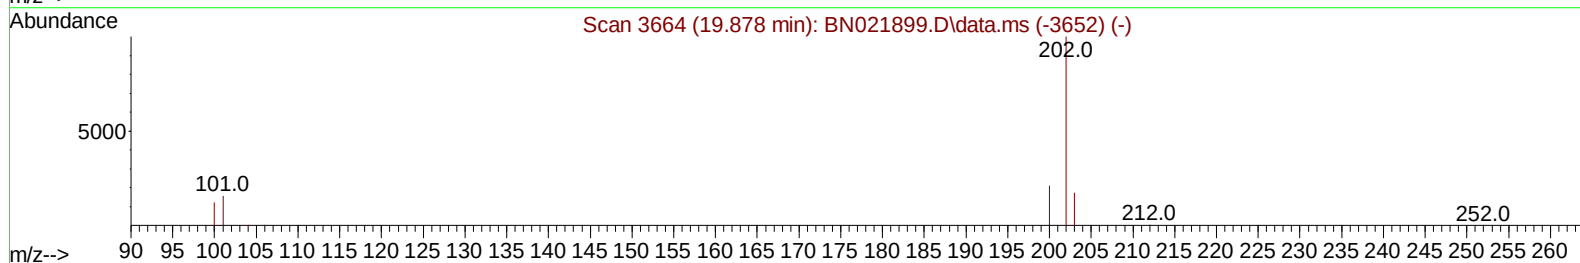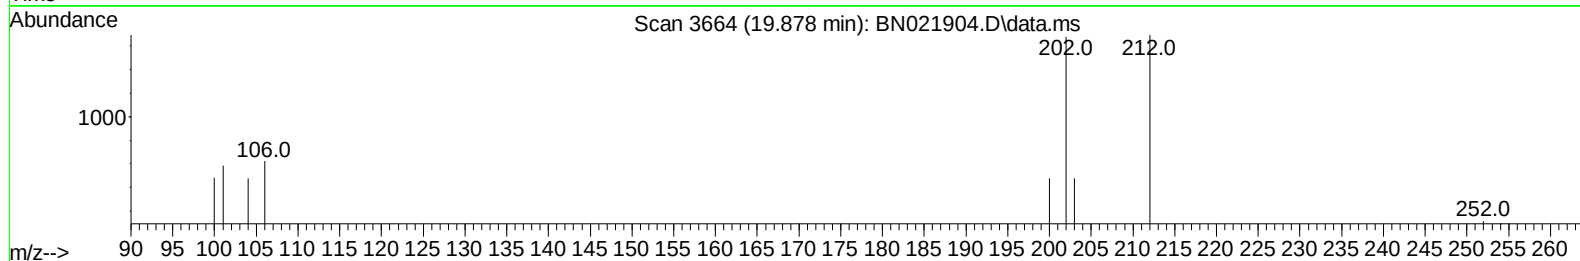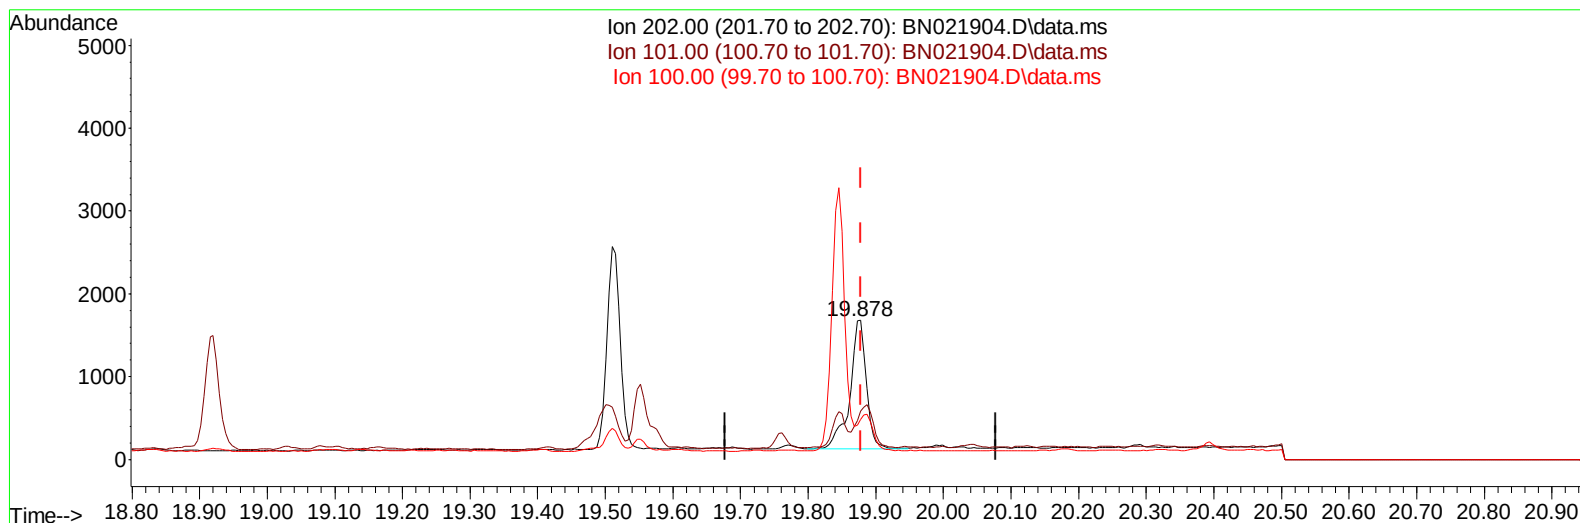

TIC: BN021904.D\data.ms

(20) Pyrene

19.878min (-0.000) 0.06 ng/u1

response 2629

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.10	34.72#
100.00	11.20	28.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021904.D
 Acq On : 23 Sep 2022 17:18
 Operator : CG/JU
 Sample : N4706-01DL 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8J8DL

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:02:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/26/2022
 Supervised By :mohammad ahmed 09/26/2022

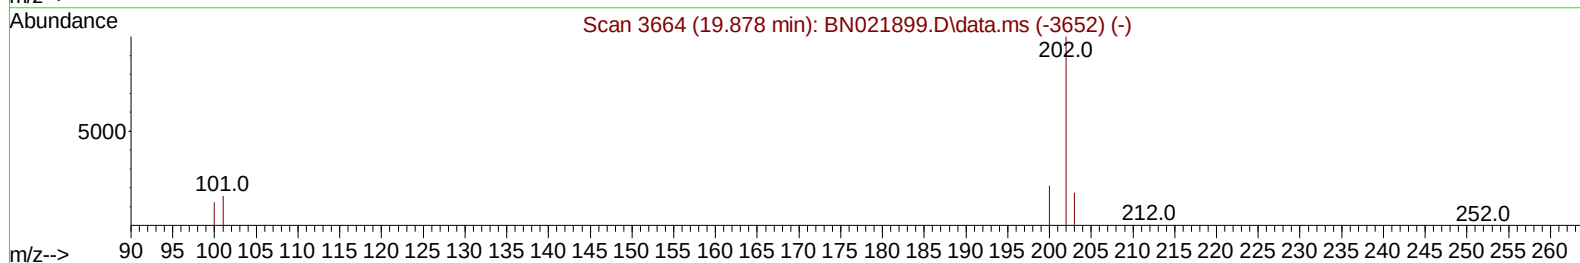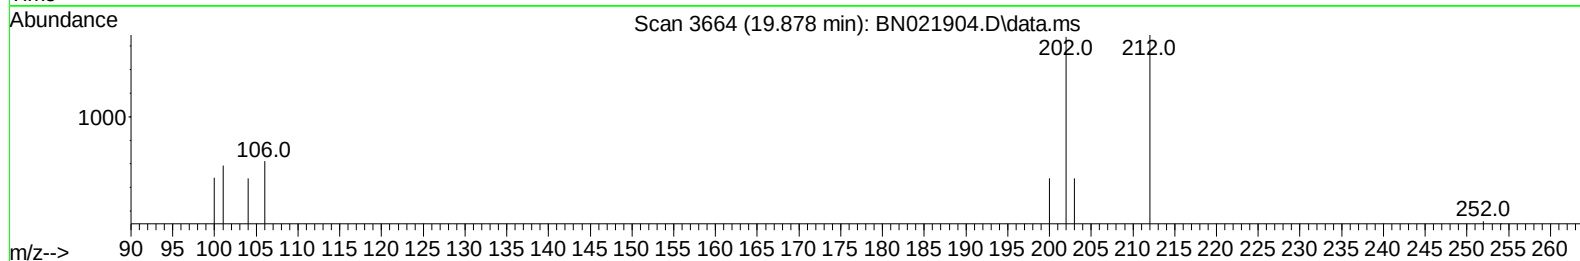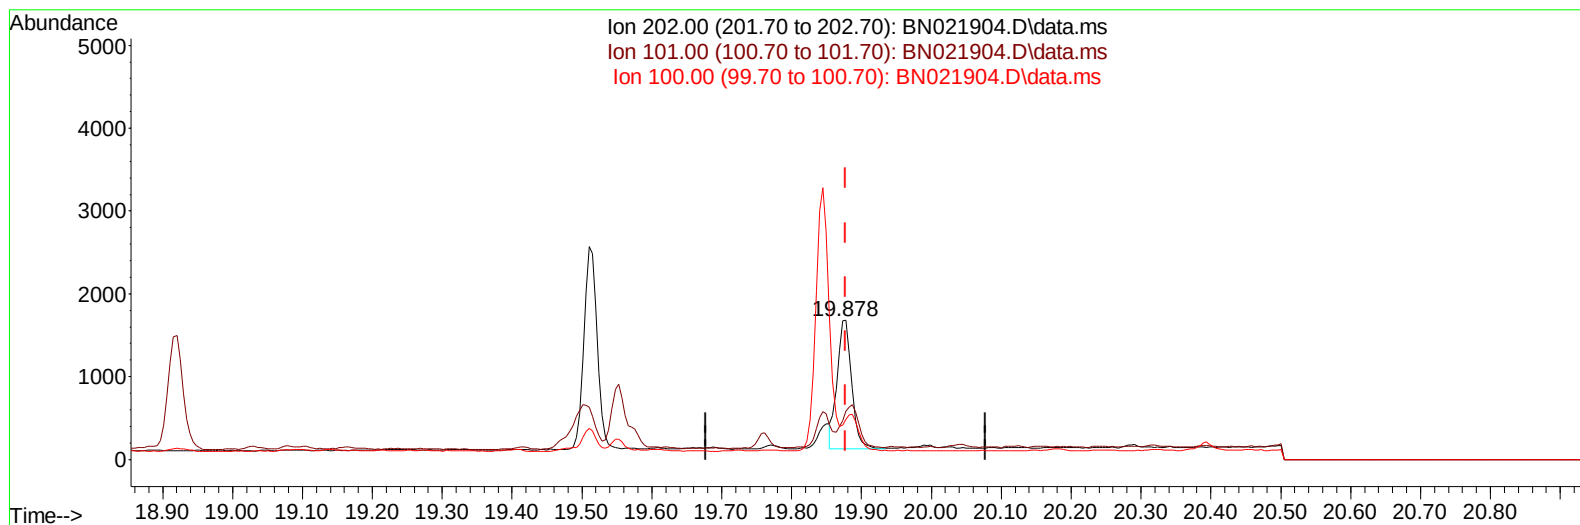

TIC: BN021904.D\data.ms

(20) Pyrene

19.878min (-0.000) 0.05 ng/ul m

response 2235

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.10	34.72#
100.00	11.20	28.71#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021904.D
 Acq On : 23 Sep 2022 17:18
 Operator : CG/JU
 Sample : N4706-01DL 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8J8DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/26/2022
 Supervised By :mohammad ahmed 09/26/2022

Quant Time: Sep 24 01:02:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.046	152		4304	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136		14371	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.703	164		8135	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188		15774	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240		9239	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264		7333	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.359	96		2197	0.415	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.461	152		1365	0.060	ng/ul	-0.01
18) Fluoranthene-d10	19.482	212		2712	0.079	ng/ul	0.00
Target Compounds				Qvalue			
5) Naphthalene	10.922	128		1390	0.034	ng/ul#	75
7) 2-Methylnaphthalene	12.533	142		2592	0.098	ng/ul	96
8) 1-Methylnaphthalene	12.753	142		5502	0.204	ng/ul	99
10) Acenaphthylene	14.425	152		804	0.024	ng/ul#	15
11) Acenaphthene	14.763	153		40183	1.388	ng/ul	98
12) Fluorene	15.748	166		21096	0.650	ng/ul	100
15) Phenanthrene	17.493	178		1473	0.030	ng/ul#	76
16) Anthracene	17.586	178		3976	0.096	ng/ul#	89
19) Fluoranthene	19.510	202		3301	0.077	ng/ul#	77
20) Pyrene	19.878	202		2235m	0.053	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021904.D
Acq On : 23 Sep 2022 17:18
Operator : CG/JU
Sample : N4706-01DL 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8J8DL

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:02:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/26/2022
Supervised By :mohammad ahmed 09/26/2022

