

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021847.D
 Acq On : 21 Sep 2022 18:42
 Operator : CG/JU
 Sample : N4649-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ39

Quant Time: Sep 22 00:46:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	5396	0.400	ng/u1	0.00
4) Naphthalene-d8	10.878	136	18110	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.708	164	10092	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.456	188	20438	0.400	ng/u1	# 0.00
17) Chrysene-d12	21.647	240	11670	0.400	ng/u1	# 0.00
23) Perylene-d12	24.152	264	9555	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	30214	4.551	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.467	152	8142	0.284	ng/u1	0.00
18) Fluoranthene-d10	19.483	212	17901	0.412	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	2815	0.413	ng/u1	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021847.D
Acq On : 21 Sep 2022 18:42
Operator : CG/JU
Sample : N4649-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ39

Quant Time: Sep 22 00:46:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

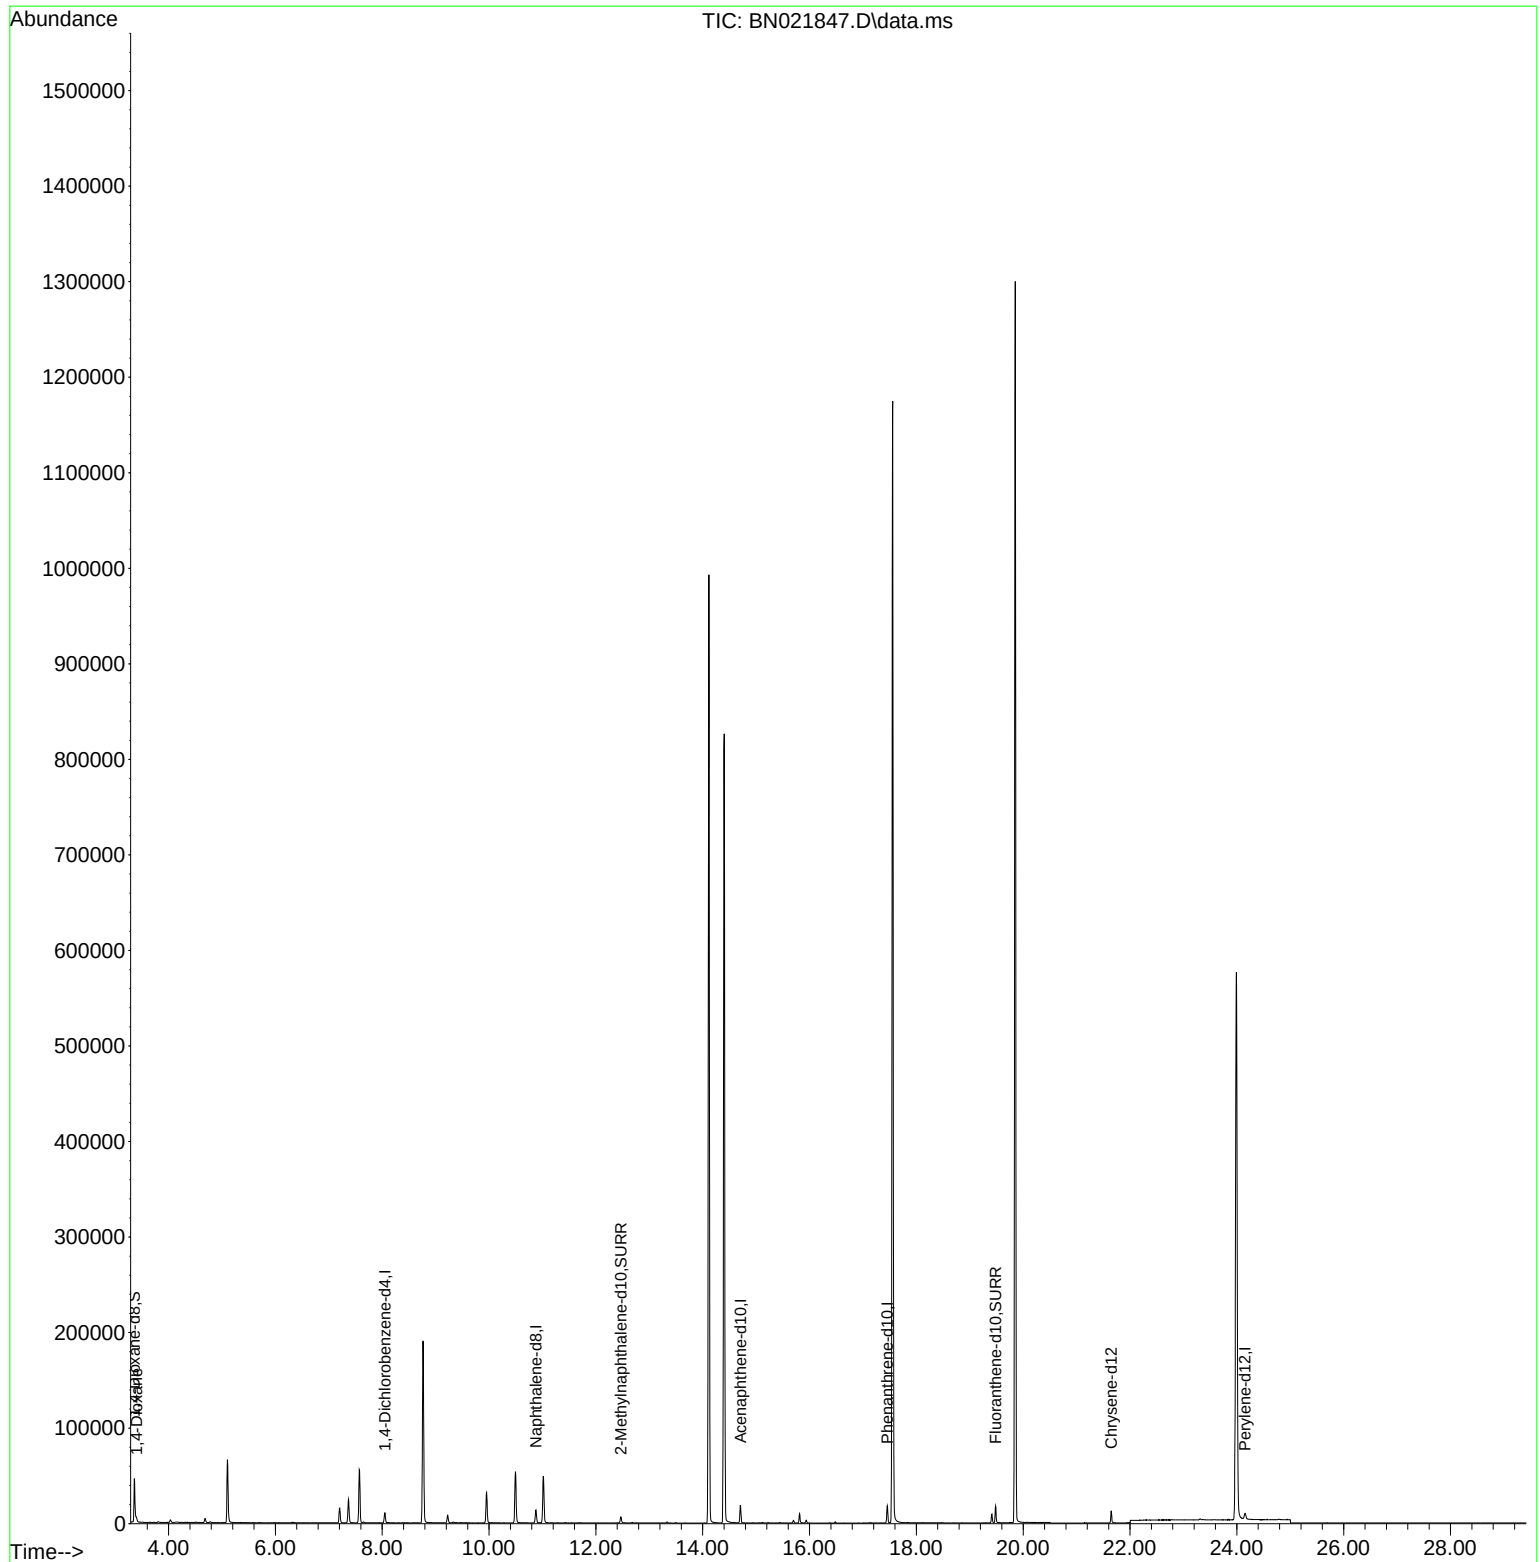

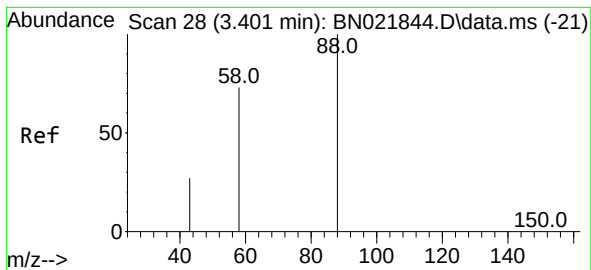

#2

1,4-Dioxane

Concen: 0.413 ng/ul

RT: 3.397 min Scan# 21

Delta R.T. -0.004 min

Lab File: BN021847.D


Acq: 21 Sep 2022 18:42

Instrument :

BNA_N

ClientSampleId :

EXZ39

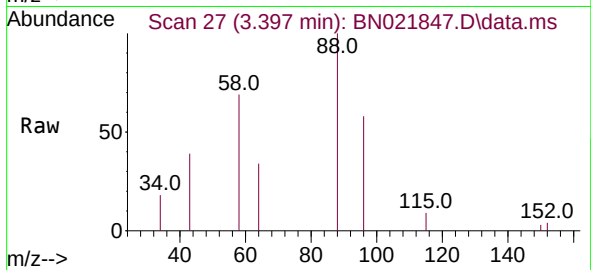

Tgt Ion: 88 Resp: 2815

Ion Ratio Lower Upper

88 100

43 38.7 31.4 47.0

58 69.1 49.0 73.6

