

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021849.D
 Acq On : 21 Sep 2022 19:57
 Operator : CG/JU
 Sample : N4649-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ40

Quant Time: Sep 22 00:46:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	6288	0.400	ng/u1	0.00
4) Naphthalene-d8	10.872	136	20891	0.400	ng/u1	#-0.01
9) Acenaphthene-d10	14.703	164	11840	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.456	188	23033	0.400	ng/u1	0.00
17) Chrysene-d12	21.647	240	13116	0.400	ng/u1	# 0.00
23) Perylene-d12	24.150	264	10659	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	28495	3.683	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.467	152	8364	0.253	ng/u1	0.00
18) Fluoranthene-d10	19.483	212	19190	0.393	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	7518	0.948	ng/u1	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021849.D
Acq On : 21 Sep 2022 19:57
Operator : CG/JU
Sample : N4649-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ40


Quant Time: Sep 22 00:46:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

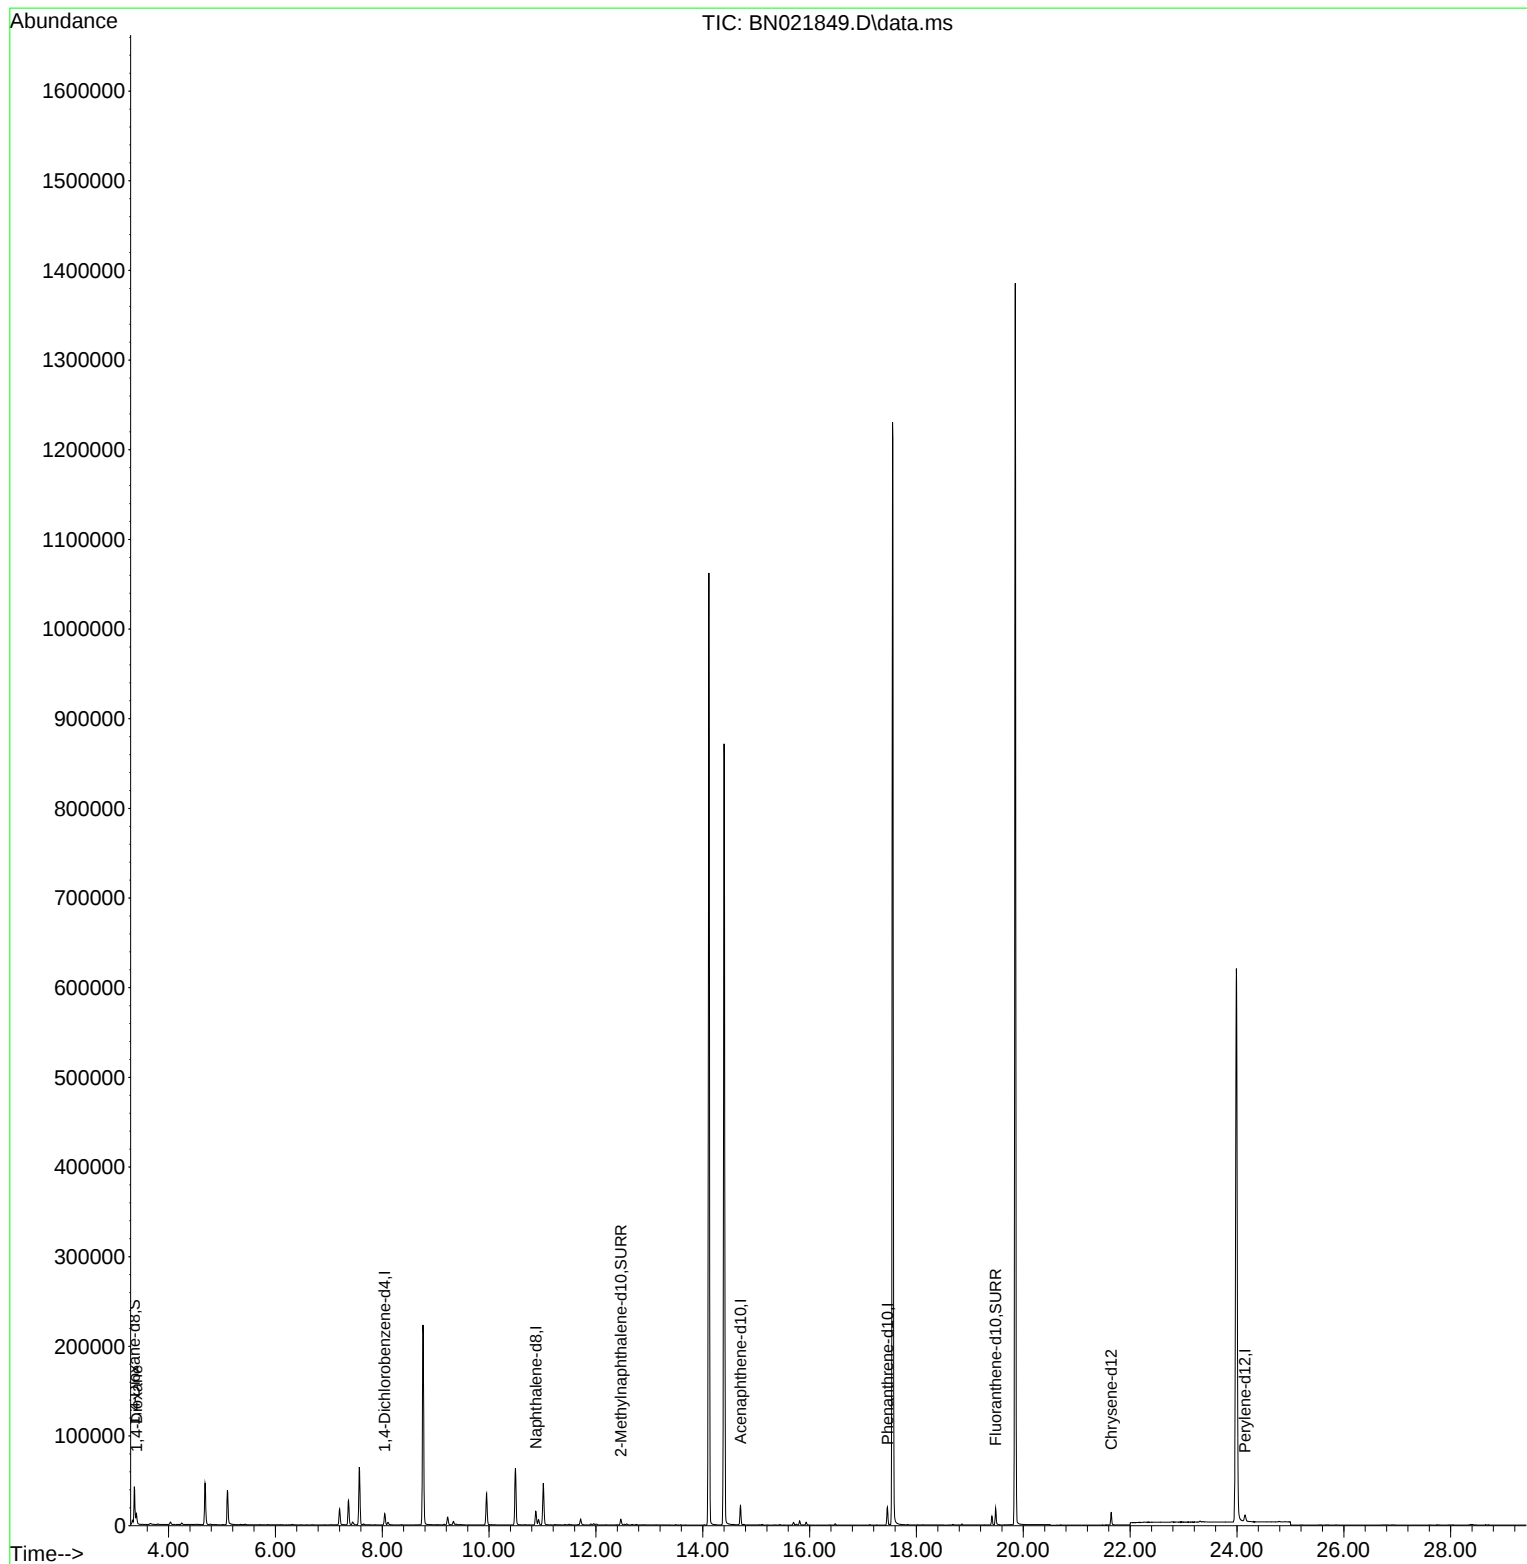

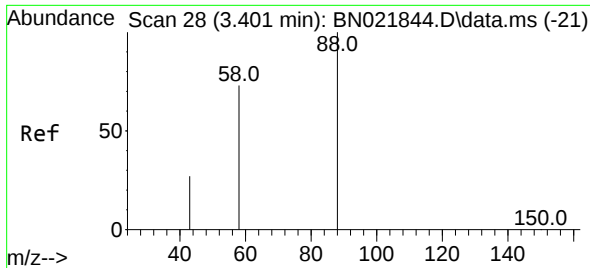

#2
 1,4-Dioxane
 Concen: 0.948 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021849.D
 Acq: 21 Sep 2022 19:57

Instrument :
 BNA_N
 ClientSampleId :
 EXZ40

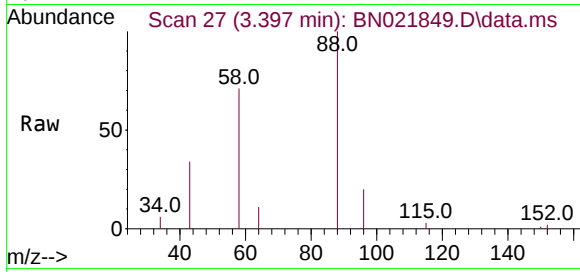

Tgt Ion:	88	Resp:	7518
Ion	Ratio	Lower	Upper
88	100		
43	33.9	31.4	47.0
58	70.8	49.0	73.6

