

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021850.D
 Acq On : 21 Sep 2022 20:35
 Operator : CG/JU
 Sample : N4649-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ21

Quant Time: Sep 22 00:46:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	5557	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	18559	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.703	164	10570	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.456	188	20240	0.400	ng/ul	0.00
17) Chrysene-d12	21.644	240	11183	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	9613	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	27719	4.055	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	9293	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	16365	0.393	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.401	88	1056	0.151	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021850.D
Acq On : 21 Sep 2022 20:35
Operator : CG/JU
Sample : N4649-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ21

Quant Time: Sep 22 00:46:54 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

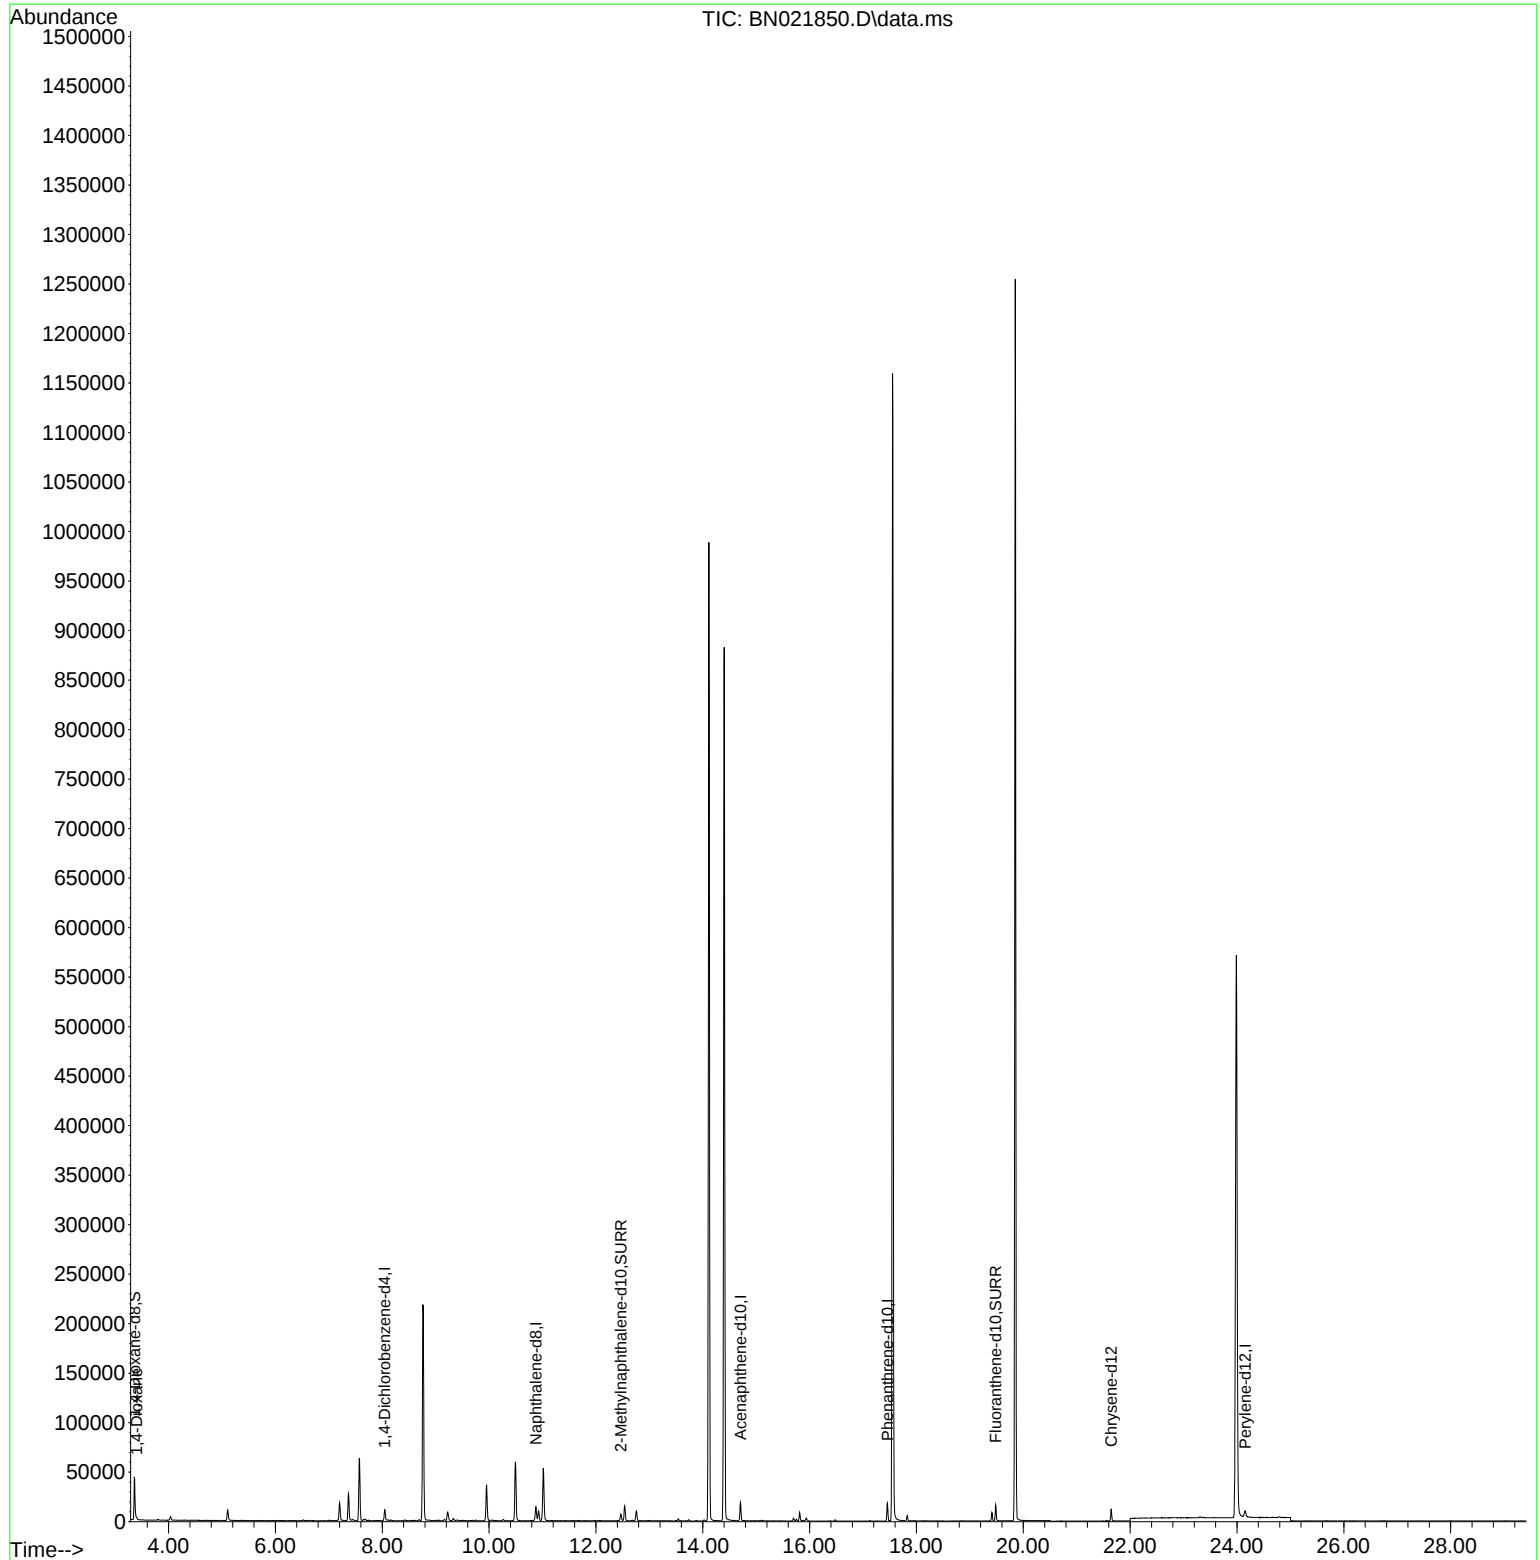

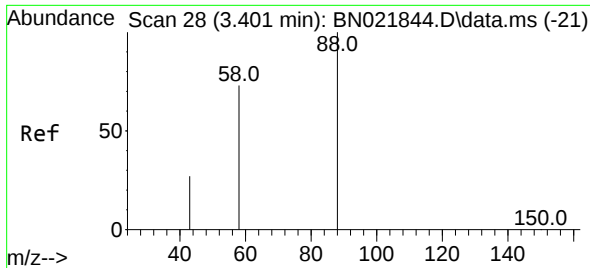

#2
 1,4-Dioxane
 Concen: 0.151 ng/ul
 RT: 3.401 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN021850.D
 Acq: 21 Sep 2022 20:35

Instrument :
 BNA_N
 ClientSampleId :
 EXZ21

Tgt Ion: 88	Resp: 1056
Ion Ratio	Lower Upper
88	100
43	47.2 31.4 47.0#
58	48.3 49.0 73.6#

