

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021855.D
 Acq On : 21 Sep 2022 23:42
 Operator : CG/JU
 Sample : N4649-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ23

Quant Time: Sep 22 00:47:42 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	5822	0.400	ng/u1	0.00
4) Naphthalene-d8	10.878	136	19320	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.703	164	10874	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.456	188	20837	0.400	ng/u1	0.00
17) Chrysene-d12	21.644	240	11623	0.400	ng/u1	# 0.00
23) Perylene-d12	24.147	264	9938	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	29324	4.094	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.467	152	9483	0.310	ng/u1	0.00
18) Fluoranthene-d10	19.483	212	17078	0.395	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	6559	0.893	ng/u1	90




(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\  
Data File : BN021855.D  
Acq On    : 21 Sep 2022   23:42  
Operator  : CG/JU  
Sample    : N4649-19  
Misc      :  
ALS Vial  : 13      Sample Multiplier: 1
```

Quant Time: Sep 22 00:47:42 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

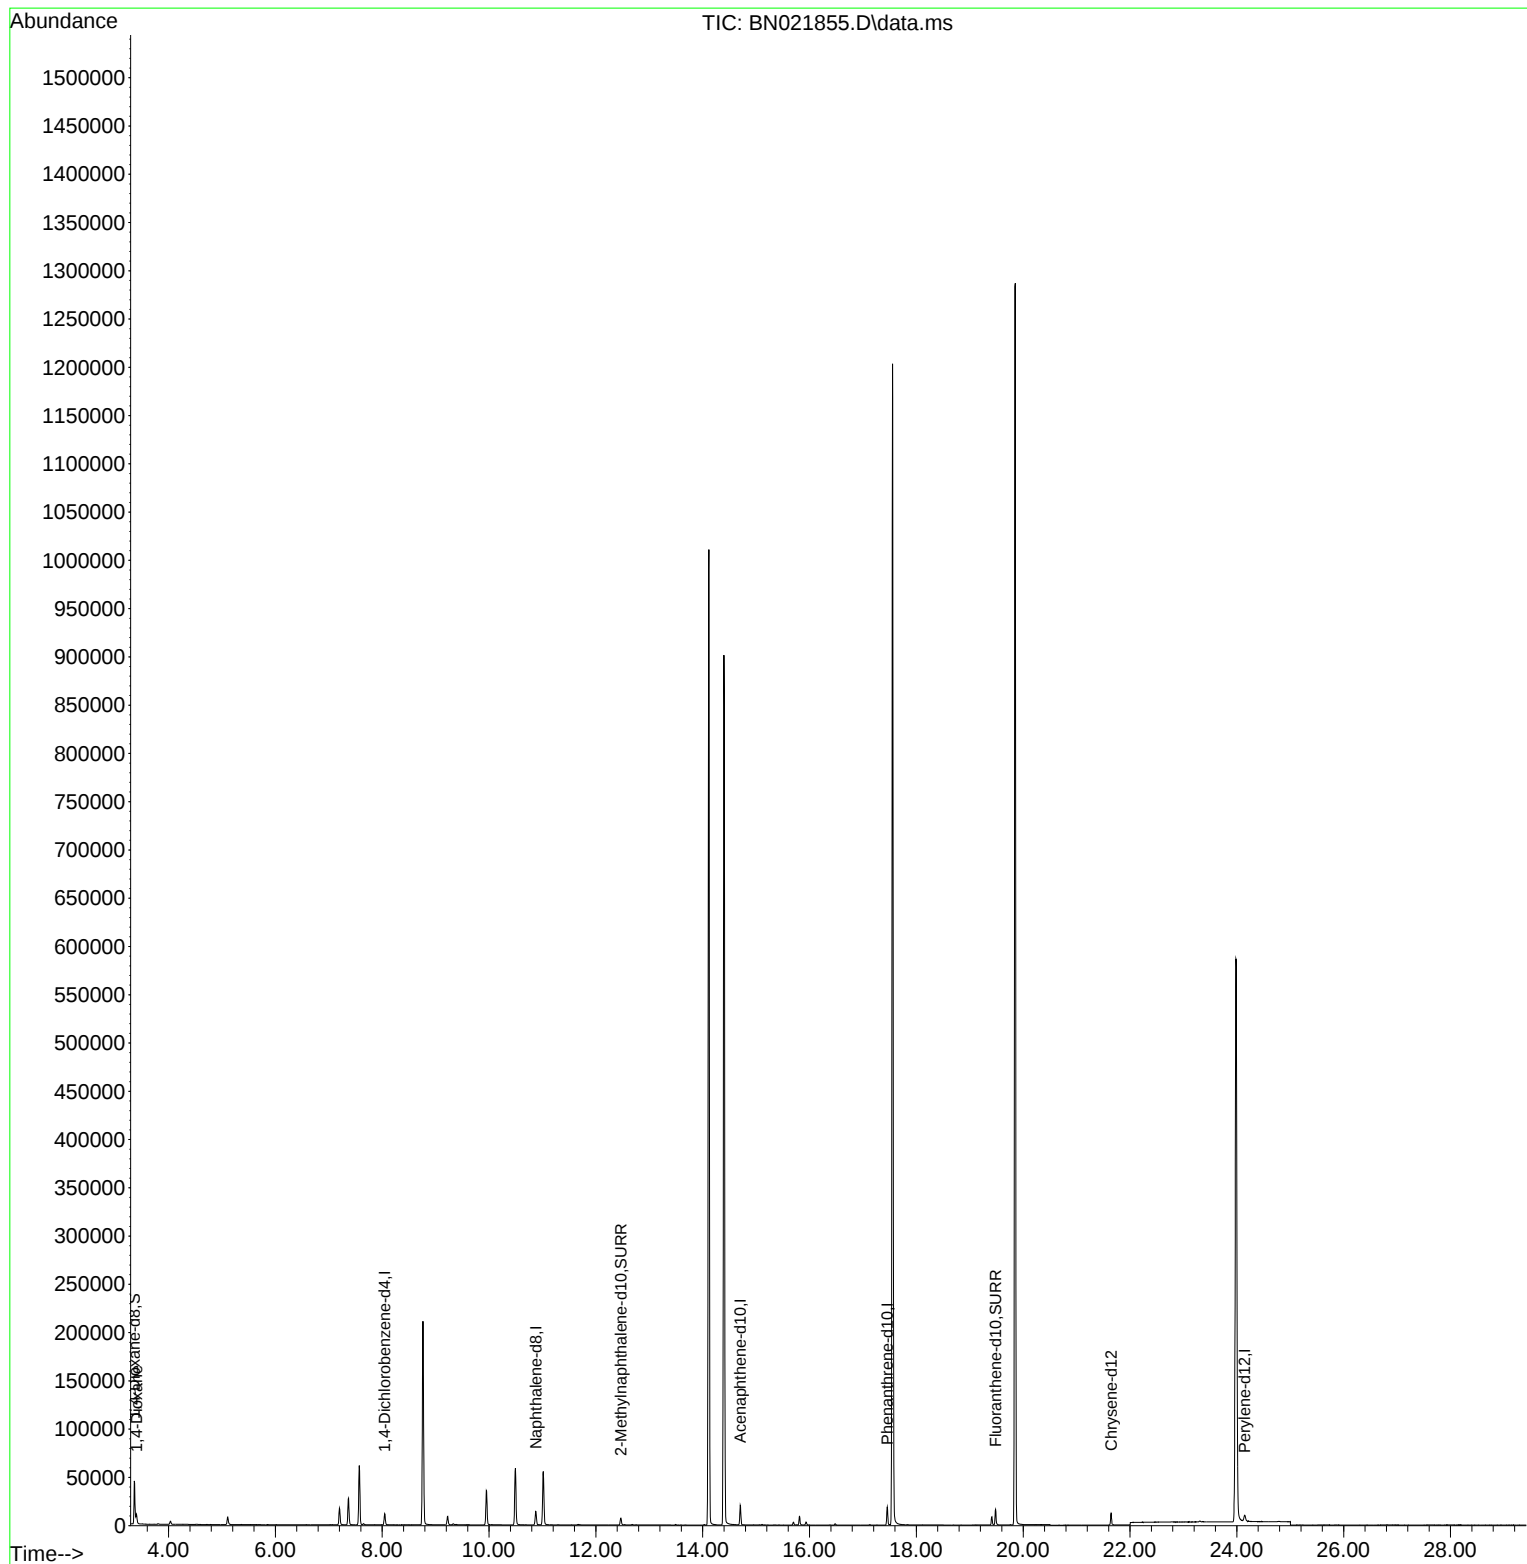

Abundance Scan 28 (3.401 min): BN021844.D\data.ms (-21)

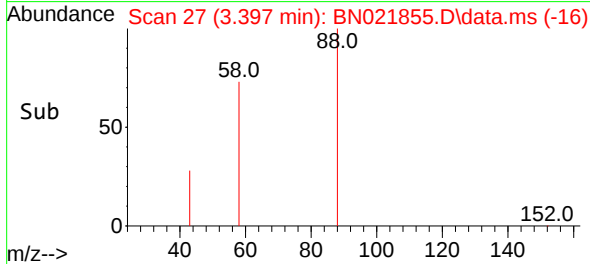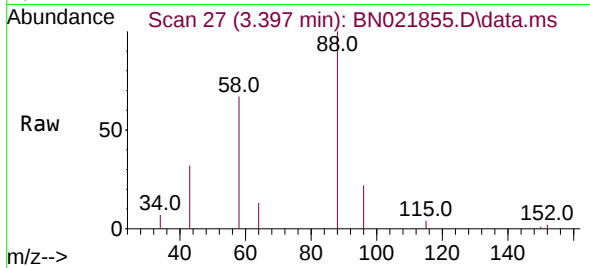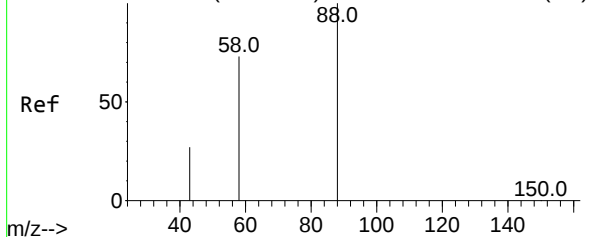

#2
1,4-Dioxane
Concen: 0.893 ng/ul
RT: 3.397 min Scan# 21
Delta R.T. -0.004 min
Lab File: BN021855.D
Acq: 21 Sep 2022 23:42

Instrument :
BNA_N
ClientSampleId :
EXZ23

Tgt Ion: 88	Resp: 6559
Ion Ratio	Lower Upper
88	100
43	31.7 31.4 47.0
58	67.3 49.0 73.6

