

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021857.D
 Acq On : 22 Sep 2022 00:56
 Operator : CG/JU
 Sample : N4649-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ41

Quant Time: Sep 22 01:42:22 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	5173	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	17395	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.703	164	10958	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.455	188	21052	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	12723	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	10133	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	44291	6.959	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.462	152	8083	0.294	ng/ul	-0.01
18) Fluoranthene-d10	19.483	212	18224	0.385	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	91293	13.986	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021857.D
Acq On : 22 Sep 2022 00:56
Operator : CG/JU
Sample : N4649-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ41


Quant Time: Sep 22 01:42:22 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

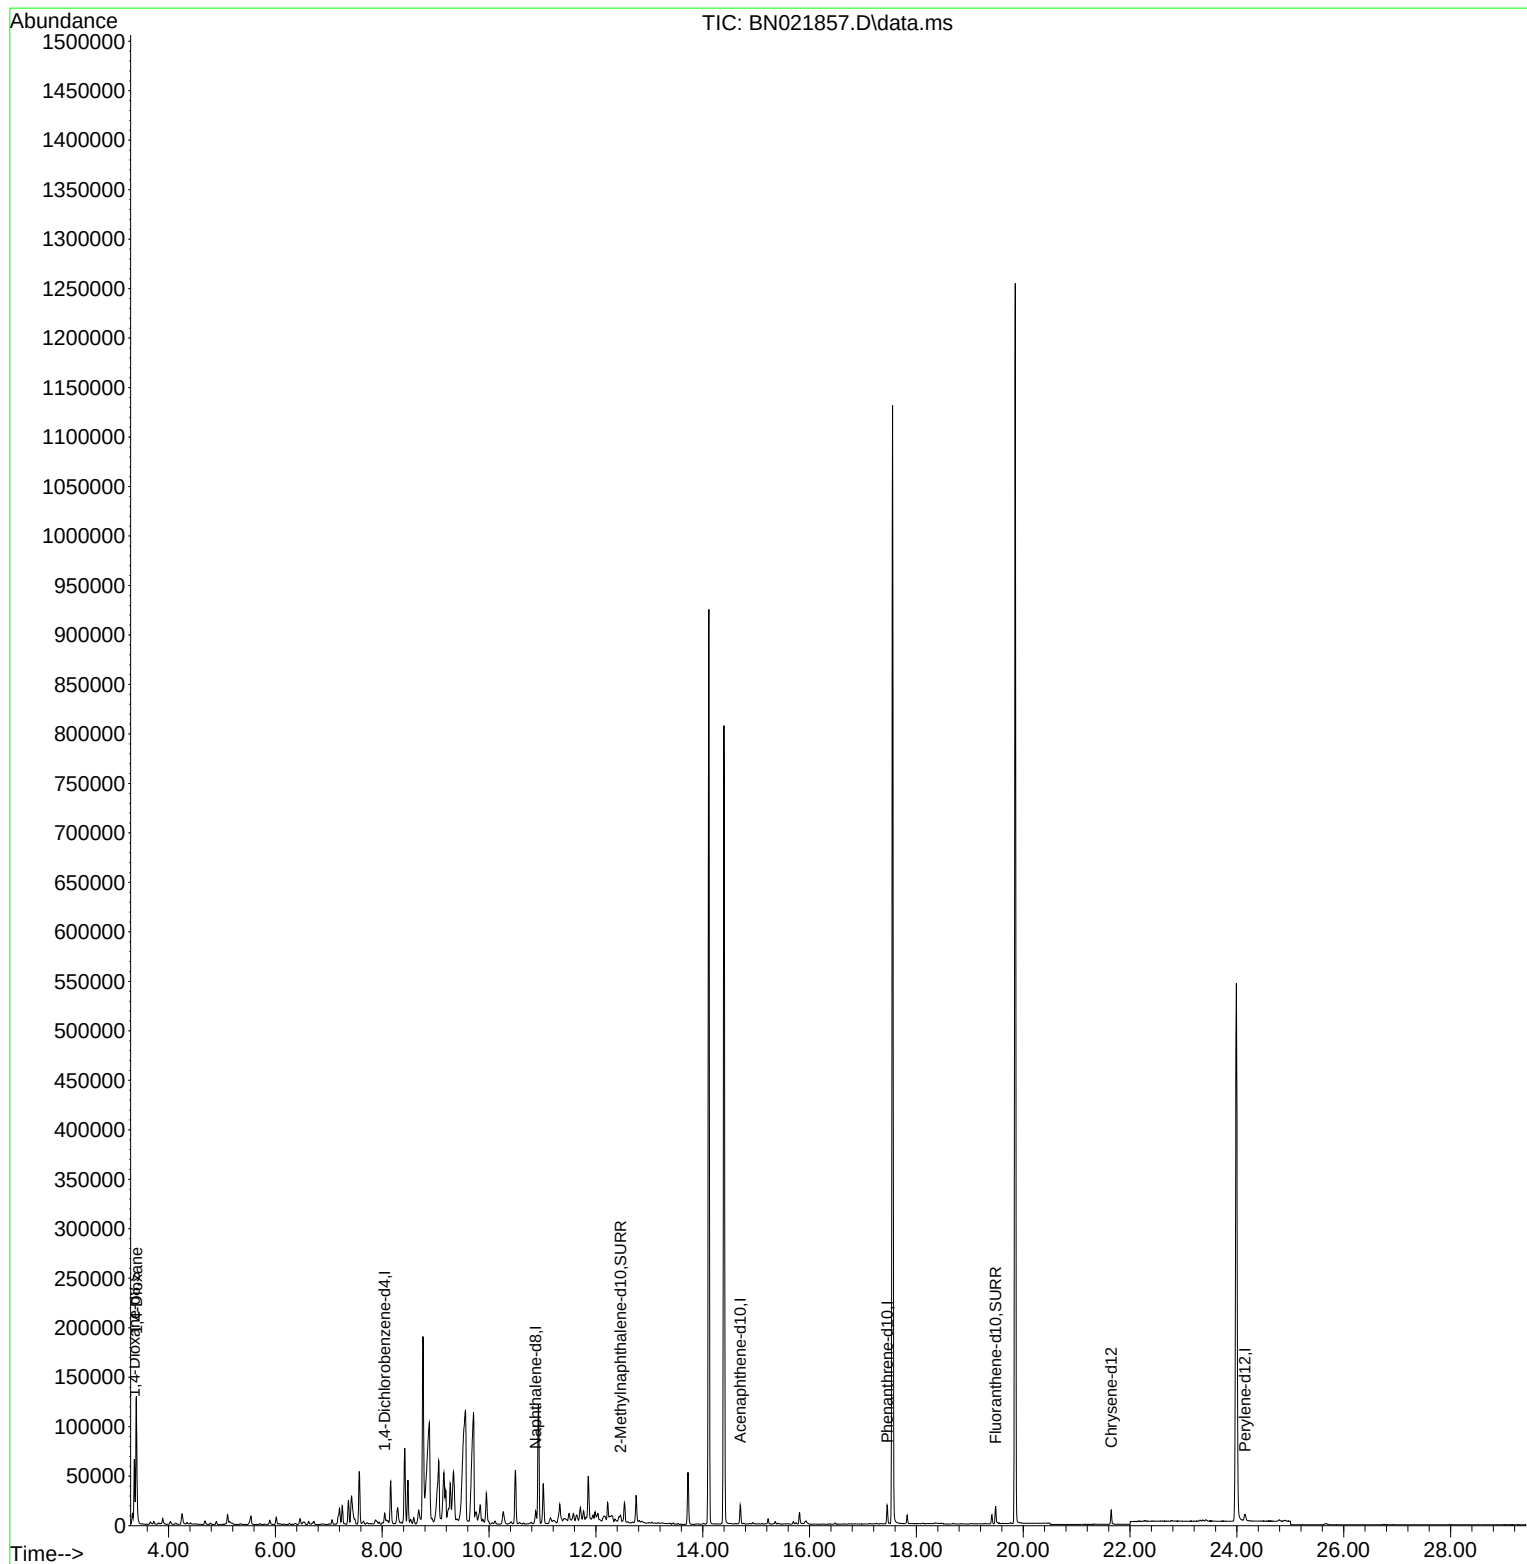

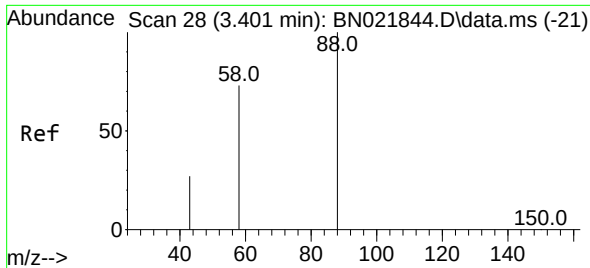

#2
 1,4-Dioxane
 Concen: 13.986 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021857.D
 Acq: 22 Sep 2022 00:56

Instrument :
 BNA_N
 ClientSampleId :
 EXZ41

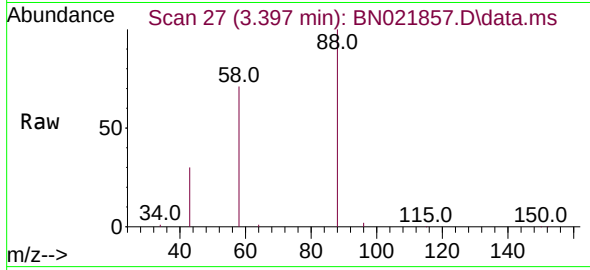

Tgt Ion: 88 Resp: 91293
 Ion Ratio Lower Upper
 88 100
 43 30.2 31.4 47.0#
 58 70.6 49.0 73.6

