

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021858.D
 Acq On : 22 Sep 2022 01:33
 Operator : CG/JU
 Sample : N4649-22
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ43

Quant Time: Sep 22 03:27:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	5382	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	18050	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.703	164	10348	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.455	188	21205	0.400	ng/ul	0.00
17) Chrysene-d12	21.644	240	12670	0.400	ng/ul	# 0.00
23) Perylene-d12	24.149	264	10223	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	27231	4.113	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.461	152	8748	0.306	ng/ul	-0.01
18) Fluoranthene-d10	19.483	212	19462	0.413	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	79112	11.649	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021858.D
Acq On : 22 Sep 2022 01:33
Operator : CG/JU
Sample : N4649-22
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ43


Quant Time: Sep 22 03:27:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

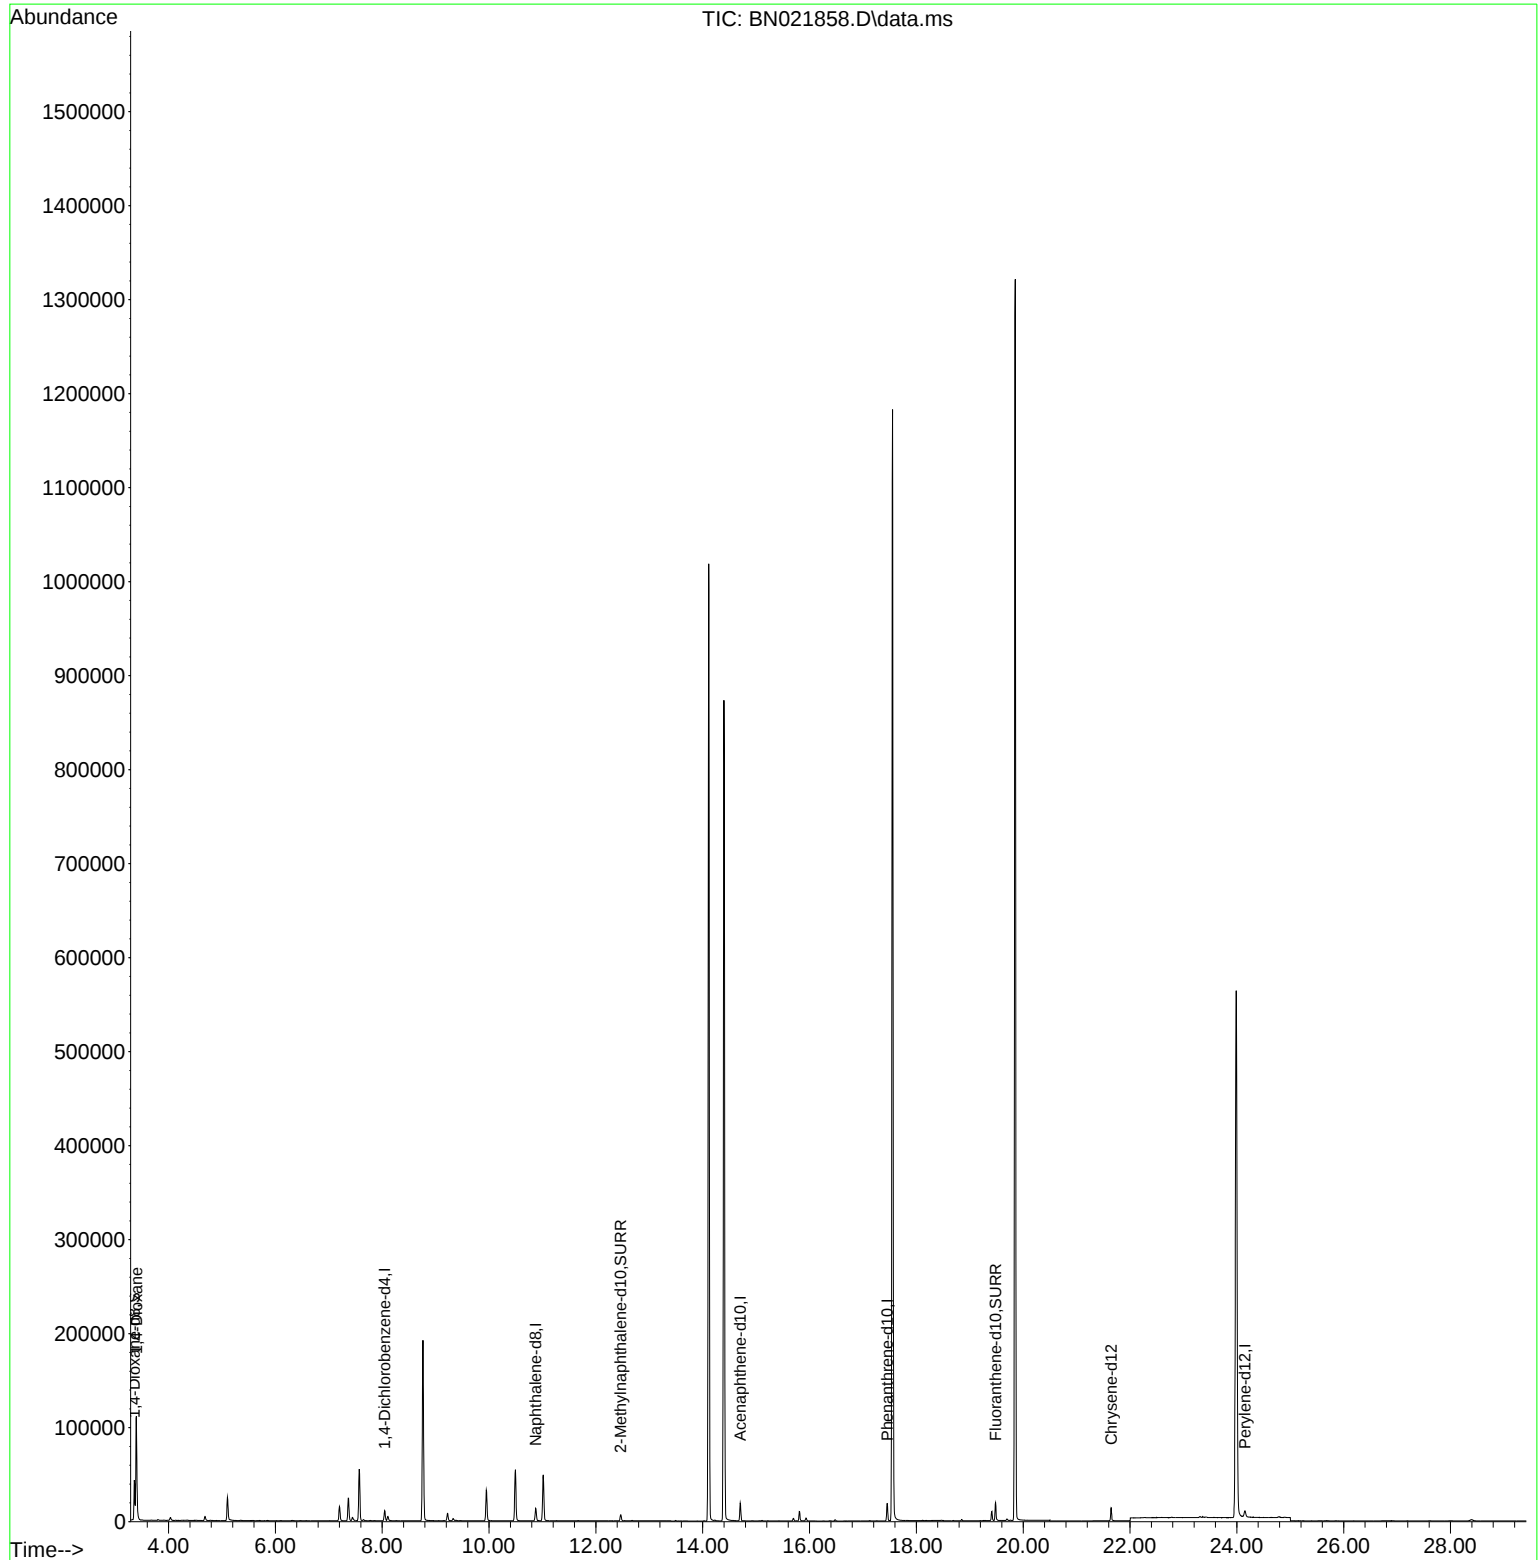

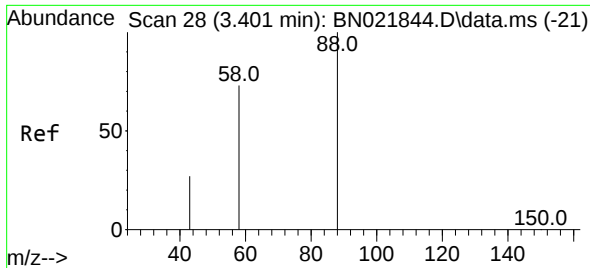

#2
 1,4-Dioxane
 Concen: 11.649 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021858.D
 Acq: 22 Sep 2022 01:33

Instrument :
 BNA_N
 ClientSampleId :
 EXZ43

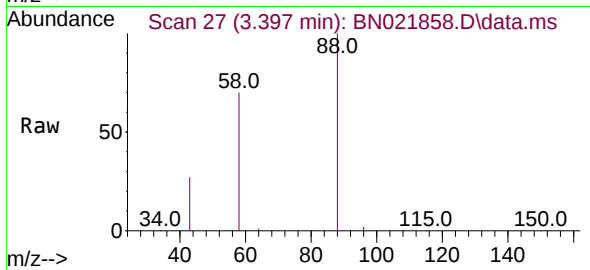

Tgt Ion: 88 Resp: 79112
 Ion Ratio Lower Upper
 88 100
 43 26.6 31.4 47.0#
 58 70.0 49.0 73.6

