

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021874.D
 Acq On : 22 Sep 2022 21:12
 Operator : CG/JU
 Sample : N4707-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8J9

Quant Time: Sep 23 02:12:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.050	152	4755	0.400	ng/ul	0.00
4) Naphthalene-d8	10.877	136	15984	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.707	164	9840	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.455	188	17949	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.650	240	10839	0.400	ng/ul	# 0.00
23) Perylene-d12	24.158	264	8848	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	26987	4.613	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	8027	0.317	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	17414	0.432	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	207511	34.584	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021874.D
Acq On : 22 Sep 2022 21:12
Operator : CG/JU
Sample : N4707-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8J9


Quant Time: Sep 23 02:12:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

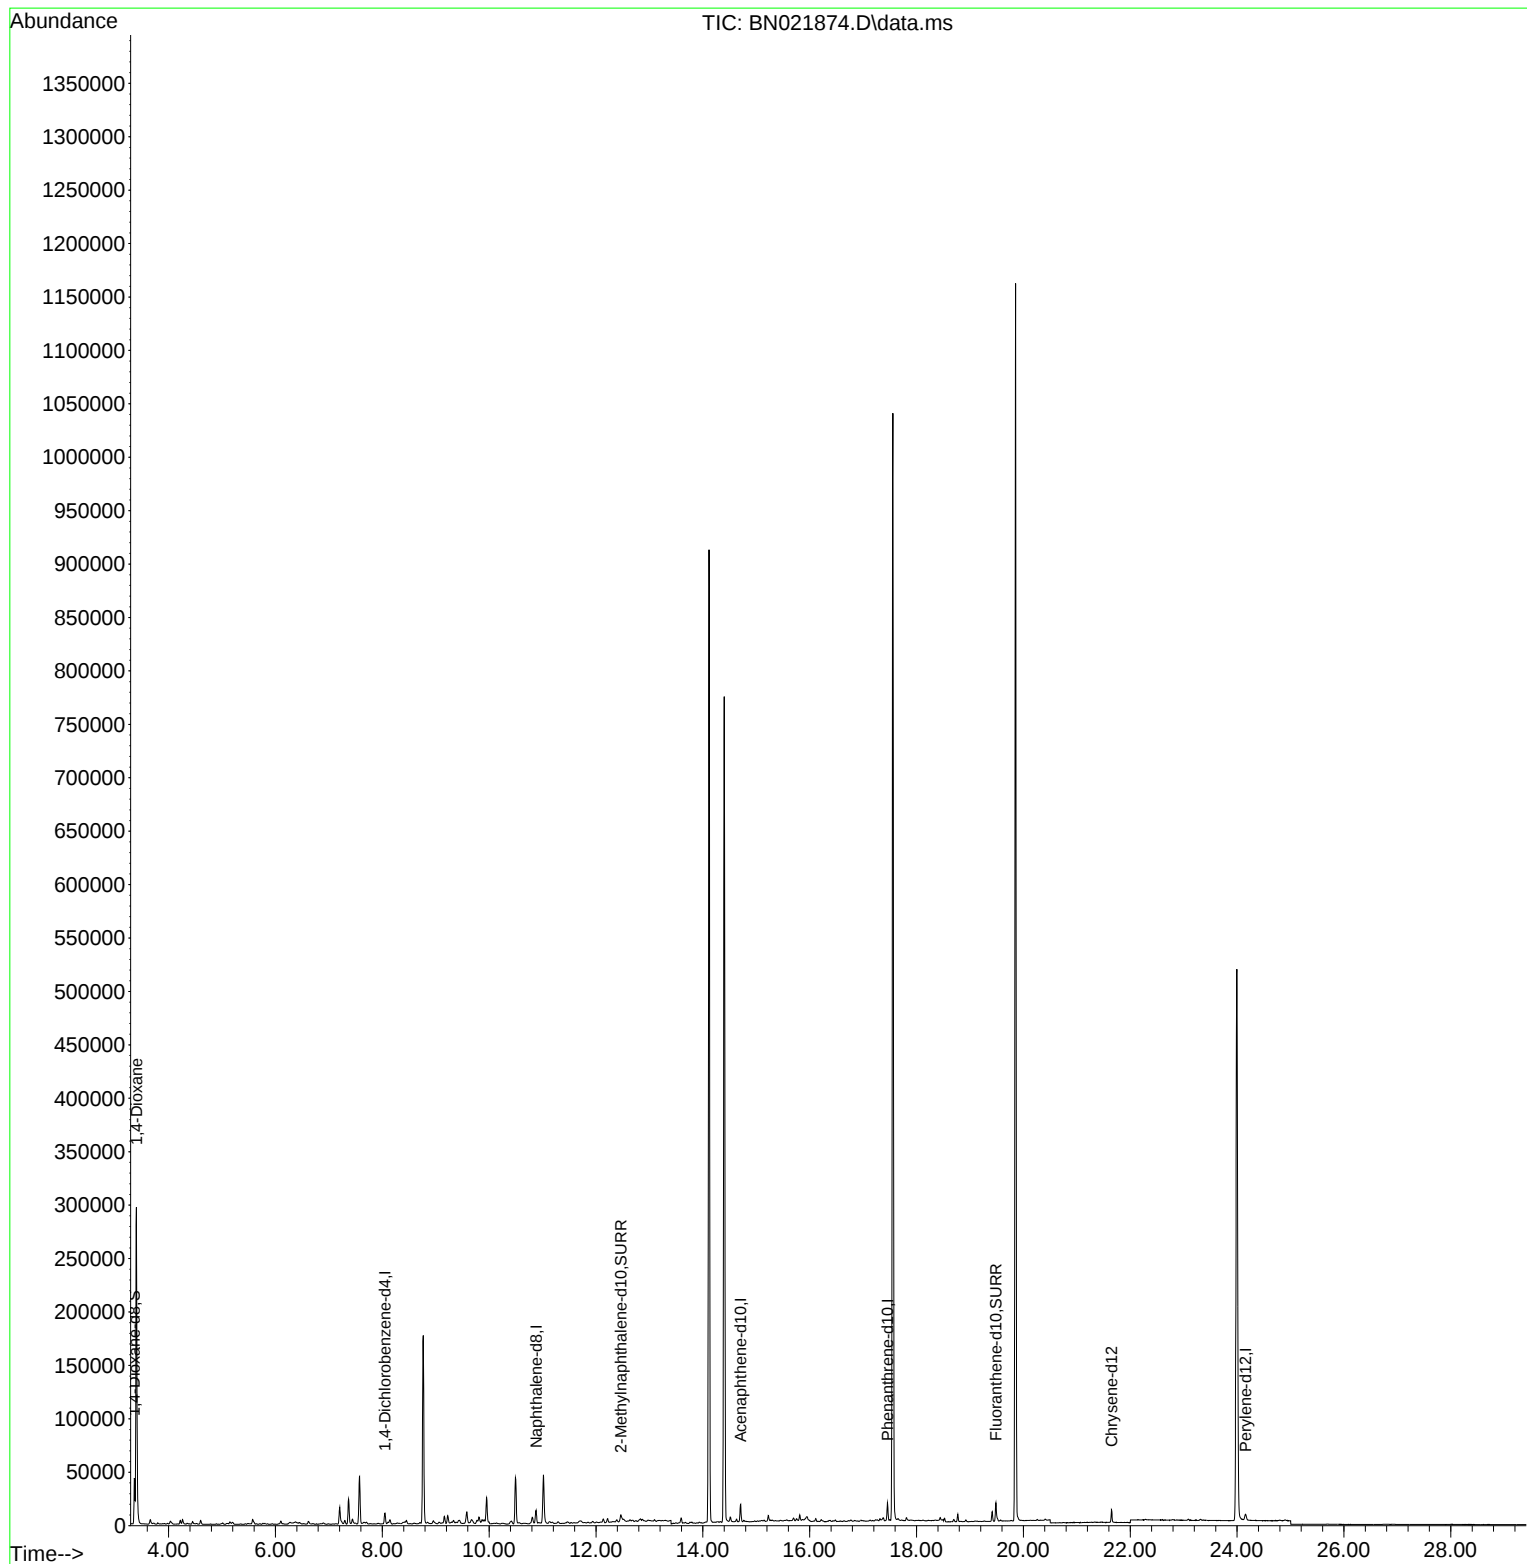

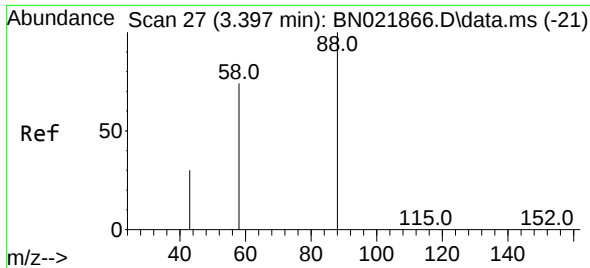

#2
 1,4-Dioxane
 Concen: 34.584 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BN021874.D
 Acq: 22 Sep 2022 21:12

Instrument :
 BNA_N
 ClientSampleId :
 CB8J9

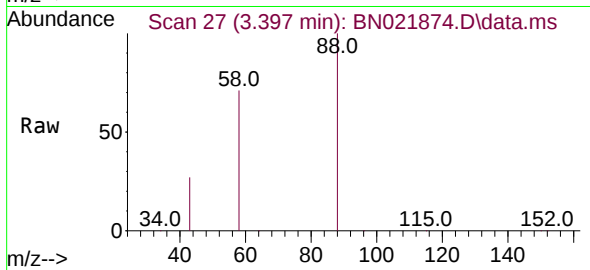

Tgt Ion: 88 Resp: 207511
 Ion Ratio Lower Upper
 88 100
 43 26.9 31.4 47.0#
 58 70.5 49.0 73.6

