

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021877.D
 Acq On : 22 Sep 2022 23:07
 Operator : CG/JU
 Sample : N4706-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8K8

Quant Time: Sep 23 02:12:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	5139	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	17081	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.707	164	9927	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.456	188	19615	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	11761	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	9543	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	24650	3.899	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	7901	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	16229	0.371	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Acenaphthene	14.768	153	1044	0.030	ng/ul	92
15) Phenanthrene	17.498	178	1428	0.023	ng/ul#	47
16) Anthracene	17.591	178	3607	0.070	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021877.D
Acq On : 22 Sep 2022 23:07
Operator : CG/JU
Sample : N4706-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8K8

Quant Time: Sep 23 02:12:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




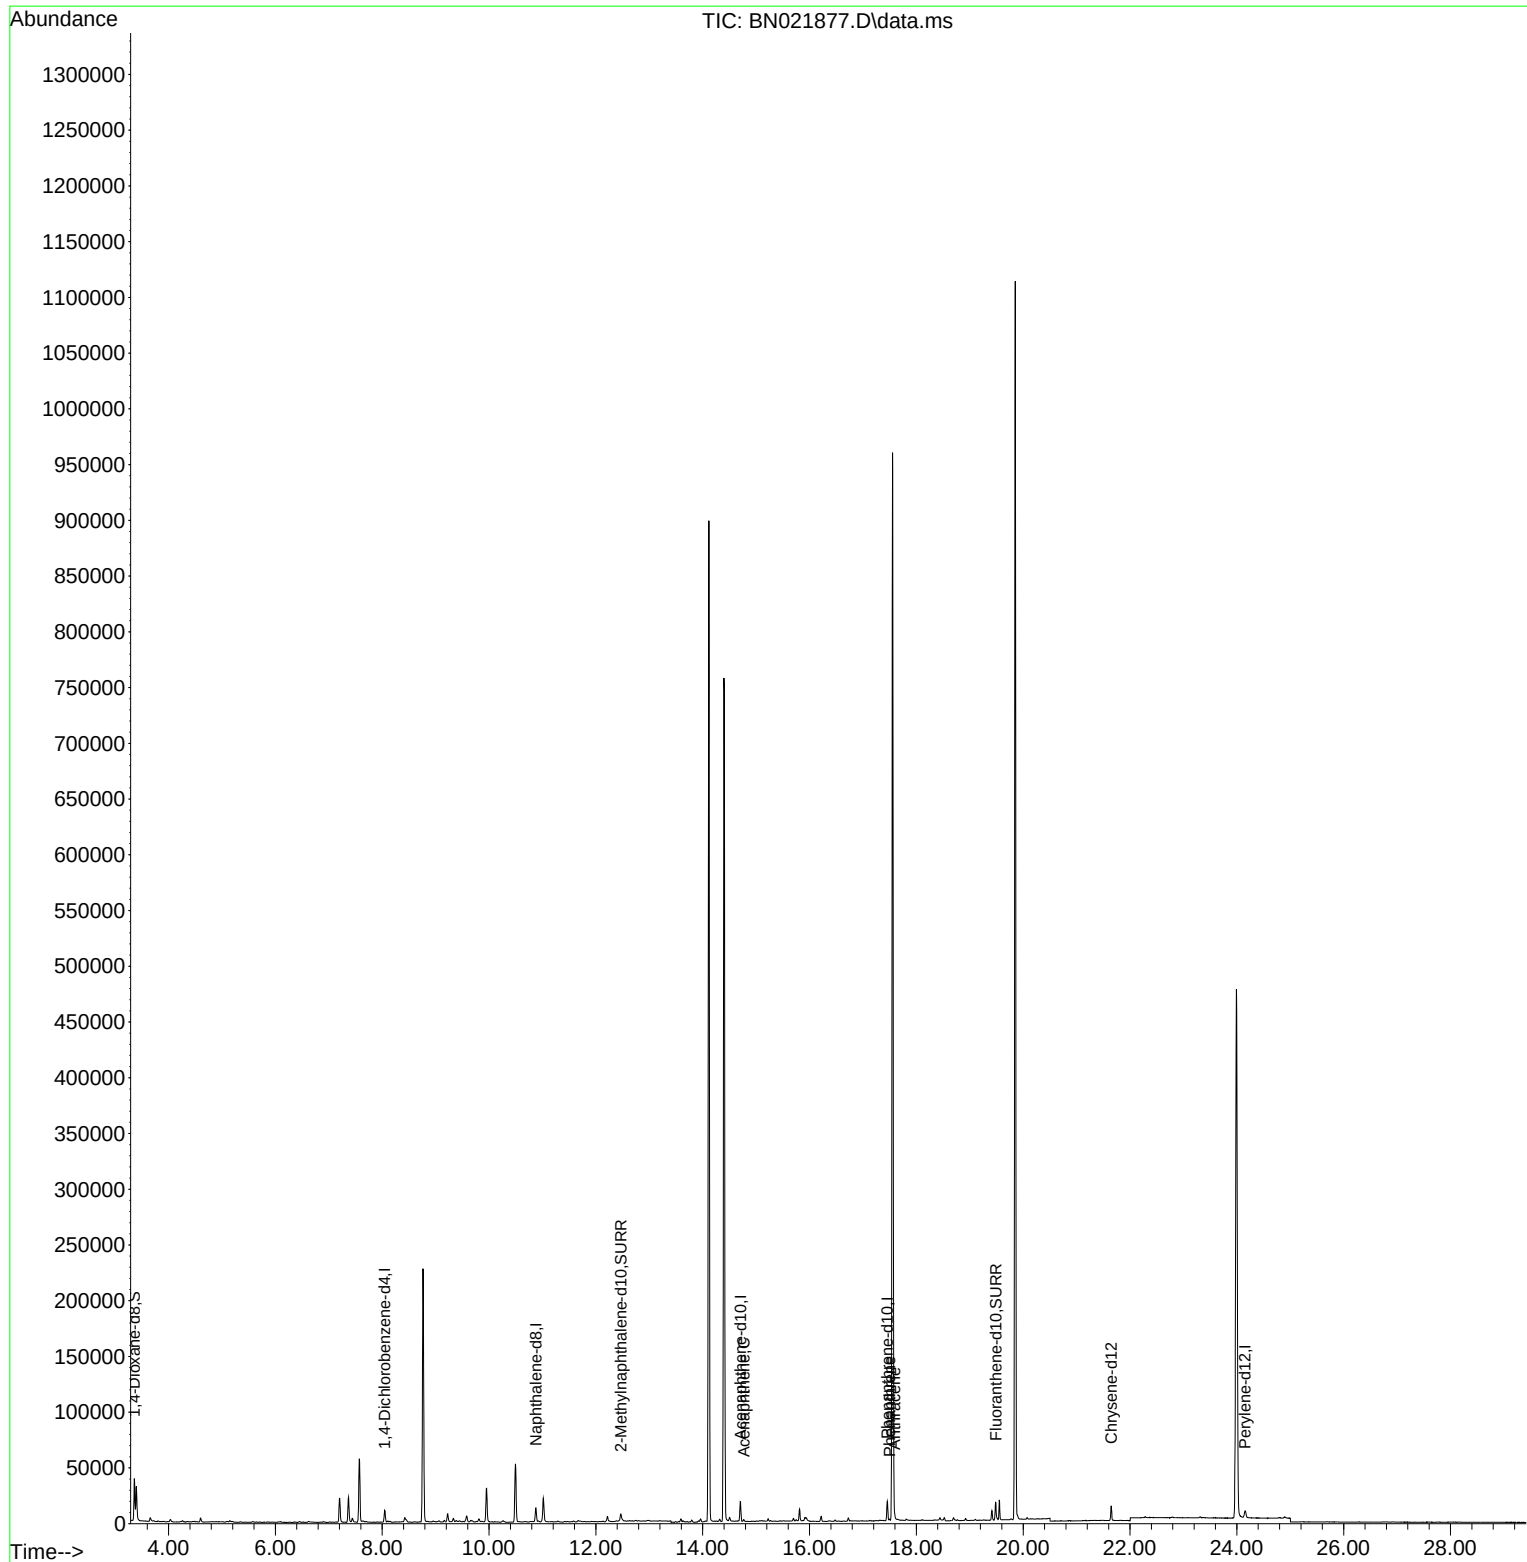


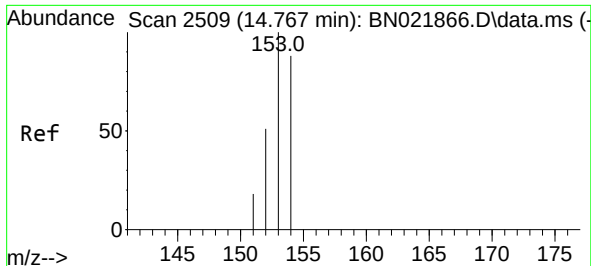

#11
Acenaphthene
Concen: 0.030 ng/ul
RT: 14.768 min Scan# 2100
Delta R.T. -0.005 min
Lab File: BN021877.D
Acq: 22 Sep 2022 23:07




Instrument :
BNA_N
ClientSampleId :
CB8K8


Tgt Ion:153 Resp: 1044
Ion Ratio Lower Upper
153 100
152 55.4 40.2 60.4
154 80.9 70.7 106.1

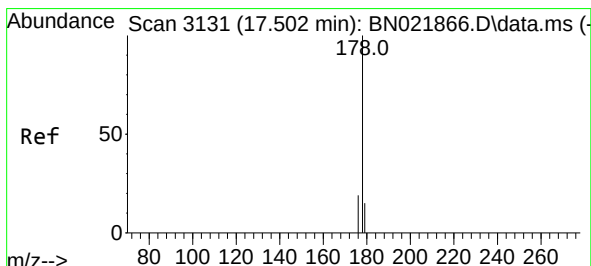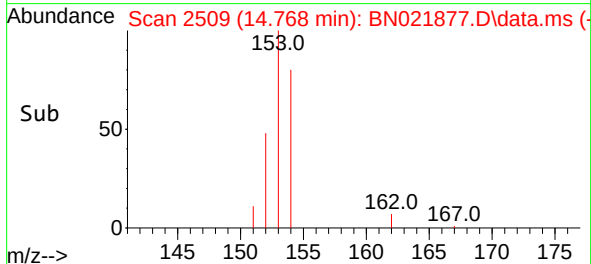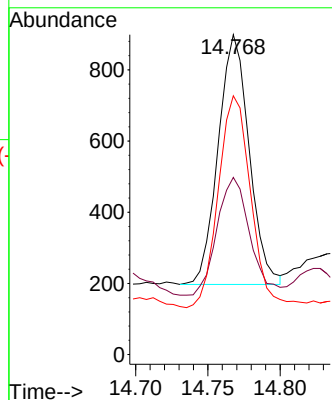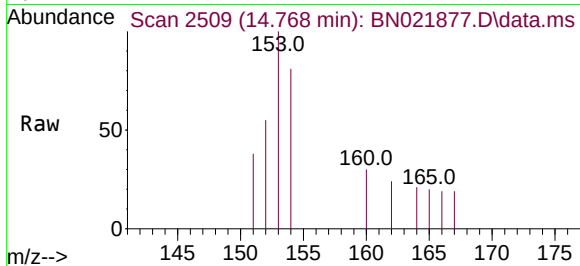

#15
Phenanthrene
Concen: 0.023 ng/ul
RT: 17.498 min Scan# 3130
Delta R.T. -0.004 min
Lab File: BN021877.D
Acq: 22 Sep 2022 23:07


Tgt Ion:178 Resp: 1428
Ion Ratio Lower Upper
178 100
179 42.7 12.8 19.2#
176 40.5 15.9 23.9#

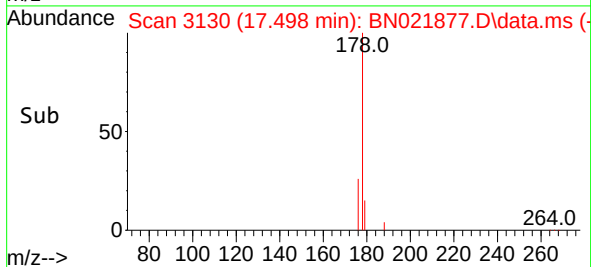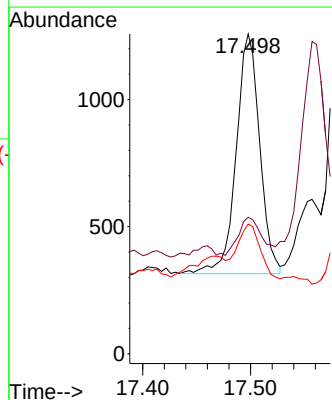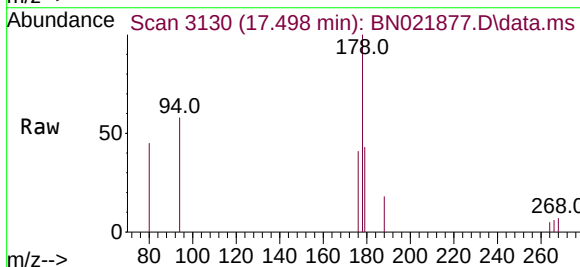

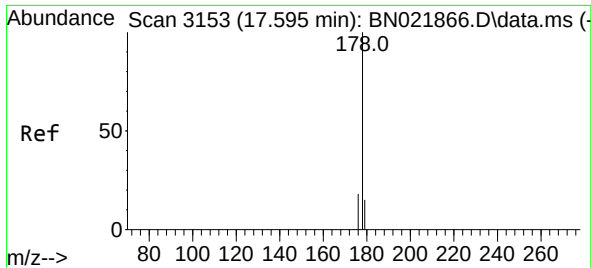

#16
 Anthracene
 Concen: 0.070 ng/ul
 RT: 17.591 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN021877.D
 Acq: 22 Sep 2022 23:07

Instrument :
 BNA_N
 ClientSampleId :
 CB8K8

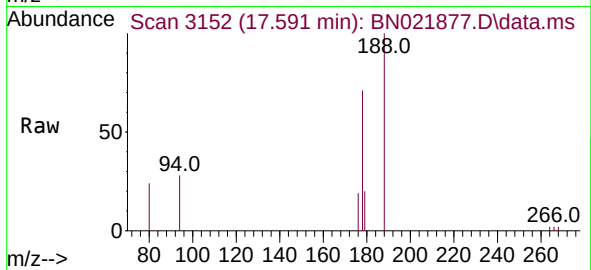

Tgt Ion:178 Resp: 3607
 Ion Ratio Lower Upper
 178 100
 179 27.9 12.9 19.3#
 176 26.6 15.9 23.9#

