

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021880.D
 Acq On : 23 Sep 2022 01:02
 Operator : CG/JU
 Sample : N4707-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8L0

Quant Time: Sep 23 02:13:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	5578	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	18223	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.703	164	11279	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.455	188	20631	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	12506	0.400	ng/ul	# 0.00
23) Perylene-d12	24.155	264	10194	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	26137	3.809	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.461	152	6525	0.226	ng/ul	-0.01
18) Fluoranthene-d10	19.483	212	13347	0.287	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	45407	6.451	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021880.D
Acq On : 23 Sep 2022 01:02
Operator : CG/JU
Sample : N4707-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8L0

Quant Time: Sep 23 02:13:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

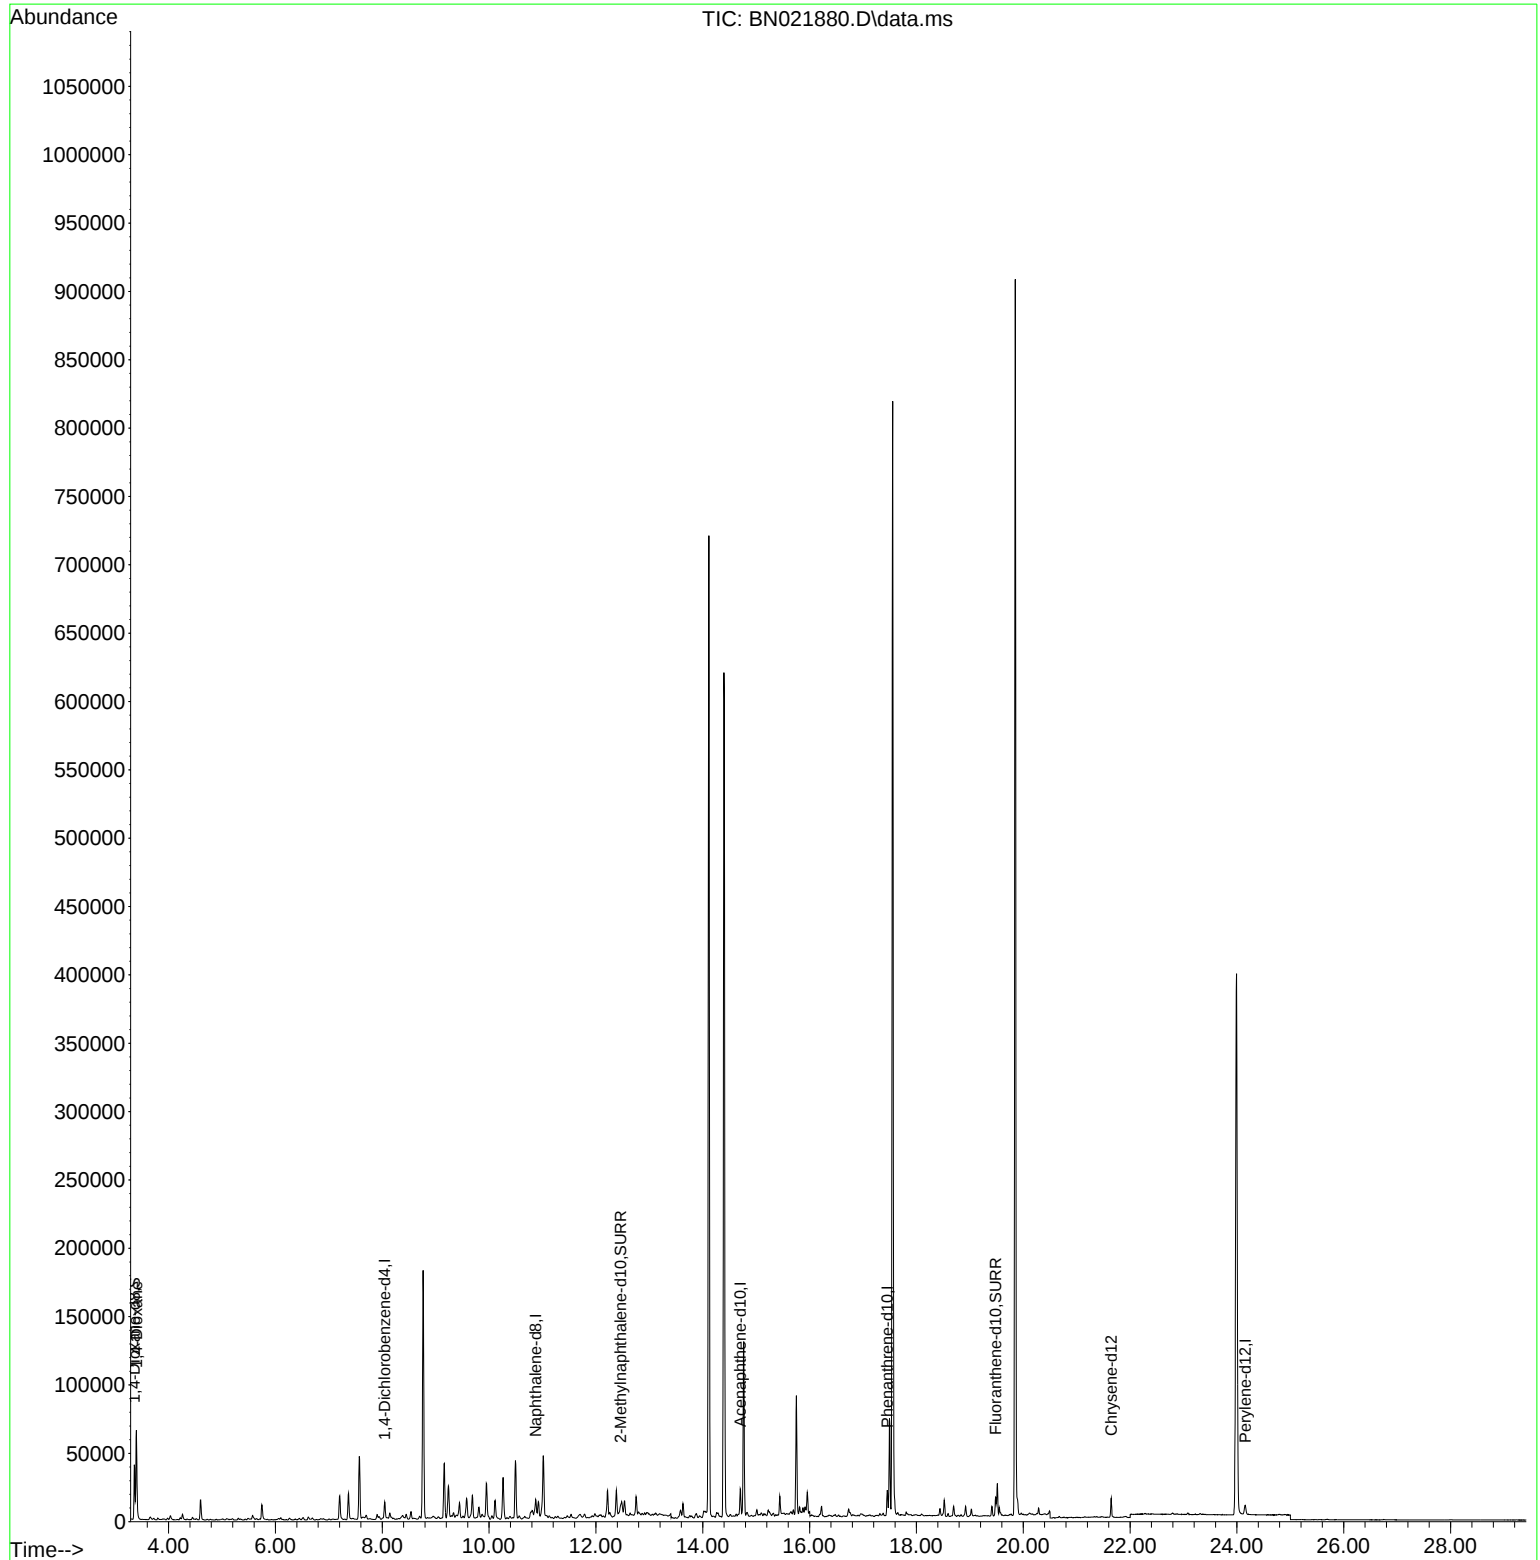

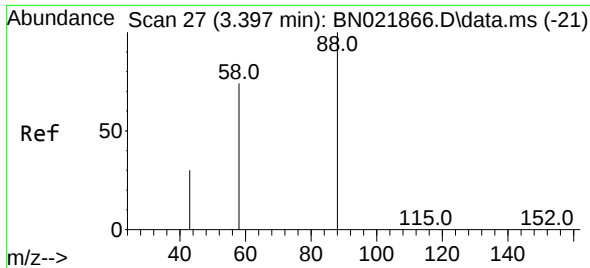

#2
 1,4-Dioxane
 Concen: 6.451 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021880.D
 Acq: 23 Sep 2022 01:02

Instrument :
 BNA_N
 ClientSampleId :
 CB8L0

Tgt Ion: 88	Resp: 45407
Ion Ratio	Lower Upper
88	100
43	28.6 31.4 47.0#
58	71.0 49.0 73.6

