

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021886.D
 Acq On : 23 Sep 2022 05:26
 Operator : CG/JU
 Sample : N4706-07
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8L2

Quant Time: Sep 23 06:05:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	668	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	1982	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.703	164	1086	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.451	188	2023	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	1358	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	1302	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	4065	4.946	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	1052	0.335	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	1980	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.498	178	142	0.022	ng/ul#	1
16) Anthracene	17.586	178	323	0.061	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021886.D
Acq On : 23 Sep 2022 05:26
Operator : CG/JU
Sample : N4706-07
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8L2

Quant Time: Sep 23 06:05:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




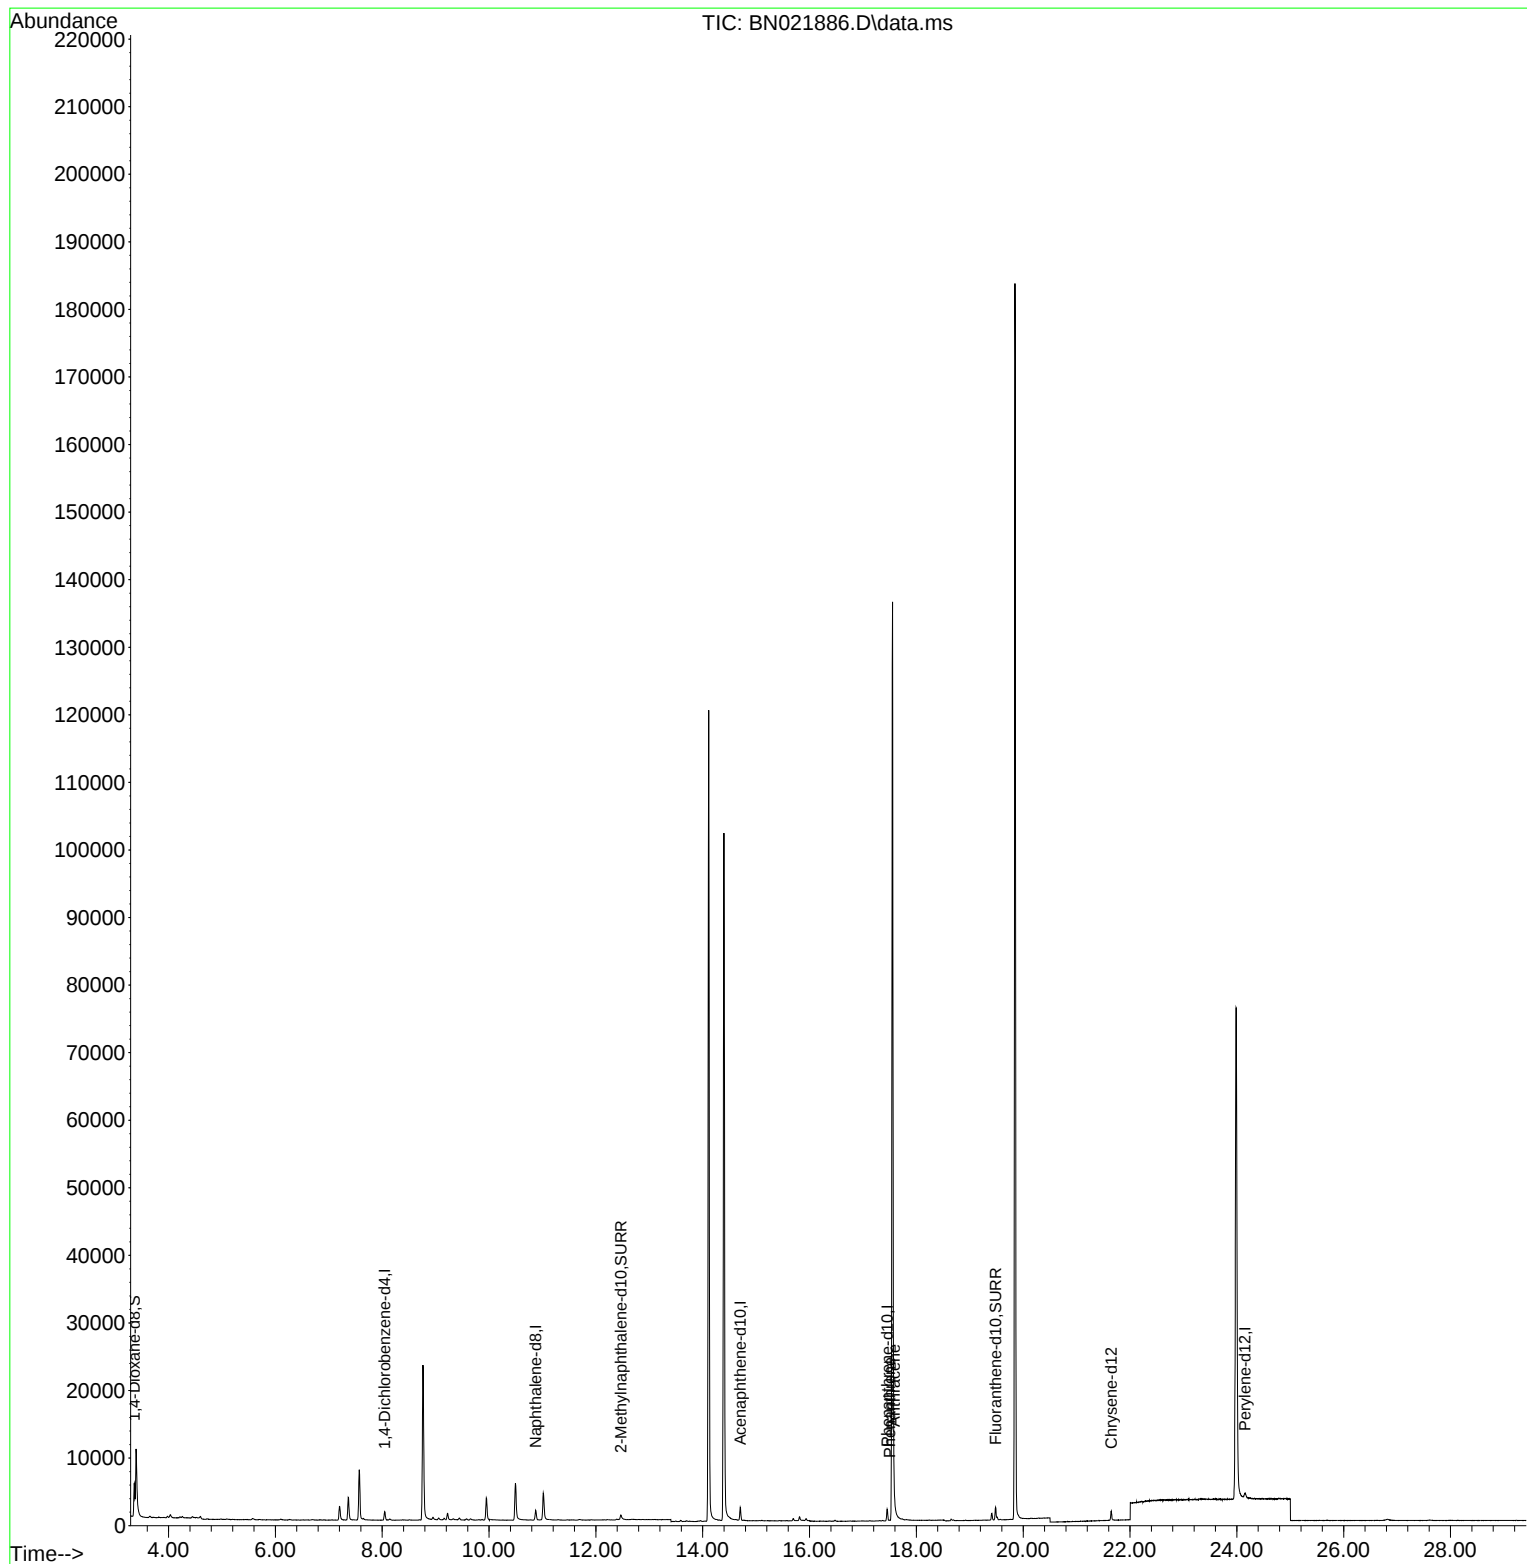


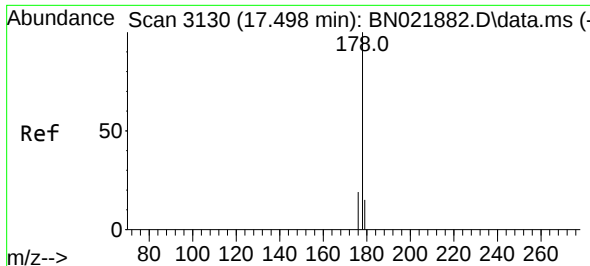

#15
Phenanthrene
Concen: 0.022 ng/ul
RT: 17.498 min Scan# 3130
Delta R.T. -0.004 min
Lab File: BN021886.D
Acq: 23 Sep 2022 05:26

Instrument :
BNA_N
ClientSampleId :
CB8L2

Tgt Ion:178 Resp: 142
Ion Ratio Lower Upper
178 100
179 69.5 12.8 19.2#
176 58.1 15.9 23.9#

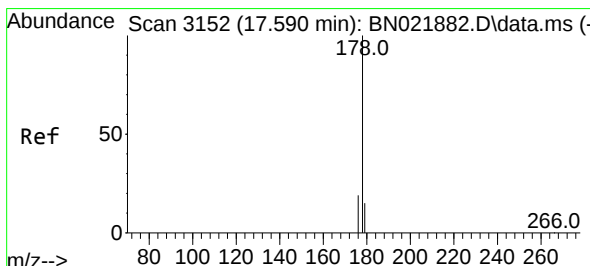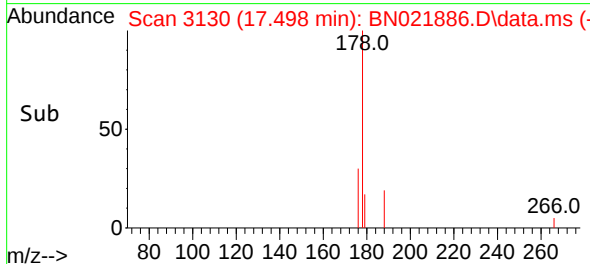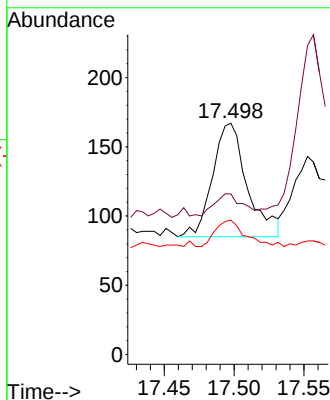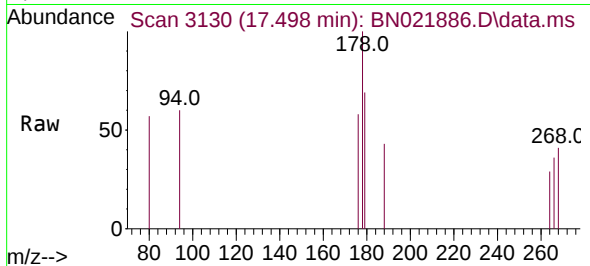

#16
Anthracene
Concen: 0.061 ng/ul
RT: 17.586 min Scan# 3151
Delta R.T. -0.009 min
Lab File: BN021886.D
Acq: 23 Sep 2022 05:26

Tgt Ion:178 Resp: 323
Ion Ratio Lower Upper
178 100
179 51.6 12.9 19.3#
176 42.6 15.9 23.9#

