

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021889.D
 Acq On : 23 Sep 2022 07:17
 Operator : CG/JU
 Sample : N4707-08
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8L4

Quant Time: Sep 23 07:43:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	7153	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	23412	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.703	164	14457	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.451	188	26740	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	17275	0.400	ng/ul	# 0.00
23) Perylene-d12	24.158	264	14508	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	31837	3.618	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.462	152	10030	0.271	ng/ul	-0.01
18) Fluoranthene-d10	19.483	212	21186	0.330	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	105993	11.743	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021889.D
Acq On : 23 Sep 2022 07:17
Operator : CG/JU
Sample : N4707-08
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8L4


Quant Time: Sep 23 07:43:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

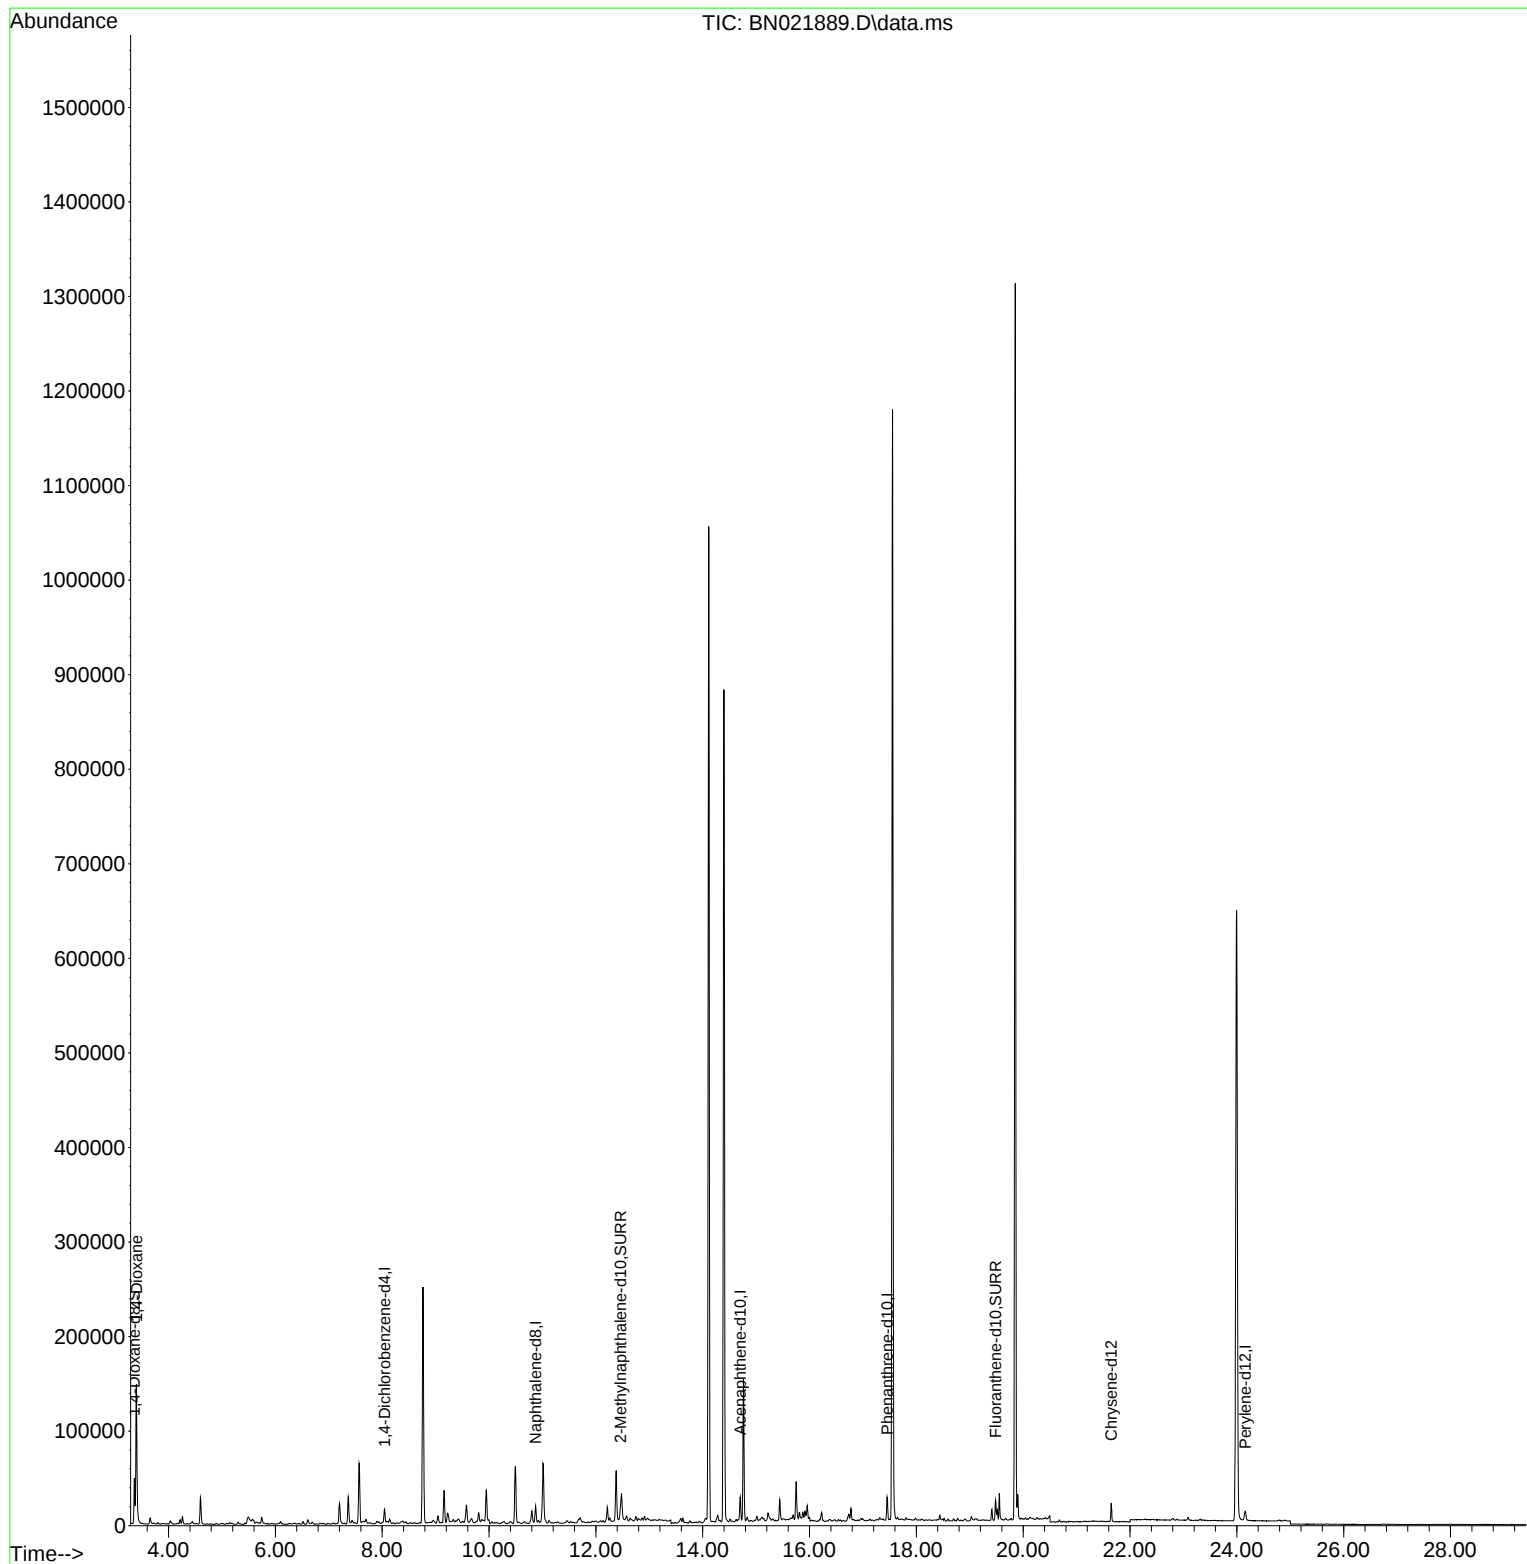

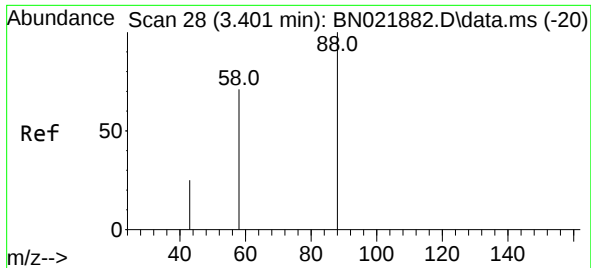

#2
 1,4-Dioxane
 Concen: 11.743 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021889.D
 Acq: 23 Sep 2022 07:17

Instrument :
 BNA_N
 ClientSampleId :
 CB8L4

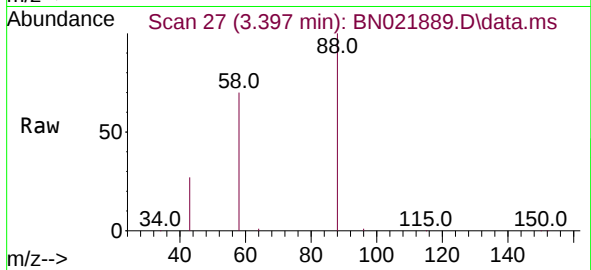

Tgt Ion: 88 Resp: 105993
 Ion Ratio Lower Upper
 88 100
 43 27.0 31.4 47.0#
 58 70.0 49.0 73.6

