

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
 Data File : BN021903.D
 Acq On : 23 Sep 2022 16:01
 Operator : CG/JU
 Sample : N4706-07
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8L2

Quant Time: Sep 24 01:02:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	5270	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	16930	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.702	164	9712	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	17776	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	10859	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	9521	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	32598	5.028	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.461	152	8682	0.324	ng/ul	-0.01
18) Fluoranthene-d10	19.482	212	15231	0.377	ng/ul	0.00
Target Compounds						
16) Anthracene	17.586	178	2060	0.044	ng/ul#	Qvalue 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092122\
Data File : BN021903.D
Acq On : 23 Sep 2022 16:01
Operator : CG/JU
Sample : N4706-07
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8L2


Quant Time: Sep 24 01:02:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

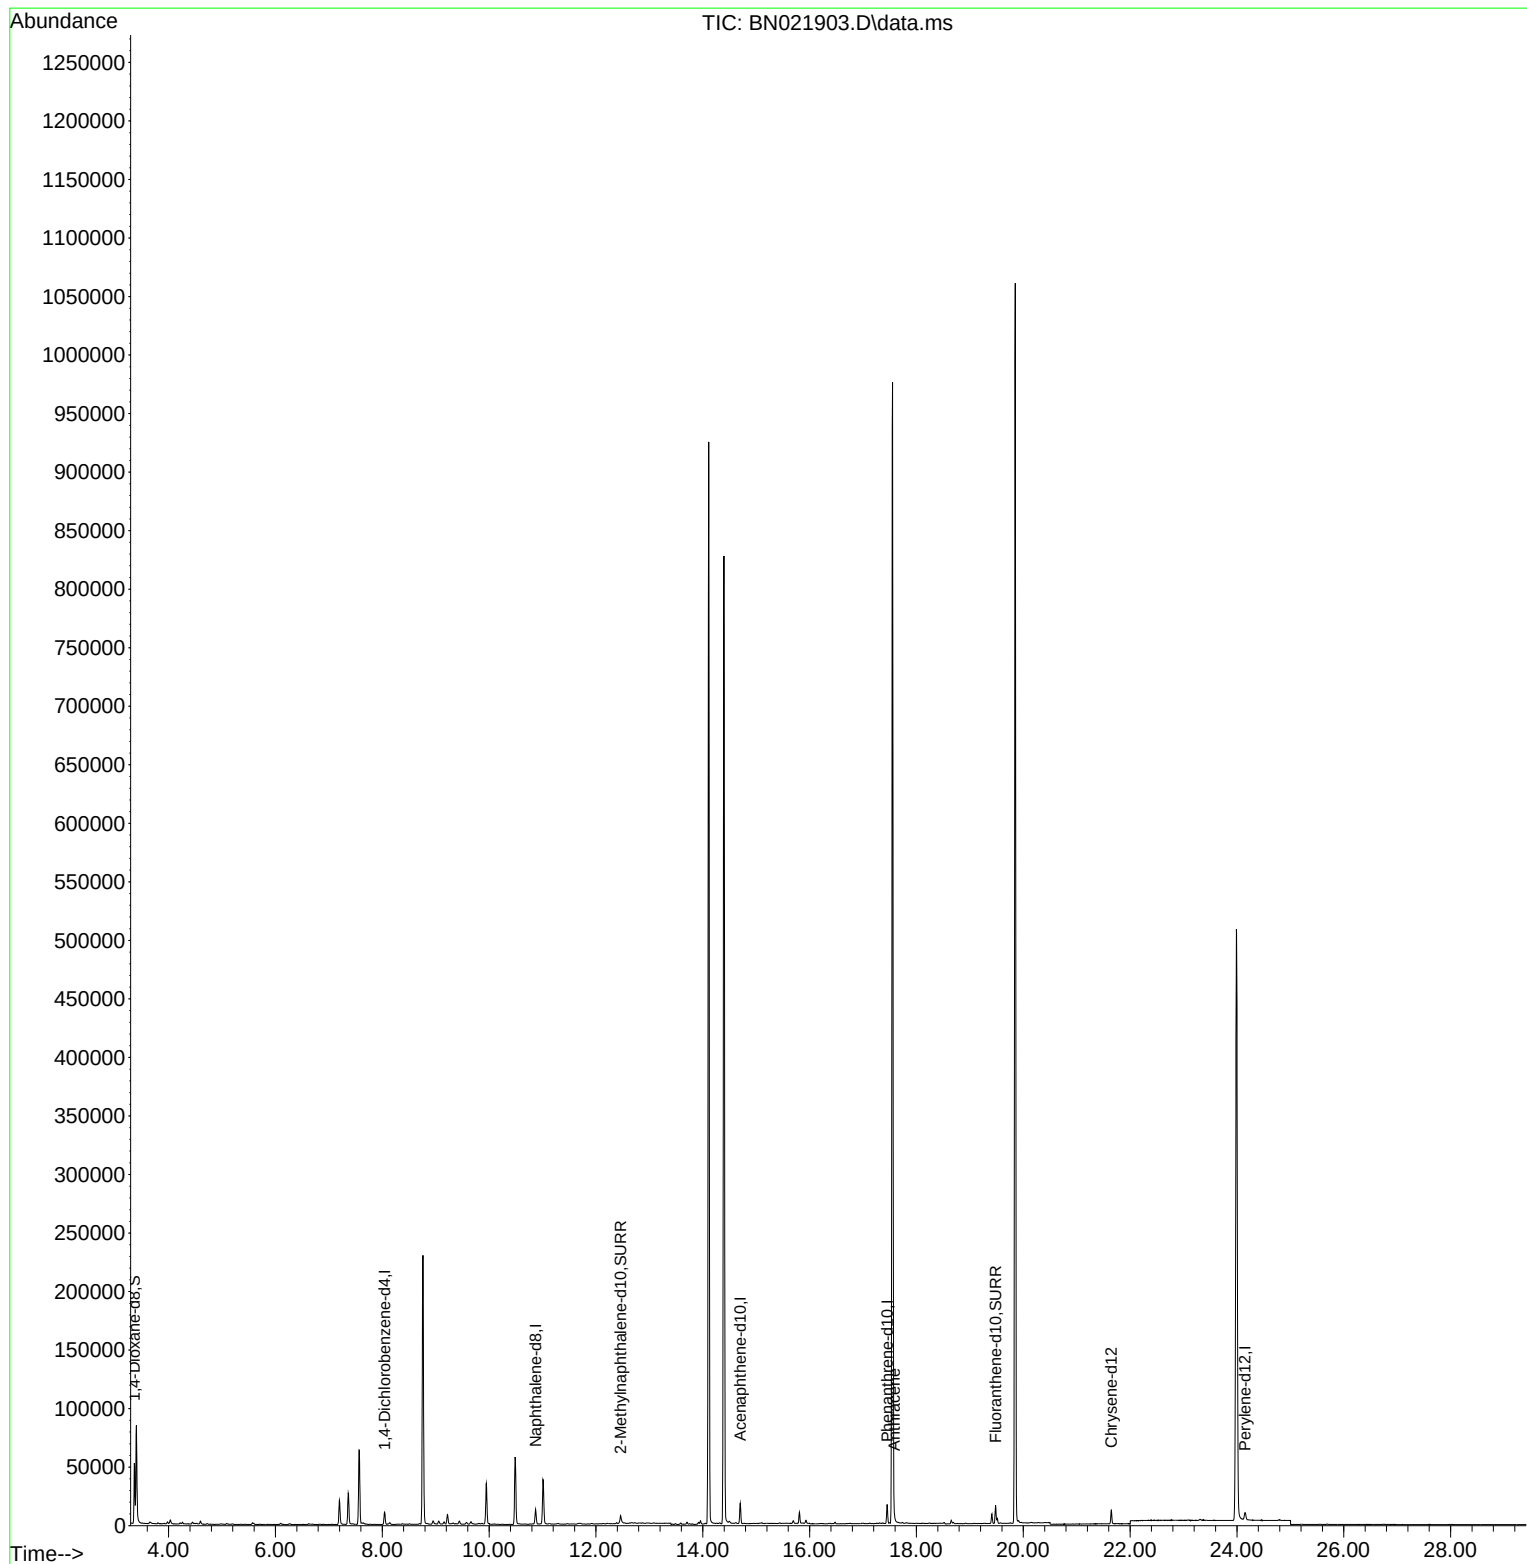

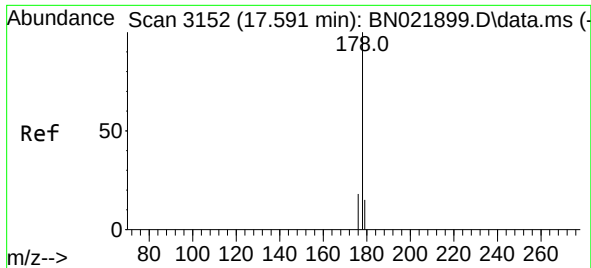

#16
 Anthracene
 Concen: 0.044 ng/ul
 RT: 17.586 min Scan# 31
 Delta R.T. -0.009 min
 Lab File: BN021903.D
 Acq: 23 Sep 2022 16:01

Instrument :
 BNA_N
 ClientSampleId :
 CB8L2

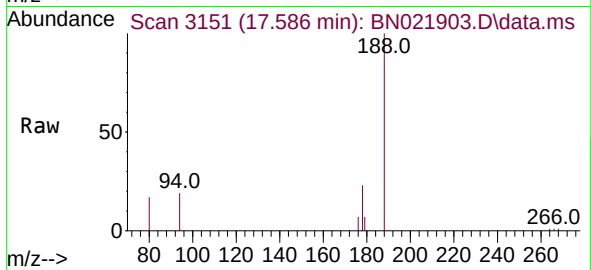

Tgt Ion:178 Resp: 2060
 Ion Ratio Lower Upper
 178 100
 179 32.2 12.9 19.3#
 176 28.4 15.9 23.9#

