

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092220\
 Data File : BN011869.D
 Acq On : 23 Sep 2020 02:29
 Operator : CG/JU
 Sample : PB131762BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB131762BL

Quant Time: Sep 23 08:27:54 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 22 14:36:55 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	3780	0.40	ng	0.00
7) Naphthalene-d8	10.478	136	14928	0.40	ng	0.00
13) Acenaphthene-d10	14.331	164	7171	0.40	ng	0.00
19) Phenanthrene-d10	17.078	188	14539	0.40	ng	0.00
29) Chrysene-d12	21.269	240	13663	0.40	ng	# 0.00
36) Perylene-d12	23.487	264	13877	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.307	112	4791	0.43	ng	0.00
5) Phenol-d6	6.869	99	5718	0.42	ng	0.00
8) Nitrobenzene-d5	8.843	82	4512	0.30	ng	0.00
11) 2-Methylnaphthalene-d10	12.064	152	8342	0.31	ng	0.00
14) 2,4,6-Tribromophenol	15.829	330	1242	0.34	ng	0.01
15) 2-Fluorobiphenyl	12.948	172	9714	0.31	ng	0.00
27) Fluoranthene-d10	19.107	212	12442	0.27	ng	0.00
31) Terphenyl-d14	19.712	244	12339	0.40	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.269	88	1733	0.31	ng	# 71
3) n-Nitrosodimethylamine	3.575	42	2344	0.31	ng	# 83
6) bis(2-Chloroethyl)ether	7.127	93	4258	0.35	ng	95
9) Naphthalene	10.516	128	12350	0.29	ng	99
10) Hexachlorobutadiene	10.808	225	1923	0.20	ng	# 99
12) 2-Methylnaphthalene	12.140	142	7828	0.27	ng	99
16) Acenaphthylene	14.040	152	9883	0.29	ng	100
17) Acenaphthene	14.395	154	6801	0.28	ng	94
18) Fluorene	15.384	166	8242	0.27	ng	99
20) 4,6-Dinitro-2-methylph...	15.461	198	617	0.25	ng	# 1
21) 4-Bromophenyl-phenylether	16.274	248	2062	0.24	ng	# 82
22) Hexachlorobenzene	16.384	284	2448	0.23	ng	# 88
23) Atrazine	16.542	200	1937	0.25	ng	# 91
24) Pentachlorophenol	16.725	266	2729	0.63	ng	99
25) Phenanthrene	17.114	178	12987	0.28	ng	99
26) Anthracene	17.211	178	11474	0.29	ng	99
28) Fluoranthene	19.137	202	14813	0.28	ng	# 95
30) Pyrene	19.499	202	15116	0.32	ng	99
32) Benzo(a)anthracene	21.248	228	13371	0.29	ng	99
33) Chrysene	21.301	228	13894	0.29	ng	99
34) Bis(2-ethylhexyl)phtha...	21.184	149	7569	0.32	ng	# 91
35) Indeno(1,2,3-cd)pyrene	25.715	276	16718	0.28	ng	# 89
37) Benzo(b)fluoranthene	22.820	252	13948	0.27	ng	# 81
38) Benzo(k)fluoranthene	22.864	252	15154	0.28	ng	# 81
39) Benzo(a)pyrene	23.388	252	12535	0.27	ng	# 73
40) Dibenzo(a,h)anthracene	25.732	278	13448	0.26	ng	# 82
41) Benzo(g,h,i)perylene	26.393	276	15598	0.29	ng	# 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092220\
 Data File : BN011869.D
 Acq On : 23 Sep 2020 02:29
 Operator : CG/JU
 Sample : PB131762BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB131762BL

Quant Time: Sep 23 08:27:54 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 22 14:36:55 2020
 Response via : Initial Calibration







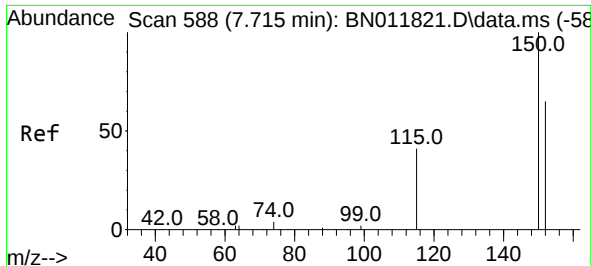

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.699 min Scan# 586
 Delta R.T. -0.000 min
 Lab File: BN011869.D
 Acq: 23 Sep 2020 02:29




Instrument :
 BNA_N
 ClientSampleId :
 PB131762BL


Tgt Ion:152 Resp: 3780
 Ion Ratio Lower Upper
 152 100
 150 154.3 118.3 177.5
 115 72.1 51.3 76.9



#2
 1,4-Dioxane
 Concen: 0.31 ng
 RT: 3.269 min Scan# 36
 Delta R.T. -0.000 min
 Lab File: BN011869.D
 Acq: 23 Sep 2020 02:29

Tgt Ion: 88 Resp: 1733
 Ion Ratio Lower Upper
 88 100
 58 85.1 63.3 94.9
 43 85.3 33.0 49.4#









#3
n-Nitrosodimethylamine
Concen: 0.31 ng
RT: 3.575 min Scan# 74
Delta R.T. -0.001 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion: 42 Resp: 2344
Ion Ratio Lower Upper
42 100
74 96.3 64.4 96.6
44 4.4 6.7 10.1#



#4
2-Fluorophenol
Concen: 0.43 ng
RT: 5.307 min Scan# 289
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion: 112 Resp: 4791
Ion Ratio Lower Upper
112 100
64 67.6 49.0 73.6
63 39.0 31.8 47.6









#5
Phenol-d6
Concen: 0.42 ng
RT: 6.869 min Scan# 483
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion: 99 Resp: 5718
Ion Ratio Lower Upper
99 100
42 29.9 23.4 35.0
71 42.3 38.1 57.1



#6
bis(2-Chloroethyl)ether
Concen: 0.35 ng
RT: 7.127 min Scan# 515
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion: 93 Resp: 4258
Ion Ratio Lower Upper
93 100
63 82.6 61.1 91.7
95 31.5 25.5 38.3









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.478 min Scan# 833
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:	136	Resp:	14928
Ion Ratio	Lower	Upper	
136	100		
137	11.6	9.5	14.3
54	6.4	5.6	8.4
68	4.4	3.2	4.8



#8
Nitrobenzene-d5
Concen: 0.30 ng
RT: 8.843 min Scan# 704
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:	82	Resp:	4512
Ion Ratio	Lower	Upper	
82	100		
128	39.4	34.2	51.2
54	53.4	43.1	64.7









#9
Naphthalene
Concen: 0.29 ng
RT: 10.516 min Scan# 836
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:128 Resp: 12350
Ion Ratio Lower Upper
128 100
129 11.5 9.7 14.5
127 13.8 11.0 16.4



#10
Hexachlorobutadiene
Concen: 0.20 ng
RT: 10.808 min Scan# 859
Delta R.T. -0.013 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:225 Resp: 1923
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.9 77.9









#11
2-Methylnaphthalene-d10
Concen: 0.31 ng
RT: 12.064 min Scan# 1038
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:152 Resp: 8342
Ion Ratio Lower Upper
152 100
151 15.8 16.7 25.1#



#12
2-Methylnaphthalene
Concen: 0.27 ng
RT: 12.140 min Scan# 1055
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:142 Resp: 7828
Ion Ratio Lower Upper
142 100
141 88.4 70.0 105.0
115 45.2 35.8 53.6









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.331 min Scan# 1281
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:164 Resp: 7171
Ion Ratio Lower Upper
164 100
162 101.1 83.6 125.4
160 46.6 41.2 61.8



#14
2,4,6-Tribromophenol
Concen: 0.34 ng
RT: 15.829 min Scan# 1399
Delta R.T. 0.013 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:330 Resp: 1242
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 53.6 33.7 50.5#









#15
2-Fluorobiphenyl
Concen: 0.31 ng
RT: 12.948 min Scan# 1172
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:	172	Resp:	9714
Ion Ratio	Lower	Upper	
172	100		
171	35.4	27.4	41.2
170	24.3	17.8	26.6



#16
Acenaphthylene
Concen: 0.29 ng
RT: 14.040 min Scan# 1258
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:	152	Resp:	9883
Ion Ratio	Lower	Upper	
152	100		
151	19.6	15.9	23.9
153	13.0	10.5	15.7









#17
Acenaphthene
Concen: 0.28 ng
RT: 14.395 min Scan# 1286
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:154 Resp: 6801
Ion Ratio Lower Upper
154 100
153 112.5 83.4 125.2
152 55.7 42.8 64.2



#18
Fluorene
Concen: 0.27 ng
RT: 15.384 min Scan# 1364
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:166 Resp: 8242
Ion Ratio Lower Upper
166 100
165 99.5 78.8 118.2
167 13.7 11.2 16.8









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.078 min Scan# 1501
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:188 Resp: 14539
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.9 7.7 11.5



#20
4,6-Dinitro-2-methylphenol
Concen: 0.25 ng
RT: 15.461 min Scan# 1370
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:198 Resp: 617
Ion Ratio Lower Upper
198 100
51 189.2 45.0 67.4#
105 85.2 30.4 45.6#









#21
4-Bromophenyl-phenylether
Concen: 0.24 ng
RT: 16.274 min Scan# 1435
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:248 Resp: 2062
Ion Ratio Lower Upper
248 100
250 100.5 82.7 124.1
141 76.4 33.7 50.5#



#22
Hexachlorobenzene
Concen: 0.23 ng
RT: 16.384 min Scan# 1444
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:284 Resp: 2448
Ion Ratio Lower Upper
284 100
142 54.1 32.4 48.6#
249 33.0 26.8 40.2





#23

Atrazine

Concen: 0.25 ng

RT: 16.542 min Scan# 1457

Delta R.T. -0.000 min

Lab File: BN011869.D

Acq: 23 Sep 2020 02:29





Tgt Ion:200 Resp: 1937

Ion Ratio Lower Upper

200 100

173 31.1 18.7 28.1#

215 46.6 40.2 60.4



#24

Pentachlorophenol

Concen: 0.63 ng

RT: 16.725 min Scan# 1472

Delta R.T. -0.000 min

Lab File: BN011869.D

Acq: 23 Sep 2020 02:29




Tgt Ion:266 Resp: 2729


Ion Ratio Lower Upper

266 100

264 63.7 51.2 76.8

268 63.8 52.4 78.6





#25

Phenanthrene

Concen: 0.28 ng

RT: 17.114 min Scan# 1504

Delta R.T. -0.000 min

Lab File: BN011869.D

Acq: 23 Sep 2020 02:29





Tgt Ion:178 Resp: 12987

Ion Ratio Lower Upper

178 100

176 19.7 15.1 22.7

179 15.5 12.3 18.5



#26

Anthracene

Concen: 0.29 ng

RT: 17.211 min Scan# 1512

Delta R.T. -0.000 min

Lab File: BN011869.D

Acq: 23 Sep 2020 02:29




Tgt Ion:178 Resp: 11474


Ion Ratio Lower Upper

178 100

176 18.7 14.6 21.8

179 15.3 12.4 18.6









#27
Fluoranthene-d10
Concen: 0.27 ng
RT: 19.107 min Scan# 1798
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:212 Resp: 12442
Ion Ratio Lower Upper
212 100
106 14.0 6.4 9.6#
104 8.8 3.9 5.9#



#28
Fluoranthene
Concen: 0.28 ng
RT: 19.137 min Scan# 1804
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:202 Resp: 14813
Ion Ratio Lower Upper
202 100
101 12.0 5.4 8.2#
203 16.6 13.8 20.6









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.269 min Scan# 2098
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:240 Resp: 13663
Ion Ratio Lower Upper
240 100
120 10.3 3.5 5.3#
236 26.8 20.5 30.7



#30
Pyrene
Concen: 0.32 ng
RT: 19.499 min Scan# 1877
Delta R.T. -0.005 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29


Tgt Ion:202 Resp: 15116
Ion Ratio Lower Upper
202 100
200 20.9 16.5 24.7
203 17.8 13.9 20.9








#31
Terphenyl-d14
Concen: 0.40 ng
RT: 19.712 min Scan# 1920
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Instrument :
BNA_N
ClientSampleId :
PB131762BL







Tgt Ion:244 Resp: 12339
Ion Ratio Lower Upper
244 100
212 8.6 7.3 10.9
122 13.8 7.8 11.6#



#32
Benzo(a)anthracene
Concen: 0.29 ng
RT: 21.248 min Scan# 2096
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:228 Resp: 13371
Ion Ratio Lower Upper
228 100
226 26.7 21.0 31.4
229 19.7 16.0 24.0









#33
Chrysene
Concen: 0.29 ng
RT: 21.301 min Scan# 2101
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:	228	Resp:	13894
Ion Ratio	Lower	Upper	
228	100		
226	29.9	23.3	34.9
229	20.1	15.8	23.8



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.32 ng
RT: 21.184 min Scan# 2090
Delta R.T. -0.000 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:	149	Resp:	7569
Ion Ratio	Lower	Upper	
149	100		
167	24.3	23.6	35.4
279	3.5	4.0	6.0#









#35
Indeno(1,2,3-cd)pyrene
Concen: 0.28 ng
RT: 25.715 min Scan# 3172
Delta R.T. -0.004 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:276 Resp: 16718
Ion Ratio Lower Upper
276 100
138 26.6 13.0 19.4#
277 24.2 20.0 30.0



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.487 min Scan# 2521
Delta R.T. -0.004 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:264 Resp: 13877
Ion Ratio Lower Upper
264 100
260 24.7 19.6 29.4
265 72.1 38.6 58.0#









#37
Benzo(b)fluoranthene
Concen: 0.27 ng
RT: 22.820 min Scan# 2326
Delta R.T. -0.004 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29




Instrument :
BNA_N
ClientSampleId :
PB131762BL


Tgt Ion:252 Resp: 13948
Ion Ratio Lower Upper
252 100
253 29.8 19.1 28.7#
125 22.2 6.2 9.2#



#38
Benzo(k)fluoranthene
Concen: 0.28 ng
RT: 22.864 min Scan# 2339
Delta R.T. -0.004 min
Lab File: BN011869.D
Acq: 23 Sep 2020 02:29

Tgt Ion:252 Resp: 15154
Ion Ratio Lower Upper
252 100
253 30.5 19.3 28.9#
125 20.3 6.0 9.0#





#39

Benzo(a)pyrene

Concen: 0.27 ng





RT: 23.388 min Scan# 2492

Delta R.T. -0.004 min

Lab File: BN011869.D

Acq: 23 Sep 2020 02:29

Tgt Ion:	252	Resp:	12535
Ion Ratio	Lower	Upper	
252	100		
253	33.3	19.8	29.6#
125	28.2	7.3	10.9#



#40

Dibenzo(a,h)anthracene

Concen: 0.26 ng




RT: 25.732 min Scan# 3177


Delta R.T. -0.000 min

Lab File: BN011869.D

Acq: 23 Sep 2020 02:29


Tgt Ion:	278	Resp:	13448
Ion Ratio	Lower	Upper	
278	100		
139	21.0	8.6	13.0#
279	31.6	19.8	29.8#





#41
 Benzo(g,h,i)perylene
 Concen: 0.29 ng
 RT: 26.393 min Scan# 3370
 Delta R.T. -0.000 min
 Lab File: BN011869.D
 Acq: 23 Sep 2020 02:29

Instrument :
 BNA_N
 ClientSampleId :
 PB131762BL



Tgt Ion:	276	Resp:	15598
Ion Ratio	Lower	Upper	
276	100		
277	25.1	19.4	29.0
138	26.7	11.3	16.9#

