


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092220\
 Data File : BN011849.D
 Acq On : 22 Sep 2020 13:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 23 11:18:21 2020

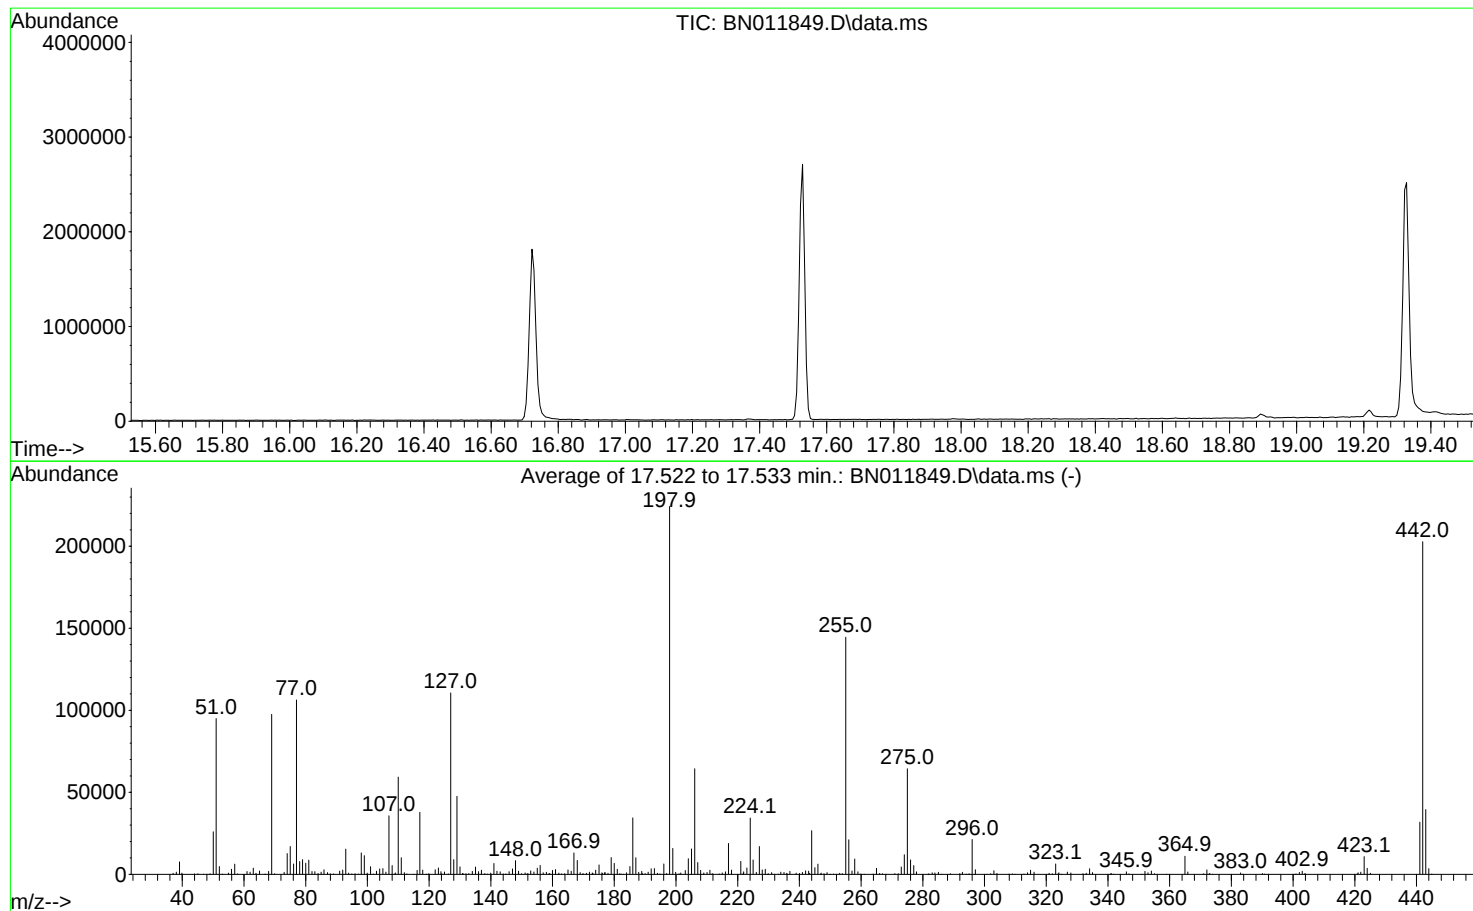

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	94968	PASS
68	69	0.00	2	1.9	1808	PASS
69	198	0.00	100	43.5	97533	PASS
70	69	0.00	2	0.4	423	PASS
127	198	10	80	49.3	110571	PASS
197	198	0.00	2	0.3	587	PASS
198	198	100	100	100.0	224213	PASS
199	198	5	9	7.0	15761	PASS
275	198	10	60	28.7	64347	PASS
365	198	1	100	4.9	11047	PASS
441	198	0.01	100	14.2	31837	PASS
442	198	50	100	90.4	202773	PASS
443	442	15	24	19.5	39456	PASS