


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092220\
Data File : BN011867.D
Acq On : 23 Sep 2020 00:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 23 11:18:21 2020

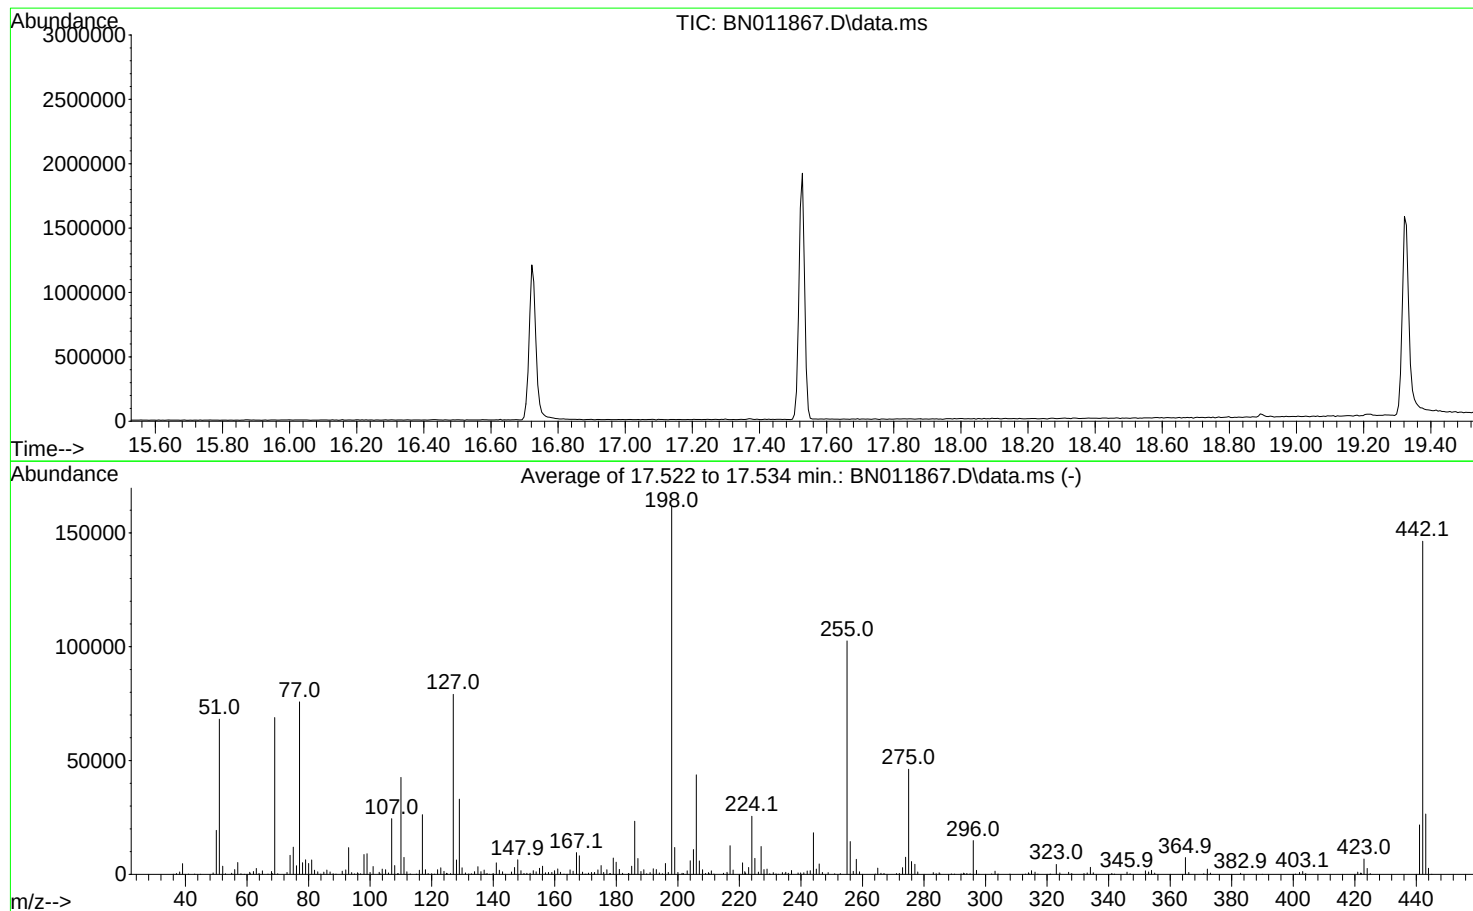

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	68205	PASS
68	69	0.00	2	1.9	1294	PASS
69	198	0.00	100	42.6	68901	PASS
70	69	0.00	2	0.4	307	PASS
127	198	10	80	48.9	79099	PASS
197	198	0.00	2	0.5	854	PASS
198	198	100	100	100.0	161611	PASS
199	198	5	9	7.3	11841	PASS
275	198	10	60	28.6	46181	PASS
365	198	1	100	4.6	7362	PASS
441	198	0.01	100	13.4	21688	PASS
442	198	50	100	90.6	146357	PASS
443	442	15	24	18.1	26523	PASS