

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092320\
 Data File : BN011884.D
 Acq On : 23 Sep 2020 15:10
 Operator : CG/JU
 Sample : SSTDIC0.2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.2

Quant Time: Sep 23 16:19:48 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 16:16:06 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.691	152	3140	0.40	ng	0.00
7) Naphthalene-d8	10.466	136	12458	0.40	ng	# 0.00
13) Acenaphthene-d10	14.319	164	6266	0.40	ng	0.00
19) Phenanthrene-d10	17.066	188	12876	0.40	ng	0.00
29) Chrysene-d12	21.269	240	11661	0.40	ng	# 0.00
36) Perylene-d12	23.487	264	11825	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	2275	0.25	ng	0.00
5) Phenol-d6	6.861	99	2647	0.23	ng	0.00
8) Nitrobenzene-d5	8.831	82	2411	0.19	ng	0.00
11) 2-Methylnaphthalene-d10	12.060	152	3871	0.18	ng	0.00
14) 2,4,6-Tribromophenol	15.816	330	569	0.18	ng	0.00
15) 2-Fluorobiphenyl	12.936	172	4679	0.17	ng	0.00
27) Fluoranthene-d10	19.102	212	7388	0.18	ng	0.00
31) Terphenyl-d14	19.708	244	5404	0.20	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.254	88	1120	0.24	ng	97
3) n-Nitrosodimethylamine	3.568	42	1400	0.22	ng	90
6) bis(2-Chloroethyl)ether	7.119	93	2198	0.22	ng	91
9) Naphthalene	10.516	128	7208	0.21	ng	99
10) Hexachlorobutadiene	10.808	225	1192	0.15	ng	# 98
12) 2-Methylnaphthalene	12.131	142	4409	0.18	ng	99
16) Acenaphthylene	14.040	152	5798	0.19	ng	99
17) Acenaphthene	14.382	154	3928	0.19	ng	89
18) Fluorene	15.372	166	4916	0.19	ng	99
20) 4,6-Dinitro-2-methylph...	15.461	198	432	0.20	ng	# 1
21) 4-Bromophenyl-phenylether	16.262	248	1303	0.17	ng	# 64
22) Hexachlorobenzene	16.372	284	1571	0.17	ng	# 84
23) Atrazine	16.542	200	1252	0.18	ng	94
24) Pentachlorophenol	16.725	266	830	0.22	ng	90
25) Phenanthrene	17.102	178	7507	0.18	ng	99
26) Anthracene	17.199	178	6440	0.18	ng	100
28) Fluoranthene	19.132	202	8463	0.18	ng	# 94
30) Pyrene	19.499	202	8826	0.22	ng	100
32) Benzo(a)anthracene	21.248	228	7166	0.18	ng	98
33) Chrysene	21.301	228	8016	0.20	ng	98
34) Bis(2-ethylhexyl)phtha...	21.195	149	5341	0.26	ng	93
35) Indeno(1,2,3-cd)pyrene	25.712	276	9353	0.18	ng	# 88
37) Benzo(b)fluoranthene	22.823	252	7639	0.17	ng	# 70
38) Benzo(k)fluoranthene	22.868	252	8457	0.19	ng	# 71
39) Benzo(a)pyrene	23.391	252	6799	0.17	ng	# 60
40) Dibenzo(a,h)anthracene	25.726	278	7315	0.17	ng	# 74
41) Benzo(g,h,i)perylene	26.390	276	8563	0.19	ng	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092320\
Data File : BN011884.D
Acq On : 23 Sep 2020 15:10
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Sep 23 16:19:48 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 16:16:06 2020
Response via : Initial Calibration




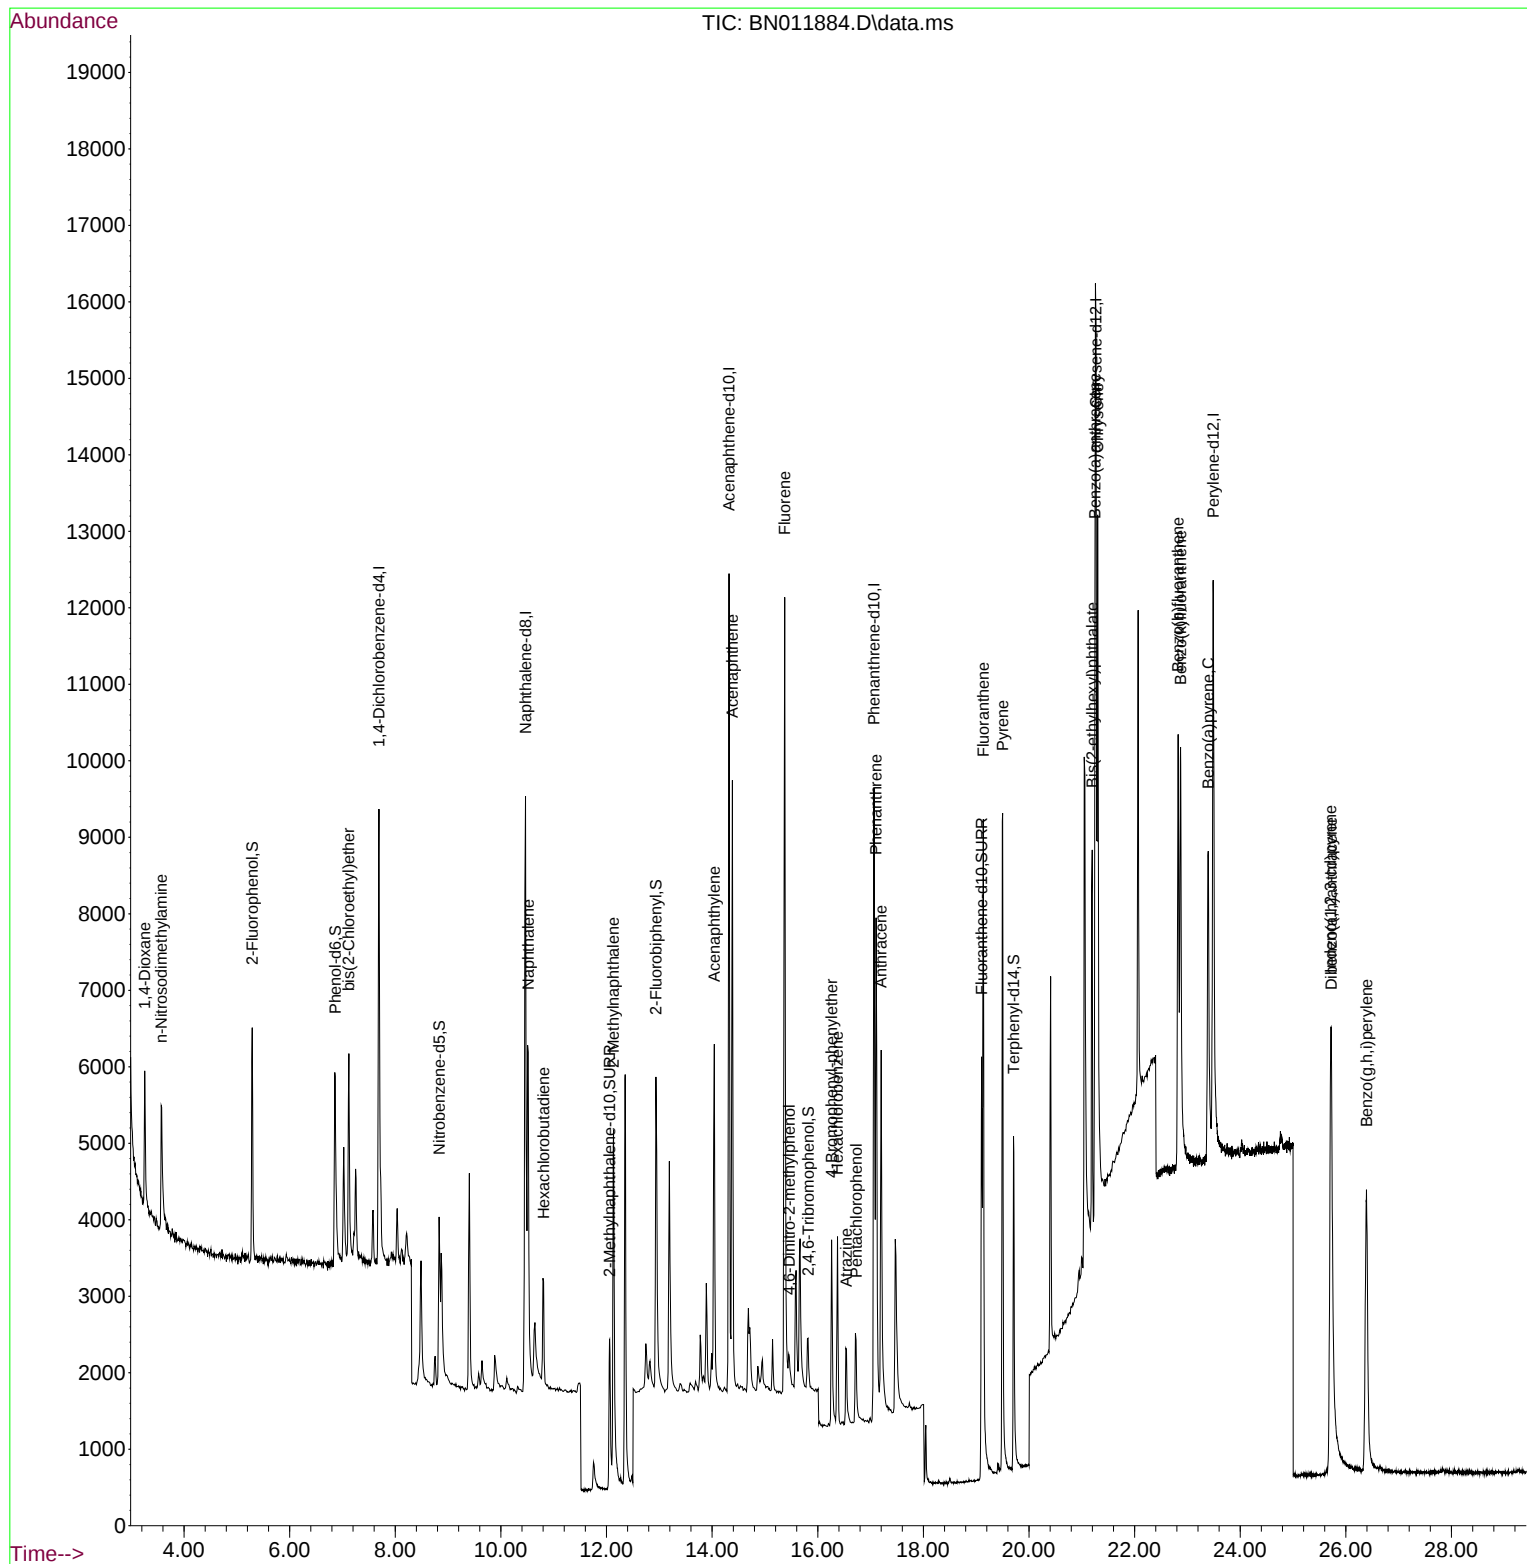




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.691 min Scan# 585
 Delta R.T. -0.000 min
 Lab File: BN011884.D
 Acq: 23 Sep 2020 15:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:152 Resp: 3140
 Ion Ratio Lower Upper
 152 100
 150 149.8 118.3 177.5
 115 71.6 51.3 76.9



#2
 1,4-Dioxane
 Concen: 0.24 ng
 RT: 3.254 min Scan# 34
 Delta R.T. 0.000 min
 Lab File: BN011884.D
 Acq: 23 Sep 2020 15:10

Tgt Ion: 88 Resp: 1120
 Ion Ratio Lower Upper
 88 100
 58 82.8 63.3 94.9
 43 40.4 33.0 49.4


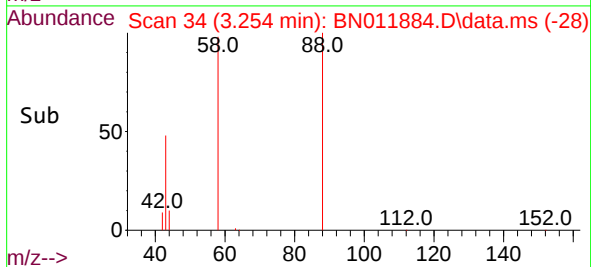

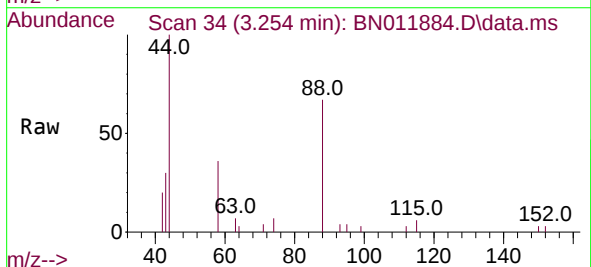


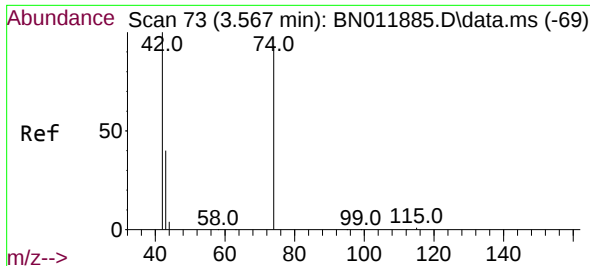

#3
n-Nitrosodimethylamine
Concen: 0.22 ng
RT: 3.568 min Scan# 73
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion: 42 Resp: 1400
Ion Ratio Lower Upper
42 100
74 90.0 64.4 96.6
44 8.4 6.7 10.1

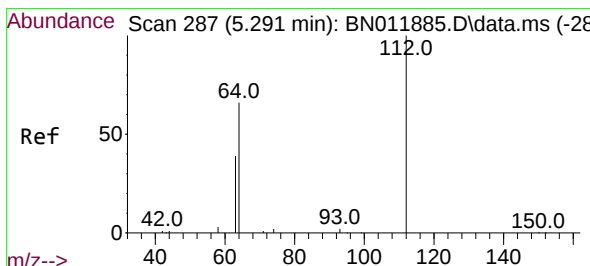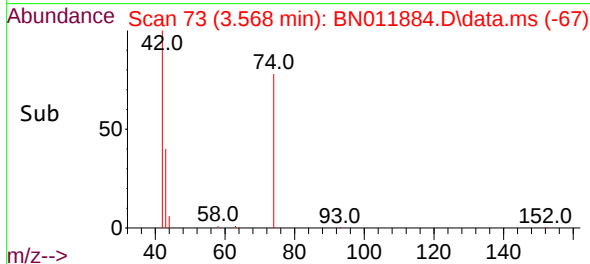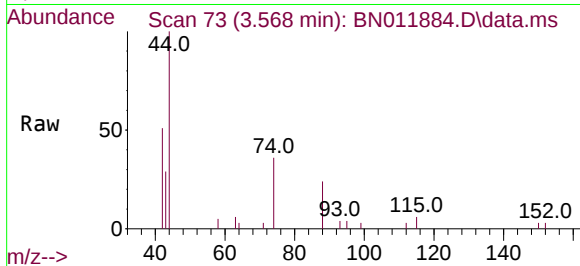

#4
2-Fluorophenol
Concen: 0.25 ng
RT: 5.291 min Scan# 287
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion: 112 Resp: 2275
Ion Ratio Lower Upper
112 100
64 69.2 49.0 73.6
63 40.2 31.8 47.6


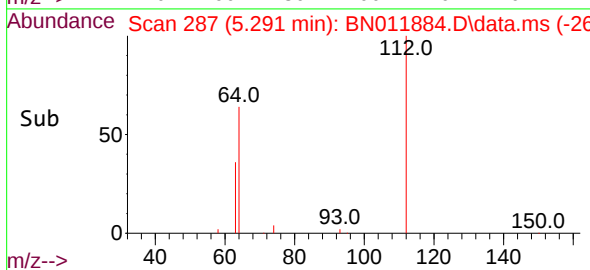

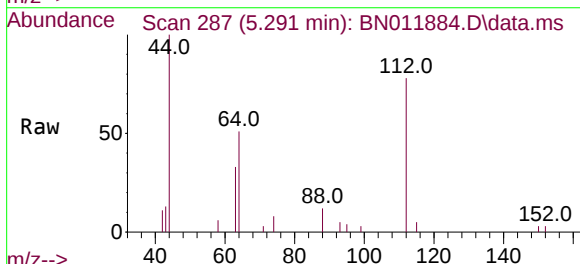




#5
Phenol-d6
Concen: 0.23 ng
RT: 6.861 min Scan# 482
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion: 99 Resp: 2647
Ion Ratio Lower Upper
99 100
42 28.6 23.4 35.0
71 45.4 38.1 57.1

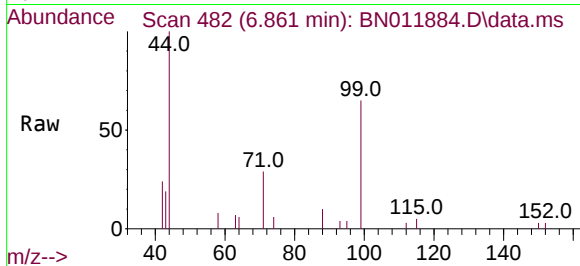

#6
bis(2-Chloroethyl)ether
Concen: 0.22 ng
RT: 7.119 min Scan# 514
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion: 93 Resp: 2198
Ion Ratio Lower Upper
93 100
63 87.1 61.1 91.7
95 33.1 25.5 38.3


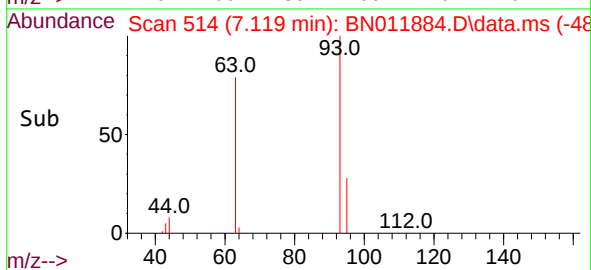

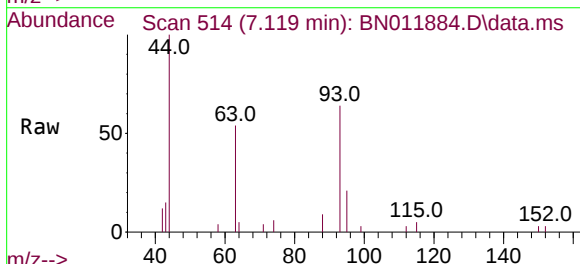




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.466 min Scan# 832
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	136	Resp:	12458
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.5	14.3
54	7.8	5.6	8.4
68	5.7	3.2	4.8

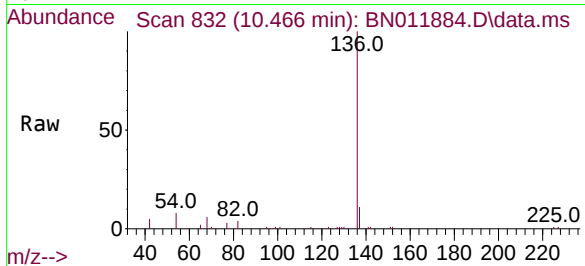

#8
Nitrobenzene-d5
Concen: 0.19 ng
RT: 8.831 min Scan# 703
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:	82	Resp:	2411
Ion	Ratio	Lower	Upper
82	100		
128	36.3	34.2	51.2
54	60.9	43.1	64.7


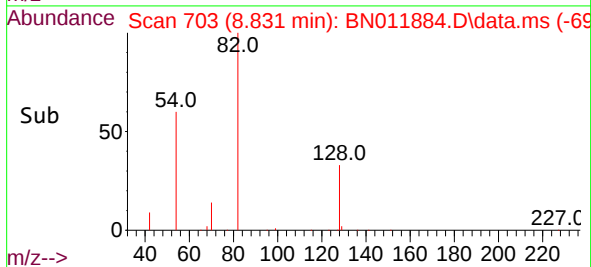

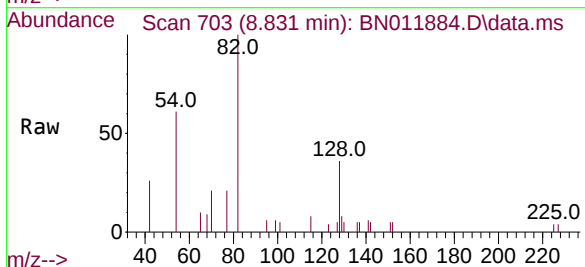




#9
Naphthalene
Concen: 0.21 ng
RT: 10.516 min Scan# 836
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:	128	Resp:	7208
Ion	Ratio	Lower	Upper
128	100		
129	12.5	9.7	14.5
127	13.9	11.0	16.4



#10
Hexachlorobutadiene
Concen: 0.15 ng
RT: 10.808 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:	225	Resp:	1192
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.4	51.9	77.9


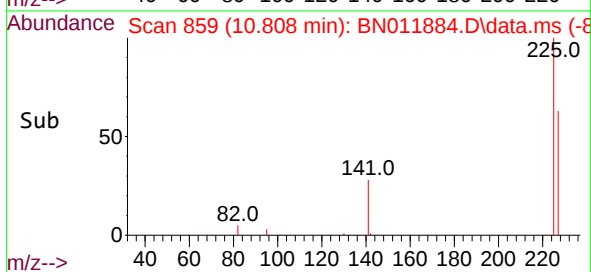






#11
2-Methylnaphthalene-d10
Concen: 0.18 ng
RT: 12.060 min Scan# 1037
Delta R.T. 0.005 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:152 Resp: 3871
Ion Ratio Lower Upper
152 100
151 19.3 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.18 ng
RT: 12.131 min Scan# 1053
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:142 Resp: 4409
Ion Ratio Lower Upper
142 100
141 88.0 70.0 105.0
115 46.2 35.8 53.6


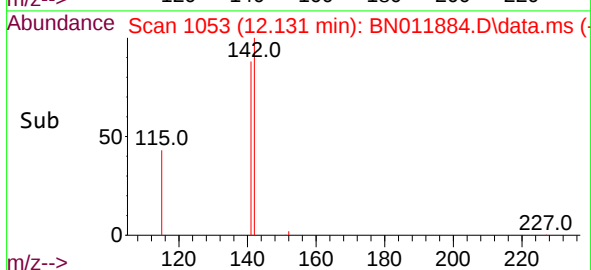






#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.319 min Scan# 1280
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:164 Resp: 6266
Ion Ratio Lower Upper
164 100
162 104.7 83.6 125.4
160 49.9 41.2 61.8



#14
2,4,6-Tribromophenol
Concen: 0.18 ng
RT: 15.816 min Scan# 1398
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:330 Resp: 569
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 55.9 33.7 50.5#


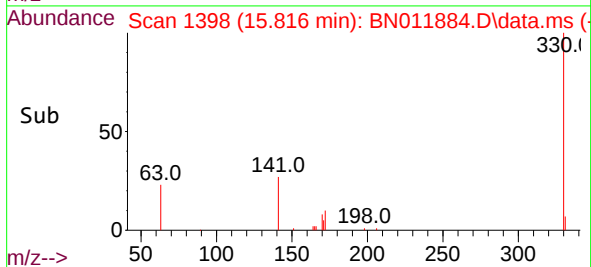

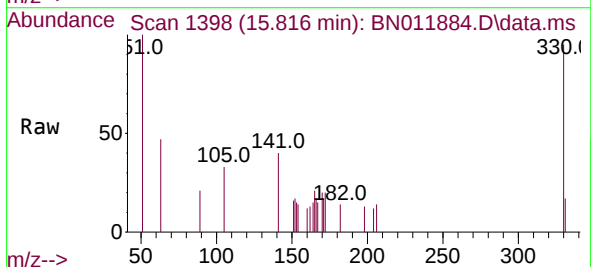




#15
2-Fluorobiphenyl
Concen: 0.17 ng
RT: 12.936 min Scan# 1171
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	172	Resp:	4679
Ion	Ratio	Lower	Upper
172	100		
171	36.8	27.4	41.2
170	26.3	17.8	26.6



#16
Acenaphthylene
Concen: 0.19 ng
RT: 14.040 min Scan# 1258
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:	152	Resp:	5798
Ion	Ratio	Lower	Upper
152	100		
151	19.1	15.9	23.9
153	12.7	10.5	15.7


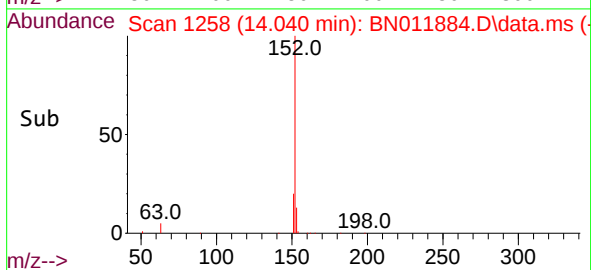






#17
Acenaphthene
Concen: 0.19 ng
RT: 14.382 min Scan# 1285
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:154 Resp: 3928
Ion Ratio Lower Upper
154 100
153 118.3 83.4 125.2
152 57.8 42.8 64.2



#18
Fluorene
Concen: 0.19 ng
RT: 15.372 min Scan# 1363
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:166 Resp: 4916
Ion Ratio Lower Upper
166 100
165 99.0 78.8 118.2
167 13.3 11.2 16.8


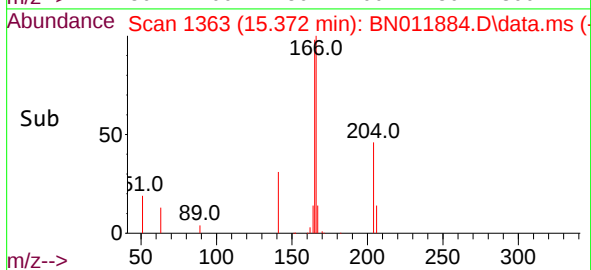






#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.066 min Scan# 1500
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:188 Resp: 12876
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.4 7.7 11.5



#20
4,6-Dinitro-2-methylphenol
Concen: 0.20 ng
RT: 15.461 min Scan# 1370
Delta R.T. 0.013 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:198 Resp: 432
Ion Ratio Lower Upper
198 100
51 257.9 45.0 67.4#
105 90.7 30.4 45.6#


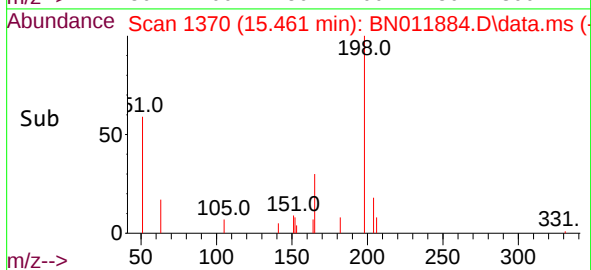






#21
4-Bromophenyl-phenylether
Concen: 0.17 ng
RT: 16.262 min Scan# 1434
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:248 Resp: 1303
Ion Ratio Lower Upper
248 100
250 91.4 82.7 124.1
141 102.5 33.7 50.5#

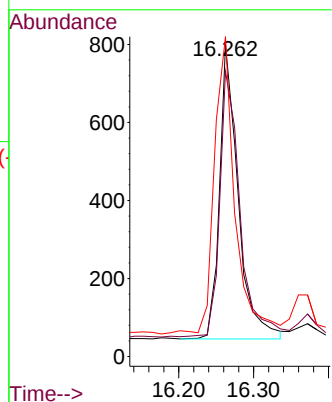

#22
Hexachlorobenzene
Concen: 0.17 ng
RT: 16.372 min Scan# 1443
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:284 Resp: 1571
Ion Ratio Lower Upper
284 100
142 57.4 32.4 48.6#
249 32.5 26.8 40.2


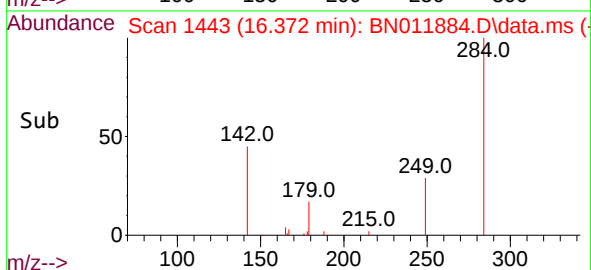




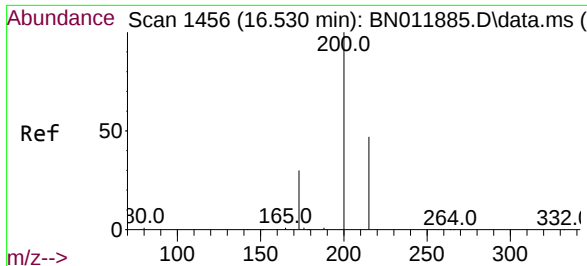

#23
Atrazine
Concen: 0.18 ng
RT: 16.542 min Scan# 1457
Delta R.T. 0.012 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:200 Resp: 1252
Ion Ratio Lower Upper
200 100
173 27.6 18.7 28.1
215 47.1 40.2 60.4

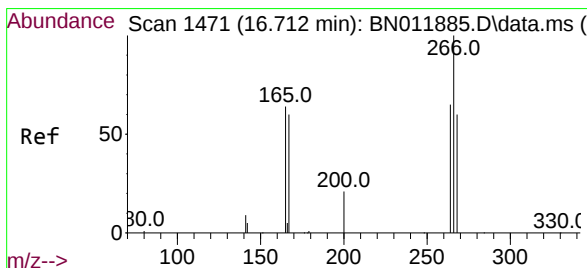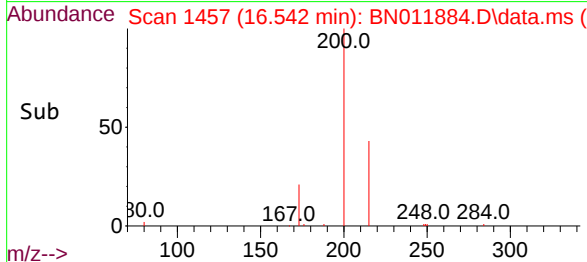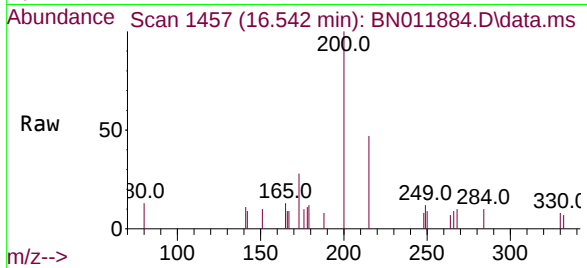

#24
Pentachlorophenol
Concen: 0.22 ng
RT: 16.725 min Scan# 1472
Delta R.T. 0.012 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:266 Resp: 830
Ion Ratio Lower Upper
266 100
264 56.5 51.2 76.8
268 57.5 52.4 78.6


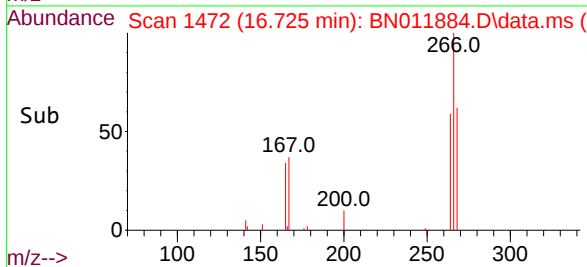

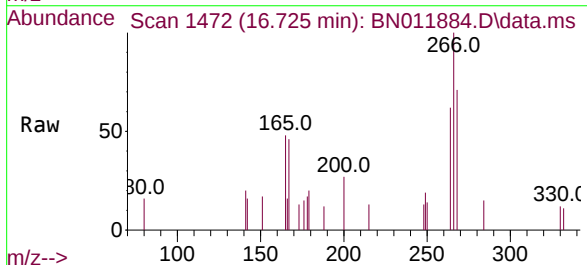


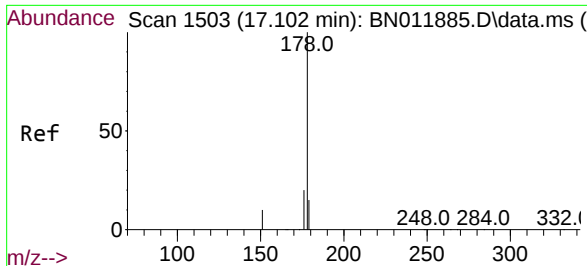

#25
Phenanthrene
Concen: 0.18 ng
RT: 17.102 min Scan# 1503
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:178 Resp: 7507
Ion Ratio Lower Upper
178 100
176 19.2 15.1 22.7
179 15.9 12.3 18.5

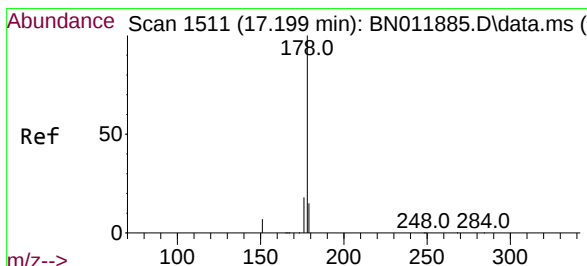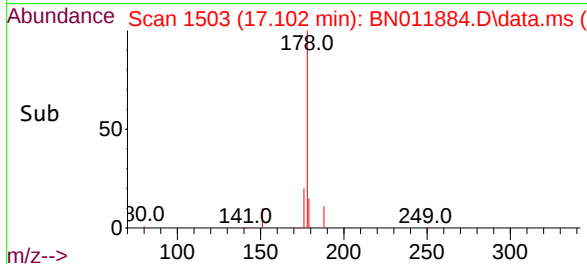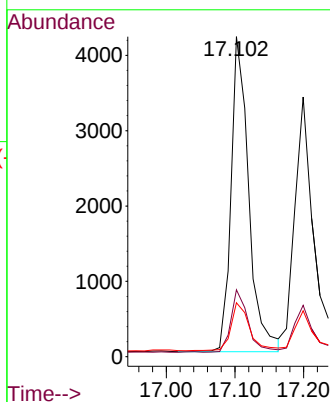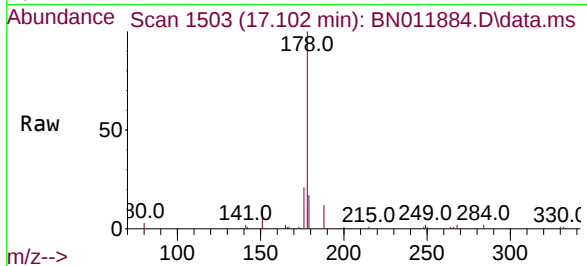

#26
Anthracene
Concen: 0.18 ng
RT: 17.199 min Scan# 1511
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:178 Resp: 6440
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.1 12.4 18.6


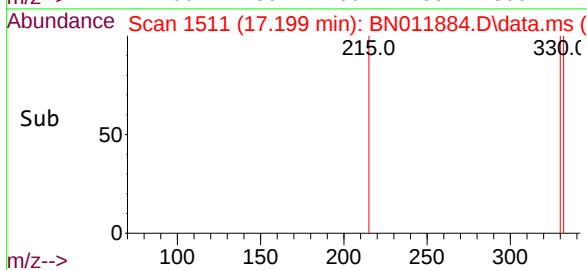

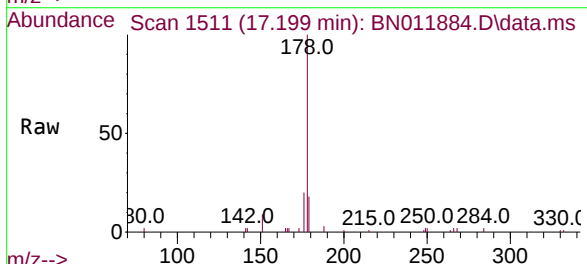




#27
Fluoranthene-d10
Concen: 0.18 ng
RT: 19.102 min Scan# 1797
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:212 Resp: 7388
Ion Ratio Lower Upper
212 100
106 14.2 6.4 9.6#
104 8.7 3.9 5.9#

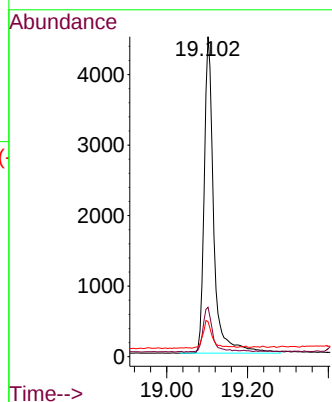

#28
Fluoranthene
Concen: 0.18 ng
RT: 19.132 min Scan# 1803
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:202 Resp: 8463
Ion Ratio Lower Upper
202 100
101 13.0 5.4 8.2#
203 16.8 13.8 20.6

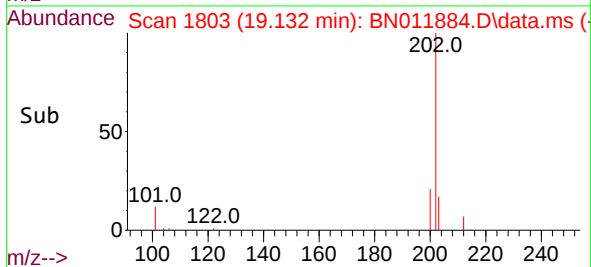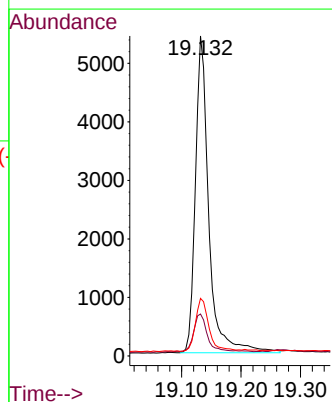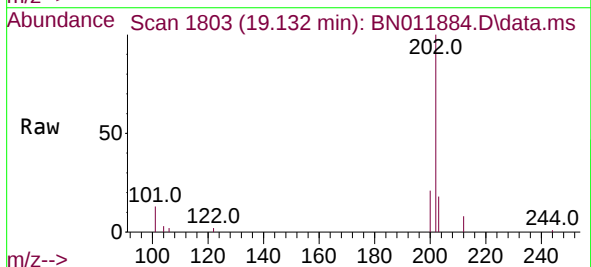



#29

Chrysene-d12

Concen: 0.40 ng

RT: 21.269 min Scan# 2098

Delta R.T. 0.000 min

Lab File: BN011884.D

Acq: 23 Sep 2020 15:10

Tgt Ion:240 Resp: 11661

Ion Ratio Lower Upper

240 100

120 12.3 3.5 5.3#





236 27.3 20.5 30.7

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.2



#30

Pyrene

Concen: 0.22 ng

RT: 19.499 min Scan# 1877

Delta R.T. 0.005 min

Lab File: BN011884.D

Acq: 23 Sep 2020 15:10




Tgt Ion:202 Resp: 8826


Ion Ratio Lower Upper

202 100

200 20.8 16.5 24.7

203 17.4 13.9 20.9



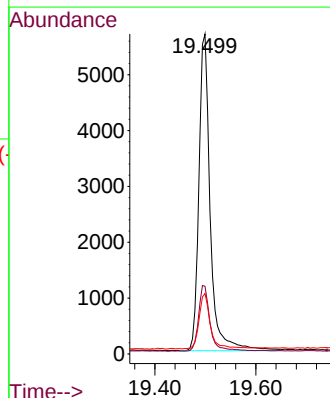





#31
 Terphenyl-d14
 Concen: 0.20 ng
 RT: 19.708 min Scan# 1919
 Delta R.T. 0.000 min
 Lab File: BN011884.D
 Acq: 23 Sep 2020 15:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:244 Resp: 5404
 Ion Ratio Lower Upper
 244 100
 212 10.4 7.3 10.9
 122 17.0 7.8 11.6#



#32
 Benzo(a)anthracene
 Concen: 0.18 ng
 RT: 21.248 min Scan# 2096
 Delta R.T. 0.000 min
 Lab File: BN011884.D
 Acq: 23 Sep 2020 15:10

Tgt Ion:228 Resp: 7166
 Ion Ratio Lower Upper
 228 100
 226 27.6 21.0 31.4
 229 19.9 16.0 24.0


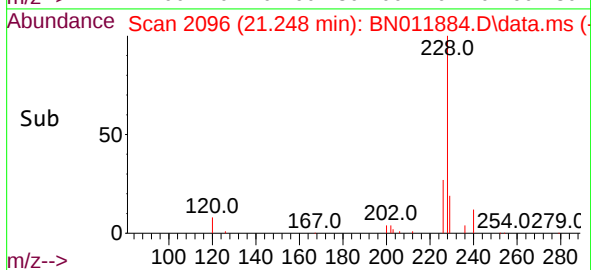




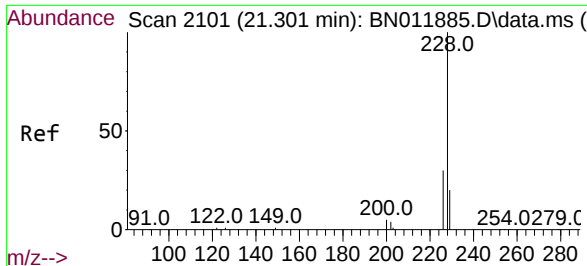

#33
Chrysene
Concen: 0.20 ng
RT: 21.301 min Scan# 2101
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	228	Resp:	8016
Ion Ratio	Lower	Upper	
228	100		
226	30.2	23.3	34.9
229	20.3	15.8	23.8

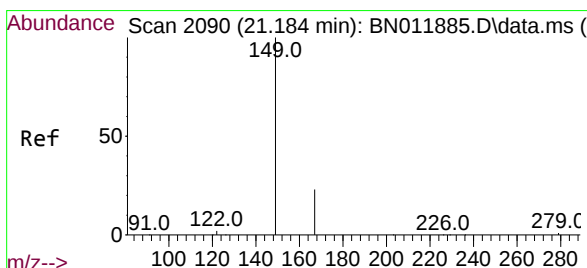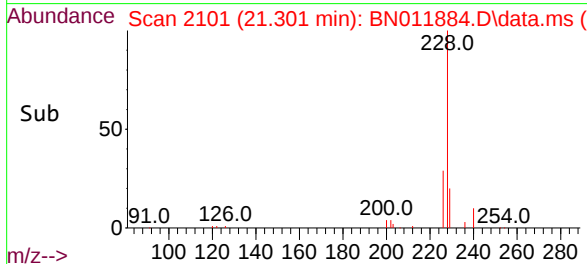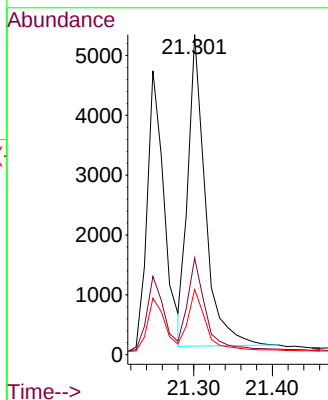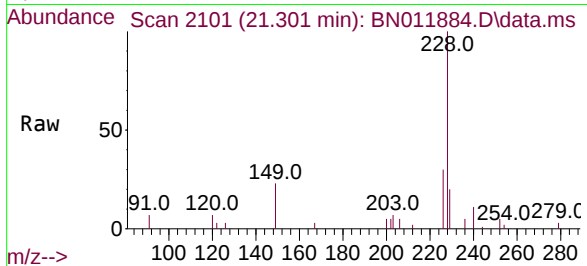

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.26 ng
RT: 21.195 min Scan# 2091
Delta R.T. 0.011 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:	149	Resp:	5341
Ion Ratio	Lower	Upper	
149	100		
167	25.0	23.6	35.4
279	4.6	4.0	6.0


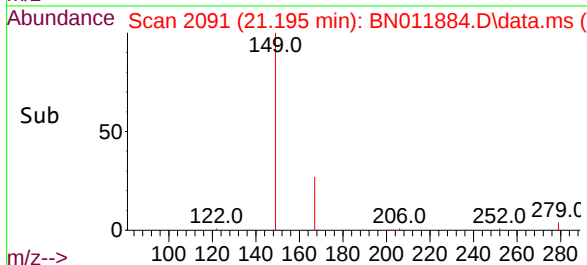
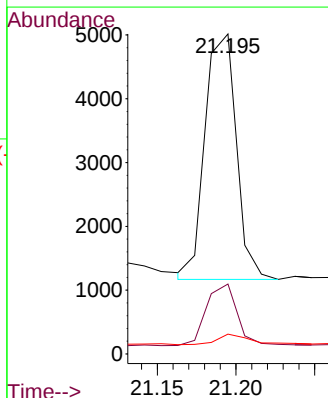
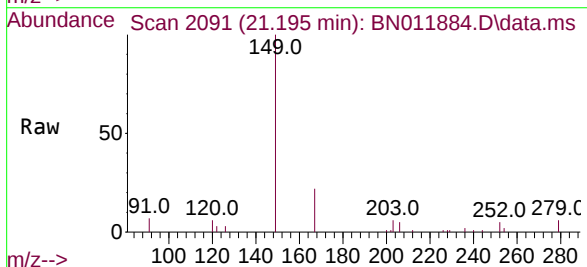




#35
Indeno(1,2,3-cd)pyrene
Concen: 0.18 ng
RT: 25.712 min Scan# 3171
Delta R.T. 0.007 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:276 Resp: 9353
Ion Ratio Lower Upper
276 100
138 26.3 13.0 19.4#
277 23.1 20.0 30.0



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.487 min Scan# 2521
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:264 Resp: 11825
Ion Ratio Lower Upper
264 100
260 25.3 19.6 29.4
265 72.9 38.6 58.0#


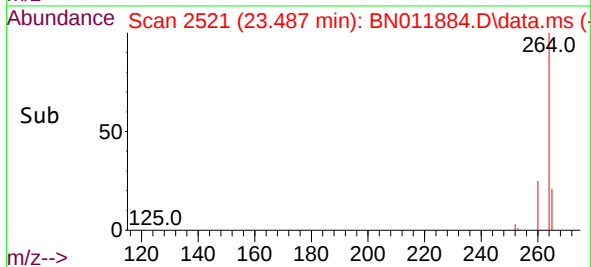

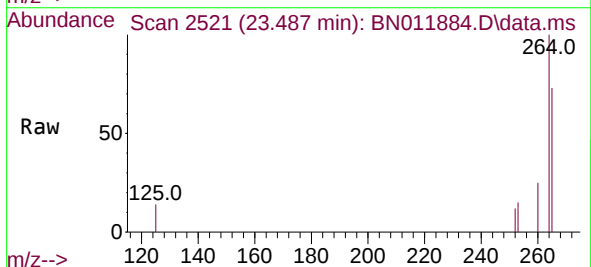




#37
Benzo(b)fluoranthene
Concen: 0.17 ng
RT: 22.823 min Scan# 2327
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10




Tgt Ion:252 Resp: 7639
Ion Ratio Lower Upper
252 100
253 34.7 19.1 28.7#
125 26.7 6.2 9.2#


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



#38
Benzo(k)fluoranthene
Concen: 0.19 ng
RT: 22.868 min Scan# 2340
Delta R.T. 0.000 min
Lab File: BN011884.D
Acq: 23 Sep 2020 15:10

Tgt Ion:252 Resp: 8457
Ion Ratio Lower Upper
252 100
253 34.8 19.3 28.9#
125 25.4 6.0 9.0#

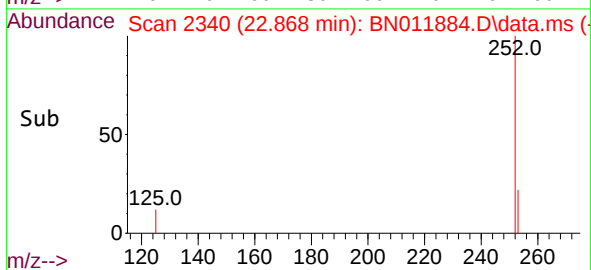



#39

Benzo(a)pyrene

Concen: 0.17 ng

RT: 23.391 min Scan# 2493

Delta R.T. 0.000 min

Lab File: BN011884.D

Acq: 23 Sep 2020 15:10





Tgt Ion:	252	Resp:	6799
Ion Ratio	Lower	Upper	
252	100		
253	39.3	19.8	29.6#
125	34.1	7.3	10.9#

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2

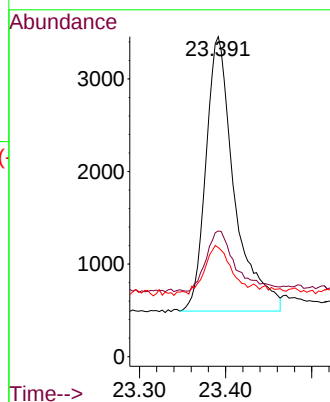

#40

Dibenzo(a,h)anthracene

Concen: 0.17 ng




RT: 25.726 min Scan# 3175


Delta R.T. 0.000 min

Lab File: BN011884.D

Acq: 23 Sep 2020 15:10

Tgt Ion:	278	Resp:	7315
Ion Ratio	Lower	Upper	
278	100		
139	22.2	8.6	13.0#
279	37.2	19.8	29.8#

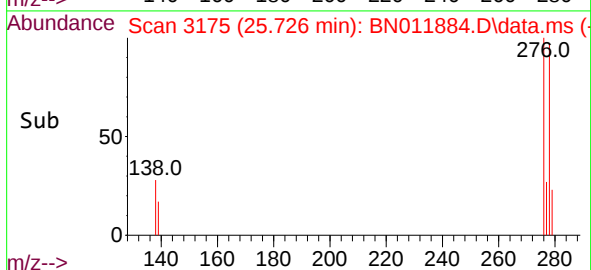

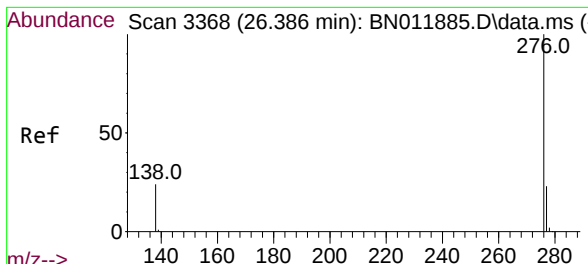

#41
 Benzo(g,h,i)perylene
 Concen: 0.19 ng
 RT: 26.390 min Scan# 3369
 Delta R.T. 0.004 min
 Lab File: BN011884.D
 Acq: 23 Sep 2020 15:10

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	276	Resp:	8563
Ion Ratio	Lower	Upper	
276	100		
277	27.2	19.4	29.0
138	27.0	11.3	16.9#

