

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092320\
 Data File : BN011882.D
 Acq On : 23 Sep 2020 13:57
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Sep 23 18:42:27 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 18:41:41 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.691	152	2810	0.40	ng	0.00
7) Naphthalene-d8	10.466	136	11592	0.40	ng	# 0.00
13) Acenaphthene-d10	14.319	164	5989	0.40	ng	0.00
19) Phenanthrene-d10	17.066	188	12441	0.40	ng	0.00
29) Chrysene-d12	21.269	240	11502	0.40	ng	# 0.00
36) Perylene-d12	23.487	264	11790	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	4433	0.45	ng	0.00
5) Phenol-d6	6.861	99	5437	0.44	ng	0.00
8) Nitrobenzene-d5	8.831	82	5216	0.44	ng	0.00
11) 2-Methylnaphthalene-d10	12.055	152	7656	0.42	ng	0.00
14) 2,4,6-Tribromophenol	15.816	330	1286	0.44	ng	0.00
15) 2-Fluorobiphenyl	12.936	172	9894	0.44	ng	0.00
27) Fluoranthene-d10	19.102	212	15144	0.41	ng	0.00
31) Terphenyl-d14	19.708	244	11549	0.44	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.254	88	2010	0.41	ng	96
3) n-Nitrosodimethylamine	3.560	42	3043	0.43	ng	90
6) bis(2-Chloroethyl)ether	7.119	93	4628	0.44	ng	97
9) Naphthalene	10.516	128	13873	0.42	ng	99
10) Hexachlorobutadiene	10.808	225	2294	0.42	ng	# 99
12) 2-Methylnaphthalene	12.131	142	8895	0.42	ng	96
16) Acenaphthylene	14.040	152	11816	0.41	ng	100
17) Acenaphthene	14.382	154	8070	0.41	ng	90
18) Fluorene	15.372	166	10055	0.42	ng	99
20) 4,6-Dinitro-2-methylph...	15.461	198	882	0.37	ng	# 11
21) 4-Bromophenyl-phenylether	16.262	248	2741	0.42	ng	# 66
22) Hexachlorobenzene	16.372	284	3247	0.42	ng	# 87
23) Atrazine	16.530	200	2564	0.41	ng	# 91
24) Pentachlorophenol	16.725	266	1575	0.42	ng	99
25) Phenanthrene	17.102	178	15702	0.41	ng	98
26) Anthracene	17.199	178	13544	0.41	ng	99
28) Fluoranthene	19.132	202	17577	0.41	ng	# 95
30) Pyrene	19.499	202	18138	0.42	ng	99
32) Benzo(a)anthracene	21.248	228	15047	0.41	ng	98
33) Chrysene	21.301	228	16614	0.42	ng	99
34) Bis(2-ethylhexyl)phtha...	21.184	149	10366	0.40	ng	# 92
35) Indeno(1,2,3-cd)pyrene	25.709	276	19924	0.44	ng	# 91
37) Benzo(b)fluoranthene	22.823	252	16076	0.40	ng	# 83
38) Benzo(k)fluoranthene	22.864	252	17865	0.41	ng	# 87
39) Benzo(a)pyrene	23.391	252	15757	0.42	ng	# 73
40) Dibenzo(a,h)anthracene	25.729	278	16235	0.42	ng	# 87
41) Benzo(g,h,i)perylene	26.386	276	17658	0.42	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092320\
Data File : BN011882.D
Acq On : 23 Sep 2020 13:57
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Sep 23 18:42:27 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 18:41:41 2020
Response via : Initial Calibration








#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.691 min Scan# 585
Delta R.T. -0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 2810
Ion Ratio Lower Upper
152 100
150 157.0 118.3 177.5
115 73.2 51.3 76.9



#2
1,4-Dioxane
Concen: 0.41 ng
RT: 3.254 min Scan# 34
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion: 88 Resp: 2010
Ion Ratio Lower Upper
88 100
58 82.9 63.3 94.9
43 42.9 33.0 49.4







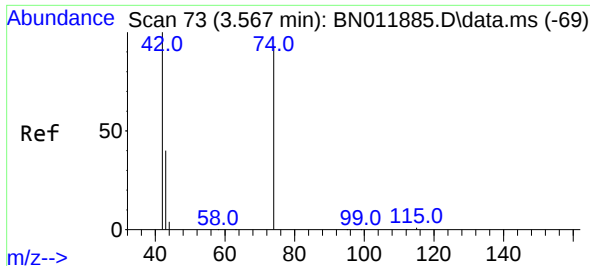

#3
n-Nitrosodimethylamine
Concen: 0.43 ng
RT: 3.560 min Scan# 72
Delta R.T. -0.007 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 42 Resp: 3043
Ion Ratio Lower Upper
42 100
74 89.9 64.4 96.6
44 9.6 6.7 10.1

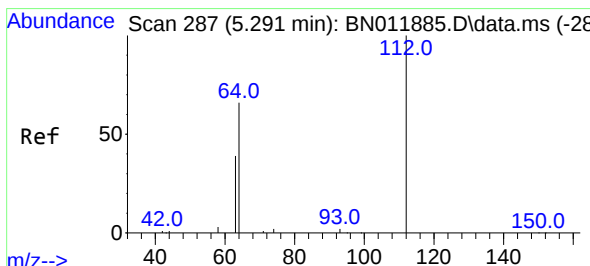

#4
2-Fluorophenol
Concen: 0.45 ng
RT: 5.291 min Scan# 287
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion: 112 Resp: 4433
Ion Ratio Lower Upper
112 100
64 68.4 49.0 73.6
63 41.1 31.8 47.6








#5
Phenol-d6
Concen: 0.44 ng
RT: 6.861 min Scan# 482
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	5437
Ion	Ratio	Lower	Upper
99	100		
42	30.6	23.4	35.0
71	45.2	38.1	57.1



#6
bis(2-Chloroethyl)ether
Concen: 0.44 ng
RT: 7.119 min Scan# 514
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:	93	Resp:	4628
Ion	Ratio	Lower	Upper
93	100		
63	79.1	61.1	91.7
95	29.9	25.5	38.3









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.466 min Scan# 832
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	11592
Ion	Ratio	Lower	Upper
136	100		
137	11.7	9.5	14.3
54	7.3	5.6	8.4
68	5.4	3.2	4.8



#8
Nitrobenzene-d5
Concen: 0.44 ng
RT: 8.831 min Scan# 703
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:	82	Resp:	5216
Ion	Ratio	Lower	Upper
82	100		
128	34.3	34.2	51.2
54	60.3	43.1	64.7









#9
Naphthalene
Concen: 0.42 ng
RT: 10.516 min Scan# 836
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	128	Resp:	13873
Ion	Ratio	Lower	Upper
128	100		
129	11.5	9.7	14.5
127	13.3	11.0	16.4



#10
Hexachlorobutadiene
Concen: 0.42 ng
RT: 10.808 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:	225	Resp:	2294
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.3	51.9	77.9








#11
2-Methylnaphthalene-d10
Concen: 0.42 ng
RT: 12.055 min Scan# 1036
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 7656
Ion Ratio Lower Upper
152 100
151 20.0 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.42 ng
RT: 12.131 min Scan# 1053
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:142 Resp: 8895
Ion Ratio Lower Upper
142 100
141 90.7 70.0 105.0
115 47.1 35.8 53.6









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.319 min Scan# 1280
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	164	Resp:	5989
Ion	Ratio	Lower	Upper
164	100		
162	102.8	83.6	125.4
160	48.5	41.2	61.8



#14
2,4,6-Tribromophenol
Concen: 0.44 ng
RT: 15.816 min Scan# 1398
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:	330	Resp:	1286
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	50.8	33.7	50.5









#15
2-Fluorobiphenyl
Concen: 0.44 ng
RT: 12.936 min Scan# 1171
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	172	Resp:	9894
Ion	Ratio	Lower	Upper
172	100		
171	36.6	27.4	41.2
170	25.0	17.8	26.6



#16
Acenaphthylene
Concen: 0.41 ng
RT: 14.040 min Scan# 1258
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:	152	Resp:	11816
Ion	Ratio	Lower	Upper
152	100		
151	19.7	15.9	23.9
153	13.1	10.5	15.7









#17
Acenaphthene
Concen: 0.41 ng
RT: 14.382 min Scan# 1285
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:154 Resp: 8070
Ion Ratio Lower Upper
154 100
153 116.5 83.4 125.2
152 58.8 42.8 64.2



#18
Fluorene
Concen: 0.42 ng
RT: 15.372 min Scan# 1363
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:166 Resp: 10055
Ion Ratio Lower Upper
166 100
165 99.4 78.8 118.2
167 13.4 11.2 16.8









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.066 min Scan# 1500
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:188 Resp: 12441
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.3 7.7 11.5



#20
4,6-Dinitro-2-methylphenol
Concen: 0.37 ng
RT: 15.461 min Scan# 1370
Delta R.T. 0.013 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:198 Resp: 882
Ion Ratio Lower Upper
198 100
51 142.8 45.0 67.4#
105 66.1 30.4 45.6#









#21
4-Bromophenyl-phenylether
Concen: 0.42 ng
RT: 16.262 min Scan# 1434
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 2741
Ion Ratio Lower Upper
248 100
250 94.7 82.7 124.1
141 102.1 33.7 50.5#



#22
Hexachlorobenzene
Concen: 0.42 ng
RT: 16.372 min Scan# 1443
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:284 Resp: 3247
Ion Ratio Lower Upper
284 100
142 55.2 32.4 48.6#
249 32.8 26.8 40.2







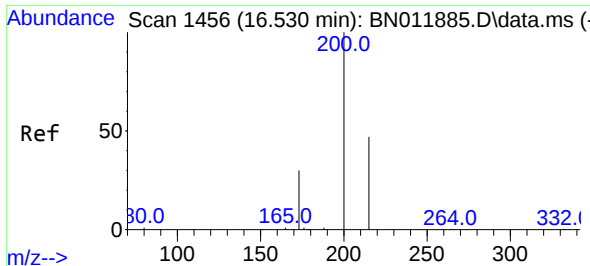

#23
Atrazine
Concen: 0.41 ng
RT: 16.530 min Scan# 1456
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:200 Resp: 2564
Ion Ratio Lower Upper
200 100
173 32.9 18.7 28.1#
215 47.4 40.2 60.4

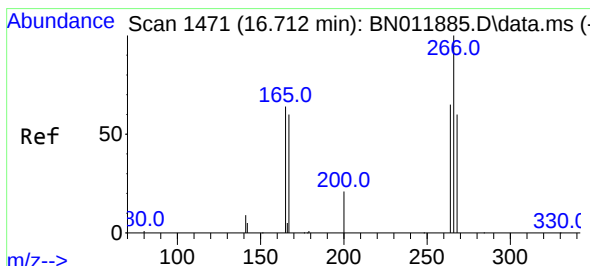

#24
Pentachlorophenol
Concen: 0.42 ng
RT: 16.725 min Scan# 1472
Delta R.T. 0.012 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:266 Resp: 1575
Ion Ratio Lower Upper
266 100
264 63.0 51.2 76.8
268 65.4 52.4 78.6








#25
Phenanthrene
Concen: 0.41 ng
RT: 17.102 min Scan# 1503
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	178	Resp:	15702
Ion	Ratio	Lower	Upper
178	100		
176	19.9	15.1	22.7
179	15.1	12.3	18.5



#26
Anthracene
Concen: 0.41 ng
RT: 17.199 min Scan# 1511
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:	178	Resp:	13544
Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.6	21.8
179	15.7	12.4	18.6









#27
Fluoranthene-d10
Concen: 0.41 ng
RT: 19.102 min Scan# 1797
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:212 Resp: 15144
Ion Ratio Lower Upper
212 100
106 13.6 6.4 9.6#
104 8.2 3.9 5.9#



#28
Fluoranthene
Concen: 0.41 ng
RT: 19.132 min Scan# 1803
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:202 Resp: 17577
Ion Ratio Lower Upper
202 100
101 12.3 5.4 8.2#
203 16.9 13.8 20.6








#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.269 min Scan# 2098
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 11502
Ion Ratio Lower Upper
240 100
120 11.5 3.5 5.3#
236 27.4 20.5 30.7



#30
Pyrene
Concen: 0.42 ng
RT: 19.499 min Scan# 1877
Delta R.T. 0.005 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:202 Resp: 18138
Ion Ratio Lower Upper
202 100
200 20.9 16.5 24.7
203 17.7 13.9 20.9









#31
 Terphenyl-d14
 Concen: 0.44 ng
 RT: 19.708 min Scan# 1919
 Delta R.T. 0.000 min
 Lab File: BN011882.D
 Acq: 23 Sep 2020 13:57




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:244	Resp:	11549
Ion Ratio	Lower	Upper
244	100	
212	9.4	7.3 10.9
122	15.1	7.8 11.6#



#32
 Benzo(a)anthracene
 Concen: 0.41 ng
 RT: 21.248 min Scan# 2096
 Delta R.T. 0.000 min
 Lab File: BN011882.D
 Acq: 23 Sep 2020 13:57

Tgt Ion:228	Resp:	15047
Ion Ratio	Lower	Upper
228	100	
226	27.8	21.0 31.4
229	20.0	16.0 24.0









#33
Chrysene
Concen: 0.42 ng
RT: 21.301 min Scan# 2101
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	228	Resp:	16614
Ion Ratio	Lower	Upper	
228	100		
226	30.1	23.3	34.9
229	20.0	15.8	23.8

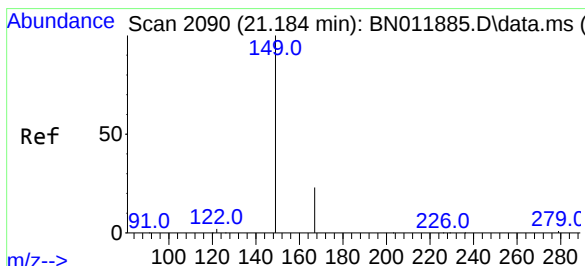

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.40 ng
RT: 21.184 min Scan# 2090
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:	149	Resp:	10366
Ion Ratio	Lower	Upper	
149	100		
167	24.7	23.6	35.4
279	3.2	4.0	6.0#









#35
Indeno(1,2,3-cd)pyrene
Concen: 0.44 ng
RT: 25.709 min Scan# 3170
Delta R.T. 0.004 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 19924
Ion Ratio Lower Upper
276 100
138 25.3 13.0 19.4#
277 24.5 20.0 30.0



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.487 min Scan# 2521
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:264 Resp: 11790
Ion Ratio Lower Upper
264 100
260 24.2 19.6 29.4
265 74.9 38.6 58.0#









#37
Benzo(b)fluoranthene
Concen: 0.40 ng
RT: 22.823 min Scan# 2327
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 16076
Ion Ratio Lower Upper
252 100
253 28.4 19.1 28.7
125 22.5 6.2 9.2#



#38
Benzo(k)fluoranthene
Concen: 0.41 ng
RT: 22.864 min Scan# 2339
Delta R.T. -0.003 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:252 Resp: 17865
Ion Ratio Lower Upper
252 100
253 28.1 19.3 28.9
125 18.2 6.0 9.0#









#39
Benzo(a)pyrene
Concen: 0.42 ng
RT: 23.391 min Scan# 2493
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 15757
Ion Ratio Lower Upper
252 100
253 31.0 19.8 29.6#
125 33.2 7.3 10.9#



#40
Dibenzo(a,h)anthracene
Concen: 0.42 ng
RT: 25.729 min Scan# 3176
Delta R.T. 0.004 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57


Tgt Ion:278 Resp: 16235
Ion Ratio Lower Upper
278 100
139 19.8 8.6 13.0#
279 29.3 19.8 29.8





#41
Benzo(g,h,i)perylene
Concen: 0.42 ng
RT: 26.386 min Scan# 3368
Delta R.T. 0.000 min
Lab File: BN011882.D
Acq: 23 Sep 2020 13:57

Tgt Ion:	276	Resp:	17658
Ion	Ratio	Lower	Upper
276	100		
277	24.4	19.4	29.0
138	25.7	11.3	16.9#



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4