

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092320\
 Data File : BN011889.D
 Acq On : 23 Sep 2020 18:09
 Operator : CG/JU
 Sample : SSTDIC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC5.0

Quant Time: Sep 23 18:37:41 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 18:06:44 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.691	152	3209	0.40	ng	0.00
7) Naphthalene-d8	10.466	136	13844	0.40	ng	0.00
13) Acenaphthene-d10	14.319	164	7342	0.40	ng	0.00
19) Phenanthrene-d10	17.066	188	14545	0.40	ng	0.00
29) Chrysene-d12	21.259	240	14787	0.40	ng	#-0.01
36) Perylene-d12	23.480	264	14167	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	54735	5.77	ng	0.00
5) Phenol-d6	6.853	99	75260	6.47	ng	0.00
8) Nitrobenzene-d5	8.831	82	74942	5.37	ng	0.00
11) 2-Methylnaphthalene-d10	12.056	152	108532	4.42	ng	0.00
14) 2,4,6-Tribromophenol	15.816	330	18010	4.82	ng	0.00
15) 2-Fluorobiphenyl	12.936	172	134164	4.22	ng	0.00
27) Fluoranthene-d10	19.102	212	213644	4.63	ng	0.00
31) Terphenyl-d14	19.703	244	155873	4.62	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.245	88	26231	5.51	ng	97
3) n-Nitrosodimethylamine	3.552	42	43068	6.76	ng	# 88
6) bis(2-Chloroethyl)ether	7.119	93	61617	6.02	ng	91
9) Naphthalene	10.504	128	189724	4.87	ng	98
10) Hexachlorobutadiene	10.808	225	29632	3.30	ng	# 98
12) 2-Methylnaphthalene	12.127	142	124434	4.63	ng	98
16) Acenaphthylene	14.040	152	182888	5.16	ng	99
17) Acenaphthene	14.382	154	124195	5.04	ng	98
18) Fluorene	15.372	166	144435	4.70	ng	100
20) 4,6-Dinitro-2-methylph...	15.448	198	16218	6.52	ng	# 83
21) 4-Bromophenyl-phenylether	16.262	248	38676	4.47	ng	# 79
22) Hexachlorobenzene	16.372	284	42955	4.02	ng	# 84
23) Atrazine	16.530	200	38328	4.93	ng	91
24) Pentachlorophenol	16.713	266	22452	5.20	ng	98
25) Phenanthrene	17.102	178	222760	4.84	ng	99
26) Anthracene	17.199	178	208553	5.22	ng	99
28) Fluoranthene	19.132	202	249354	4.63	ng	# 95
30) Pyrene	19.494	202	254807	4.94	ng	100
32) Benzo(a)anthracene	21.248	228	238161	4.76	ng	99
33) Chrysene	21.301	228	241286	4.69	ng	99
34) Bis(2-ethylhexyl)phtha...	21.184	149	166660	6.47	ng	# 91
35) Indeno(1,2,3-cd)pyrene	25.702	276	287531	4.48	ng	# 89
37) Benzo(b)fluoranthene	22.813	252	245482	4.65	ng	# 94
38) Benzo(k)fluoranthene	22.857	252	248719	4.56	ng	# 94
39) Benzo(a)pyrene	23.381	252	226354	4.81	ng	# 93
40) Dibenzo(a,h)anthracene	25.712	278	235917	4.55	ng	# 92
41) Benzo(g,h,i)perylene	26.376	276	242582	4.39	ng	# 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092320\
Data File : BN011889.D
Acq On : 23 Sep 2020 18:09
Operator : CG/JU
Sample : SSTDIC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Sep 23 18:37:41 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 18:06:44 2020
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.691 min Scan# 585
 Delta R.T. -0.000 min
 Lab File: BN011889.D
 Acq: 23 Sep 2020 18:09

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:152 Resp: 3209




Ion	Ratio	Lower	Upper
152	100		
150	154.1	118.3	177.5
115	70.9	51.3	76.9




#2
 1,4-Dioxane
 Concen: 5.51 ng
 RT: 3.245 min Scan# 33
 Delta R.T. -0.008 min
 Lab File: BN011889.D
 Acq: 23 Sep 2020 18:09

Tgt Ion: 88 Resp: 26231

Ion	Ratio	Lower	Upper
88	100		
58	83.5	63.3	94.9
43	41.2	33.0	49.4









#3
n-Nitrosodimethylamine
Concen: 6.76 ng
RT: 3.552 min Scan# 71
Delta R.T. -0.015 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion: 42 Resp: 43068
Ion Ratio Lower Upper
42 100
74 91.8 64.4 96.6
44 5.5 6.7 10.1#



#4
2-Fluorophenol
Concen: 5.77 ng
RT: 5.291 min Scan# 287
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion: 112 Resp: 54735
Ion Ratio Lower Upper
112 100
64 69.3 49.0 73.6
63 41.1 31.8 47.6








#5
Phenol-d6
Concen: 6.47 ng
RT: 6.853 min Scan# 481
Delta R.T. -0.008 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 75260
Ion Ratio Lower Upper
99 100
42 29.5 23.4 35.0
71 45.1 38.1 57.1



#6
bis(2-Chloroethyl)ether
Concen: 6.02 ng
RT: 7.119 min Scan# 514
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion: 93 Resp: 61617
Ion Ratio Lower Upper
93 100
63 87.3 61.1 91.7
95 32.1 25.5 38.3









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.466 min Scan# 832
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	13844
Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.5	14.3
54	6.7	5.6	8.4
68	4.5	3.2	4.8



#8
Nitrobenzene-d5
Concen: 5.37 ng
RT: 8.831 min Scan# 703
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:	82	Resp:	74942
Ion	Ratio	Lower	Upper
82	100		
128	36.3	34.2	51.2
54	53.2	43.1	64.7









#9
Naphthalene
Concen: 4.87 ng
RT: 10.504 min Scan# 835
Delta R.T. -0.012 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:128 Resp: 189724
Ion Ratio Lower Upper
128 100
129 11.0 9.7 14.5
127 13.2 11.0 16.4



#10
Hexachlorobutadiene
Concen: 3.30 ng
RT: 10.808 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:225 Resp: 29632
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.6 51.9 77.9








#11
2-Methylnaphthalene-d10
Concen: 4.42 ng
RT: 12.056 min Scan# 1036
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 108532
Ion Ratio Lower Upper
152 100
151 20.2 16.7 25.1



#12
2-Methylnaphthalene
Concen: 4.63 ng
RT: 12.127 min Scan# 1052
Delta R.T. -0.004 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:142 Resp: 124434
Ion Ratio Lower Upper
142 100
141 89.7 70.0 105.0
115 46.5 35.8 53.6









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.319 min Scan# 1280
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:164 Resp: 7342
Ion Ratio Lower Upper
164 100
162 101.4 83.6 125.4
160 48.3 41.2 61.8



#14
2,4,6-Tribromophenol
Concen: 4.82 ng
RT: 15.816 min Scan# 1398
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:330 Resp: 18010
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 58.5 33.7 50.5#









#15
2-Fluorobiphenyl
Concen: 4.22 ng
RT: 12.936 min Scan# 1171
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	172	Resp:	134164
Ion	Ratio	Lower	Upper
172	100		
171	35.3	27.4	41.2
170	24.2	17.8	26.6



#16
Acenaphthylene
Concen: 5.16 ng
RT: 14.040 min Scan# 1258
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:	152	Resp:	182888
Ion	Ratio	Lower	Upper
152	100		
151	19.6	15.9	23.9
153	12.9	10.5	15.7









#17
Acenaphthene
Concen: 5.04 ng
RT: 14.382 min Scan# 1285
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:154 Resp: 124195
Ion Ratio Lower Upper
154 100
153 106.1 83.4 125.2
152 52.5 42.8 64.2



#18
Fluorene
Concen: 4.70 ng
RT: 15.372 min Scan# 1363
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:166 Resp: 144435
Ion Ratio Lower Upper
166 100
165 98.2 78.8 118.2
167 13.4 11.2 16.8









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.066 min Scan# 1500
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:188	Resp:	14545
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	9.6	11.5



#20
4,6-Dinitro-2-methylphenol
Concen: 6.52 ng
RT: 15.448 min Scan# 1369
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:198	Resp:	16218
Ion Ratio	Lower	Upper
198	100	
51	39.0	45.0
105	33.5	45.6









#21
4-Bromophenyl-phenylether
Concen: 4.47 ng
RT: 16.262 min Scan# 1434
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 38676
Ion Ratio Lower Upper
248 100
250 98.2 82.7 124.1
141 79.9 33.7 50.5#



#22
Hexachlorobenzene
Concen: 4.02 ng
RT: 16.372 min Scan# 1443
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:284 Resp: 42955
Ion Ratio Lower Upper
284 100
142 57.8 32.4 48.6#
249 32.4 26.8 40.2









#23
Atrazine
Concen: 4.93 ng
RT: 16.530 min Scan# 1456
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:200 Resp: 38328
Ion Ratio Lower Upper
200 100
173 27.9 18.7 28.1
215 44.4 40.2 60.4



#24
Pentachlorophenol
Concen: 5.20 ng
RT: 16.713 min Scan# 1471
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:266 Resp: 22452
Ion Ratio Lower Upper
266 100
264 62.9 51.2 76.8
268 63.1 52.4 78.6








#25
Phenanthrene
Concen: 4.84 ng
RT: 17.102 min Scan# 1503
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:178 Resp: 222760
Ion Ratio Lower Upper
178 100
176 19.4 15.1 22.7
179 15.2 12.3 18.5



#26
Anthracene
Concen: 5.22 ng
RT: 17.199 min Scan# 1511
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:178 Resp: 208553
Ion Ratio Lower Upper
178 100
176 18.8 14.6 21.8
179 15.3 12.4 18.6









#27
Fluoranthene-d10
Concen: 4.63 ng
RT: 19.102 min Scan# 1797
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:212 Resp: 213644
Ion Ratio Lower Upper
212 100
106 14.4 6.4 9.6#
104 8.3 3.9 5.9#



#28
Fluoranthene
Concen: 4.63 ng
RT: 19.132 min Scan# 1803
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:202 Resp: 249354
Ion Ratio Lower Upper
202 100
101 12.6 5.4 8.2#
203 17.2 13.8 20.6








#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.259 min Scan# 2097
Delta R.T. -0.010 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 14787
Ion Ratio Lower Upper
240 100
120 12.3 3.5 5.3#
236 26.5 20.5 30.7



#30
Pyrene
Concen: 4.94 ng
RT: 19.494 min Scan# 1876
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:202 Resp: 254807
Ion Ratio Lower Upper
202 100
200 20.9 16.5 24.7
203 17.4 13.9 20.9









#31
Terphenyl-d14
Concen: 4.62 ng
RT: 19.703 min Scan# 1918
Delta R.T. -0.005 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:244 Resp: 155873
Ion Ratio Lower Upper
244 100
212 9.2 7.3 10.9
122 15.4 7.8 11.6#



#32
Benzo(a)anthracene
Concen: 4.76 ng
RT: 21.248 min Scan# 2096
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:228 Resp: 238161
Ion Ratio Lower Upper
228 100
226 25.7 21.0 31.4
229 20.0 16.0 24.0









#33
Chrysene
Concen: 4.69 ng
RT: 21.301 min Scan# 2101
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 241286
Ion Ratio Lower Upper
228 100
226 28.4 23.3 34.9
229 19.9 15.8 23.8

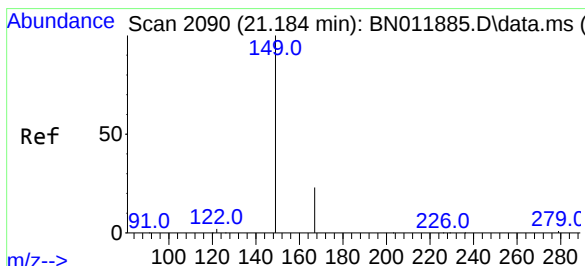

#34
Bis(2-ethylhexyl)phthalate
Concen: 6.47 ng
RT: 21.184 min Scan# 2090
Delta R.T. 0.000 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:149 Resp: 166660
Ion Ratio Lower Upper
149 100
167 24.1 23.6 35.4
279 3.0 4.0 6.0#









#35
Indeno(1,2,3-cd)pyrene
Concen: 4.48 ng
RT: 25.702 min Scan# 3168
Delta R.T. -0.003 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:276 Resp: 287531
Ion Ratio Lower Upper
276 100
138 27.8 13.0 19.4#
277 24.8 20.0 30.0



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.480 min Scan# 2519
Delta R.T. -0.007 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09


Tgt Ion:264 Resp: 14167
Ion Ratio Lower Upper
264 100
260 24.2 19.6 29.4
265 67.0 38.6 58.0#








#37
Benzo(b)fluoranthene
Concen: 4.65 ng
RT: 22.813 min Scan# 2324
Delta R.T. -0.010 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0






Tgt Ion:252 Resp: 245482
Ion Ratio Lower Upper
252 100
253 22.1 19.1 28.7
125 12.4 6.2 9.2#



#38
Benzo(k)fluoranthene
Concen: 4.56 ng
RT: 22.857 min Scan# 2337
Delta R.T. -0.010 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:252 Resp: 248719
Ion Ratio Lower Upper
252 100
253 22.0 19.3 28.9
125 11.9 6.0 9.0#









#39
Benzo(a)pyrene
Concen: 4.81 ng
RT: 23.381 min Scan# 2490
Delta R.T. -0.010 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 226354
Ion Ratio Lower Upper
252 100
253 22.3 19.8 29.6
125 13.7 7.3 10.9#



#40
Dibenzo(a,h)anthracene
Concen: 4.55 ng
RT: 25.712 min Scan# 3171
Delta R.T. -0.013 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Tgt Ion:278 Resp: 235917
Ion Ratio Lower Upper
278 100
139 18.3 8.6 13.0#
279 23.7 19.8 29.8



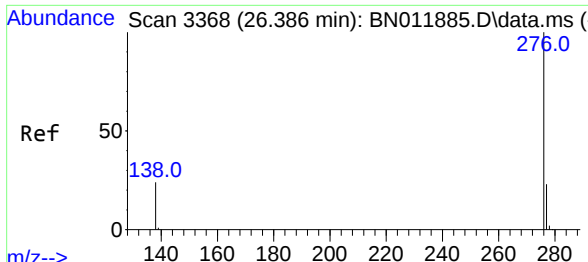

#41
Benzo(g,h,i)perylene
Concen: 4.39 ng
RT: 26.376 min Scan# 3365
Delta R.T. -0.010 min
Lab File: BN011889.D
Acq: 23 Sep 2020 18:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:276 Resp: 242582
Ion Ratio Lower Upper
276 100
277 23.6 19.4 29.0
138 23.9 11.3 16.9#

