
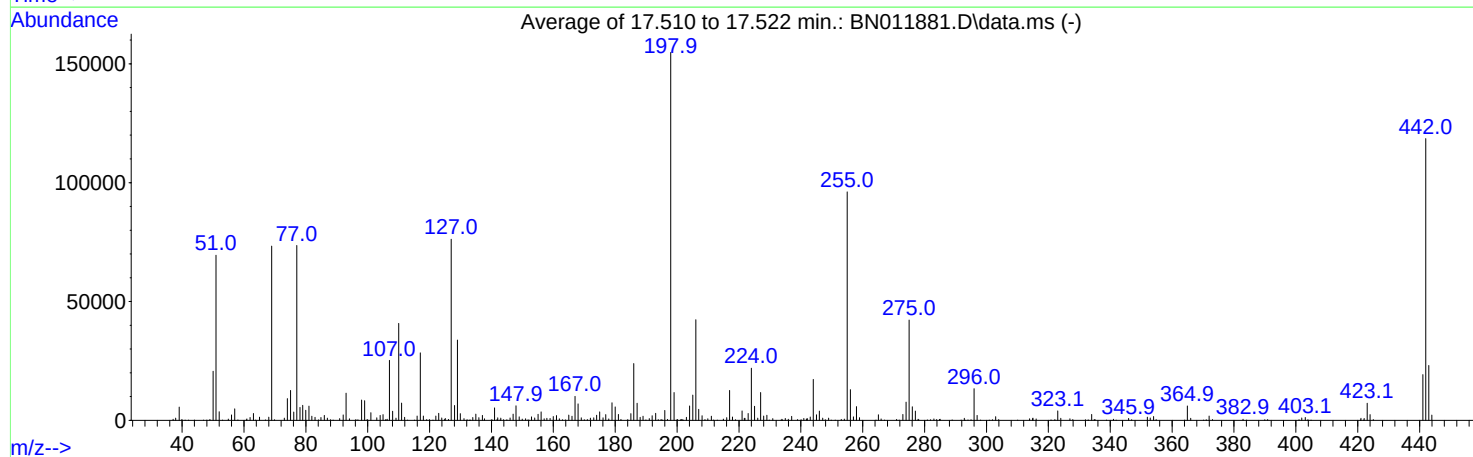


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092320\
 Data File : BN011881.D
 Acq On : 23 Sep 2020 13:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 23 18:41:41 2020

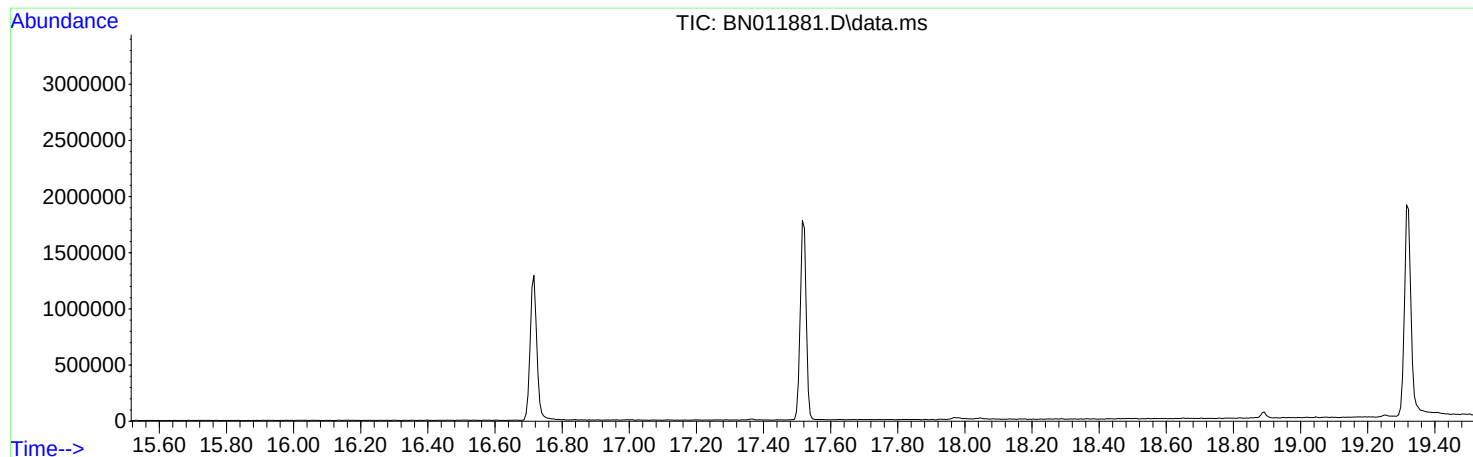

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	69441	PASS
68	69	0.00	2	1.8	1333	PASS
69	198	0.00	100	47.4	73317	PASS
70	69	0.00	2	0.4	297	PASS
127	198	10	80	49.2	76213	PASS
197	198	0.00	2	0.3	391	PASS
198	198	100	100	100.0	154768	PASS
199	198	5	9	7.6	11698	PASS
275	198	10	60	27.3	42221	PASS
365	198	1	100	3.9	6049	PASS
441	198	0.01	100	12.4	19246	PASS
442	198	50	100	76.6	118565	PASS
443	442	15	24	19.5	23114	PASS