

Data File : BN002833.D
Acq On : 24 Sep 2018 18:59
Operator : JU/SJ
Sample : PB113143BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK43

Quant Time: Sep 25 05:44:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 25 05:43:40 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	128379	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	555435	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	321368	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	657469	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	570202	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	544314	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	17654	6.34	ng/uL	0.00
5) Phenol-d5	6.83	99	351368	32.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	228910	33.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	294700	32.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	293786	34.79	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	149572	34.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	172732	35.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	284544	32.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	424123	41.71	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	1060983	42.18	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1282935	39.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	121969	29.32	ng/ul	0.00
57) Fluorene-d10	15.27	176	895232	40.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	138980	33.80	ng/ul	0.00
70) Anthracene-d10	17.13	188	1331414	42.42	ng/ul	0.00
78) Pyrene-d10	19.43	212	1315120	43.71	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	1238986	43.24	ng/ul	0.00


Target Compounds				Qvalue	
15) N-Nitroso-di-n-propylamine	8.35	70	6871	1.051 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN002833.D
Acq On : 24 Sep 2018 18:59
Operator : JU/SJ
Sample : PB113143BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK43

Quant Time: Sep 25 05:44:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 25 05:43:40 2018
Response via : Initial Calibration

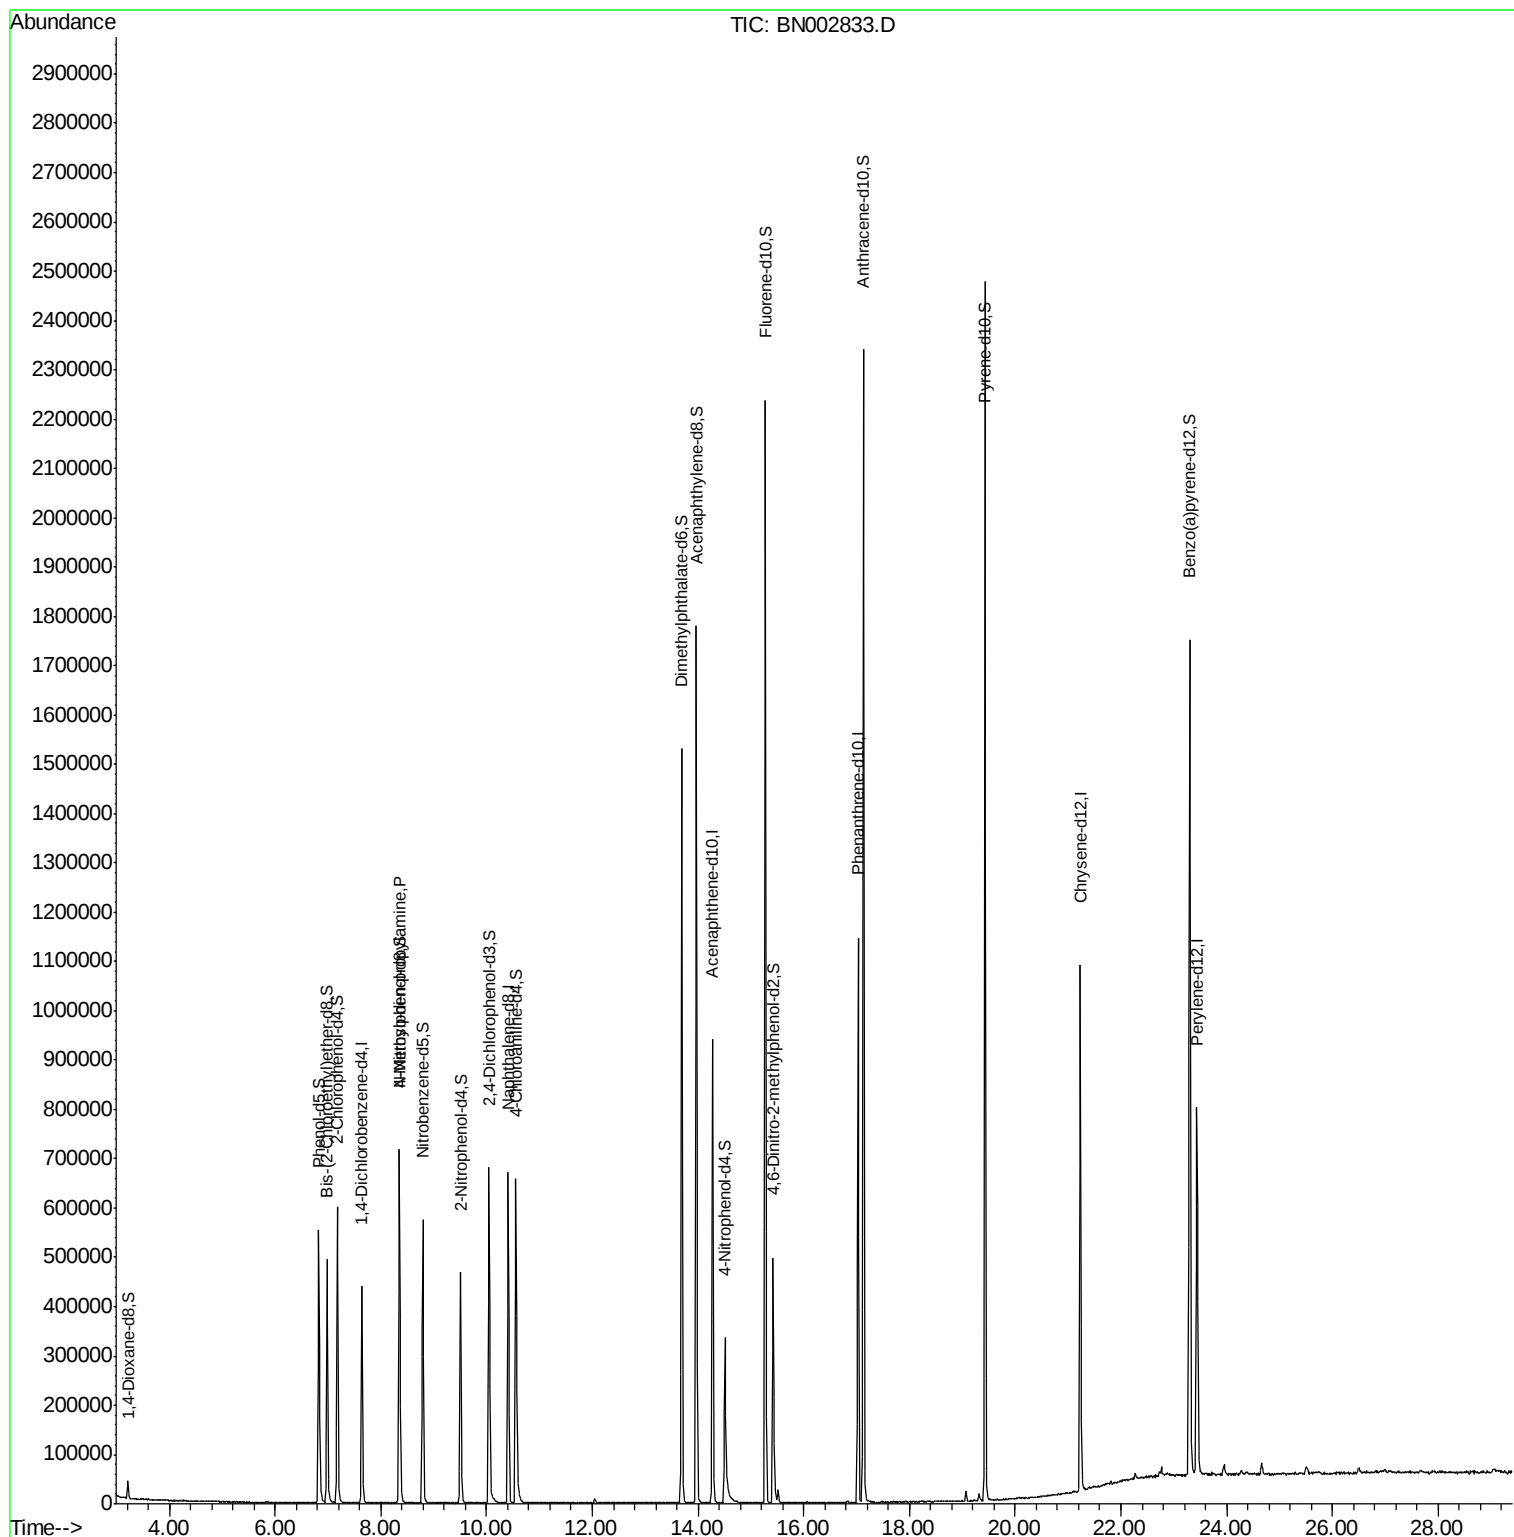

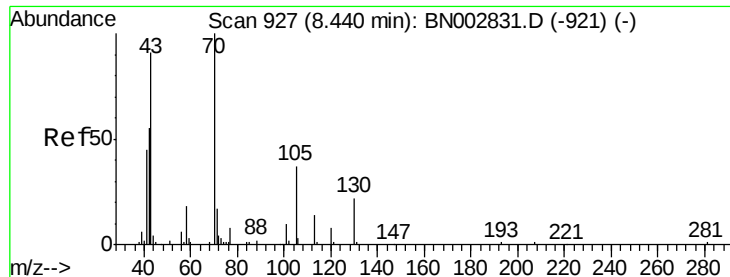

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.051 ng/ul
 RT: 8.35 min Scan# 912
 Delta R.T. -0.09 min
 Lab File: BN002833.D
 Acq: 24 Sep 2018 18:59

Instrument :
 BNA_N
 ClientSampleId :
 SBLK43

Tgt Ion: 70 Resp: 6871
 Ion Ratio Lower Upper
 70 100
 42 362.5 47.7 71.5#
 101 0.0 8.0 12.0#
 130 0.0 16.0 24.0#

