

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092418\
 Data File : BN002842.D
 Acq On : 25 Sep 2018 00:13
 Operator : JU/SJ
 Sample : J5036-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C08W6

Manual Integrations
 APPROVED

Sohil
 9/25/2018 12:07:41 PM

Quant Time: Sep 25 06:10:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 25 05:43:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	138916	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	581393	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	319841	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	651269	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	607868	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	628834	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	18618	6.18	ng/uL	0.00
5) Phenol-d5	6.83	99	96646	8.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	264060	36.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	286965	29.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	176830	19.35	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	171400	38.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	194129	38.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	309957	33.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	8233m	0.77	ng/ul	0.02
43) Dimethylphthalate-d6	13.69	166	988901	39.50	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1278770	39.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	23505m	5.68	ng/ul	0.02
57) Fluorene-d10	15.27	176	862892	39.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	131503	32.28	ng/ul	0.00
70) Anthracene-d10	17.13	188	1236990	39.78	ng/ul	0.00
78) Pyrene-d10	19.43	212	1243044	38.75	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	1310344	39.59	ng/ul	0.00
Target Compounds						
20) Nitrobenzene	8.83	77	261782	25.008	ng/ul	0.79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092418\
Data File : BN002842.D
Acq On : 25 Sep 2018 00:13
Operator : JU/SJ
Sample : J5036-02
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C08W6

Quant Time: Sep 25 06:10:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 25 05:43:40 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
9/25/2018 12:07:41 PM

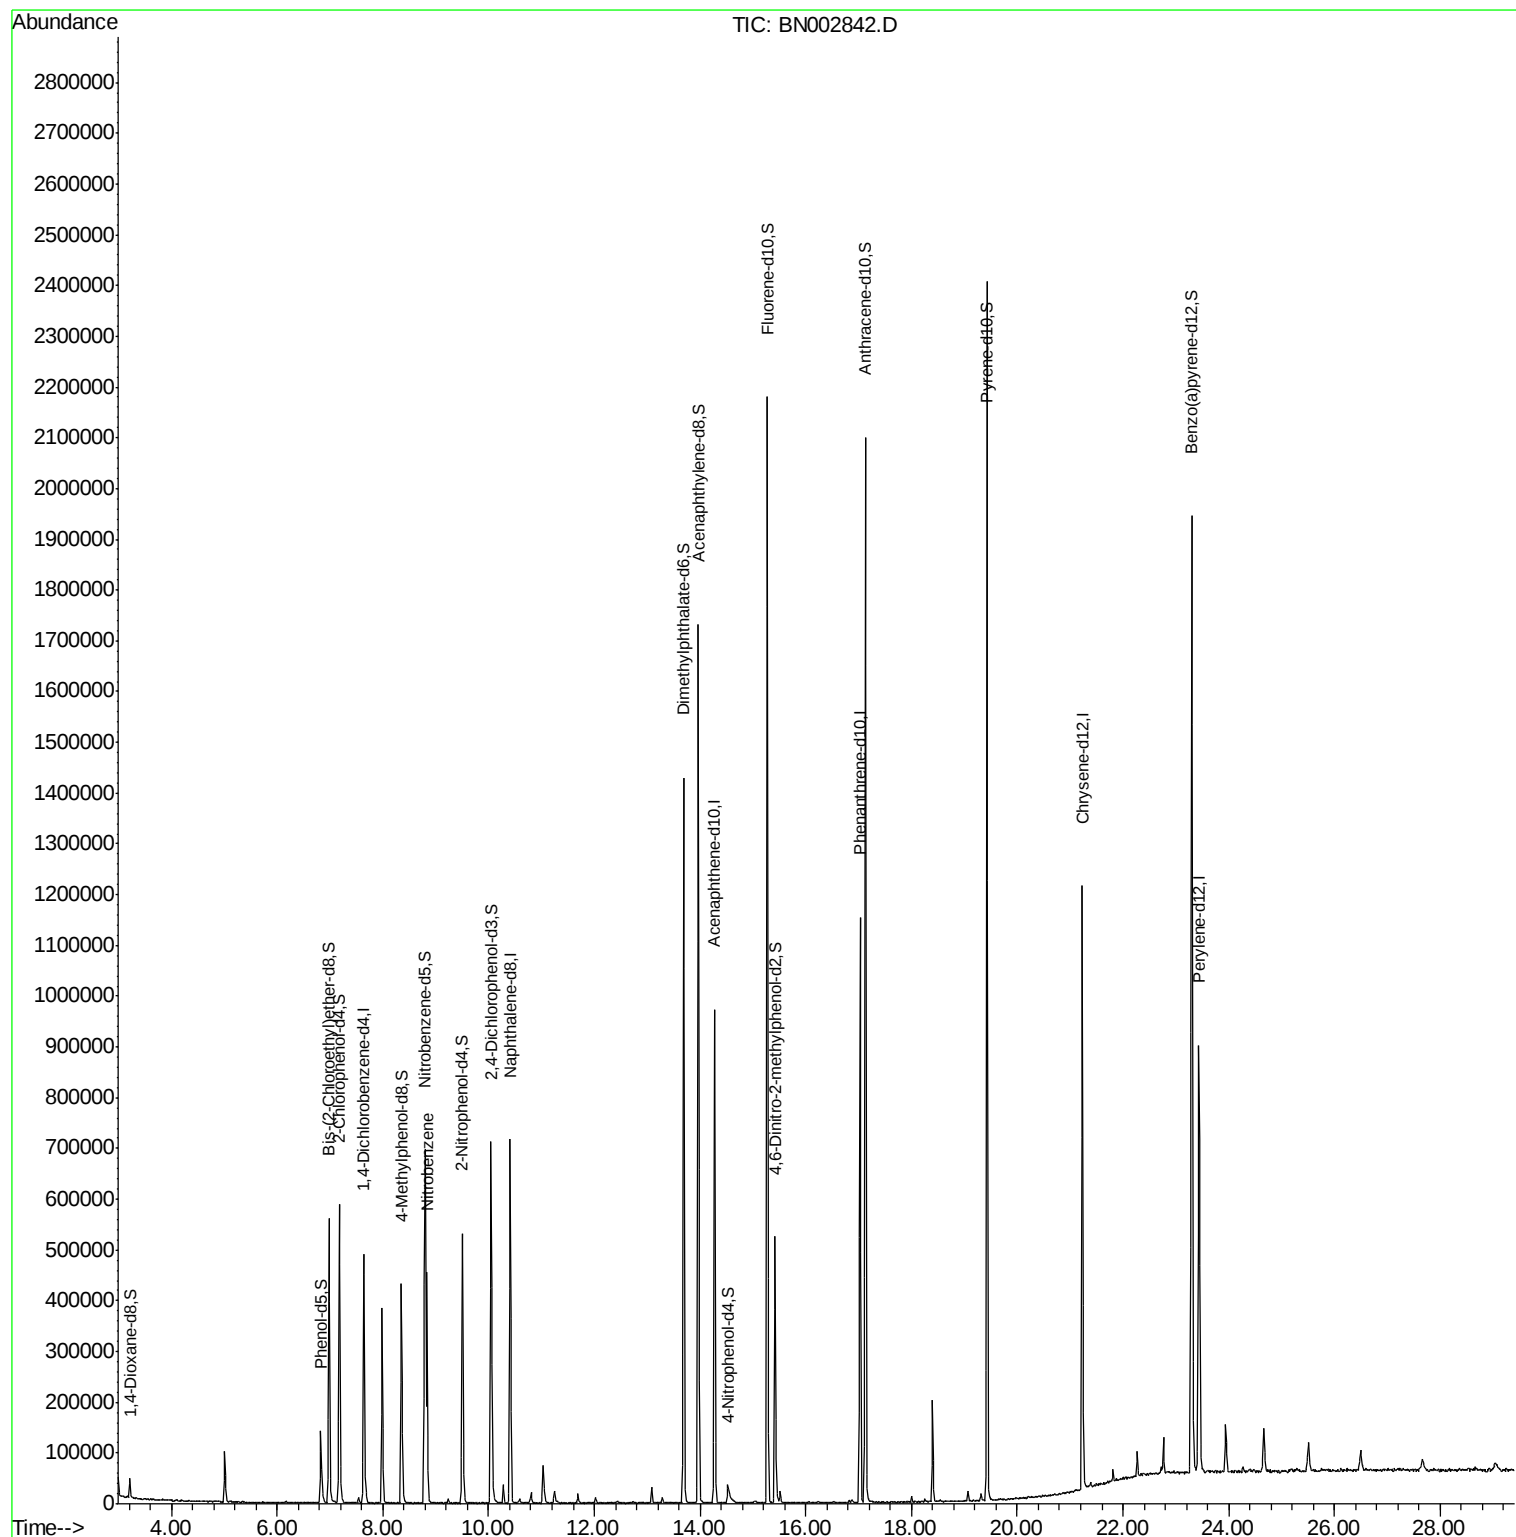

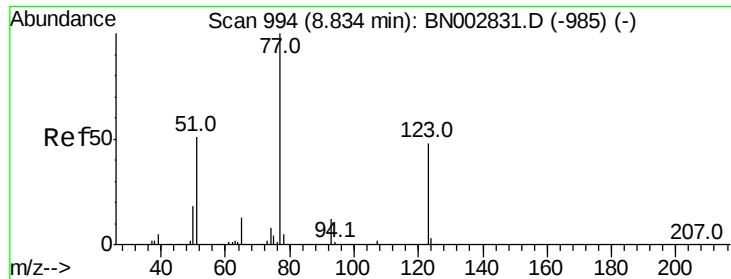

#20
 Nitrobenzene
 Concen: 25.008 ng/ul
 RT: 8.83 min Scan# 994
 Delta R.T. 0.00 min
 Lab File: BN002842.D
 Acq: 25 Sep 2018 00:13

Instrument :
 BNA_N
 ClientSampleId :
 C08W6

Tot Ion	Ratio	Lower	Upper
77	100		
123	47.1	35.8	53.8
65	13.3	11.1	16.7

Manual Integrations
 APPROVED

Sohil
 9/25/2018 12:07:41 PM

