

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092420\
 Data File : BN011925.D
 Acq On : 24 Sep 2020 21:59
 Operator : CG/JU
 Sample : L4083-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE104D1-20200917

Quant Time: Sep 25 01:41:21 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 18:41:41 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.683	152	3915	0.40	ng	0.00
7) Naphthalene-d8	10.453	136	16089	0.40	ng	#-0.01
13) Acenaphthene-d10	14.306	164	8914	0.40	ng	-0.01
19) Phenanthrene-d10	17.053	188	17663	0.40	ng	#-0.01
29) Chrysene-d12	21.259	240	15658	0.40	ng	#-0.01
36) Perylene-d12	23.470	264	15870	0.40	ng	#-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	1302	0.09	ng	0.00
5) Phenol-d6	6.853	99	925	0.05	ng	0.00
8) Nitrobenzene-d5	8.831	82	3987	0.24	ng	0.00
11) 2-Methylnaphthalene-d10	12.051	152	6484	0.25	ng	0.00
14) 2,4,6-Tribromophenol	15.803	330	1007	0.23	ng	-0.01
15) 2-Fluorobiphenyl	12.936	172	8318	0.25	ng	0.00
27) Fluoranthene-d10	19.097	212	15260	0.29	ng	0.00
31) Terphenyl-d14	19.698	244	12713	0.36	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.245	88	19605	2.88	ng	Qvalue 97
34) Bis(2-ethylhexyl)phtha...	21.174	149	1867	0.05	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092420\
Data File : BN011925.D
Acq On : 24 Sep 2020 21:59
Operator : CG/JU
Sample : L4083-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE104D1-20200917

Quant Time: Sep 25 01:41:21 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 18:41:41 2020
Response via : Initial Calibration




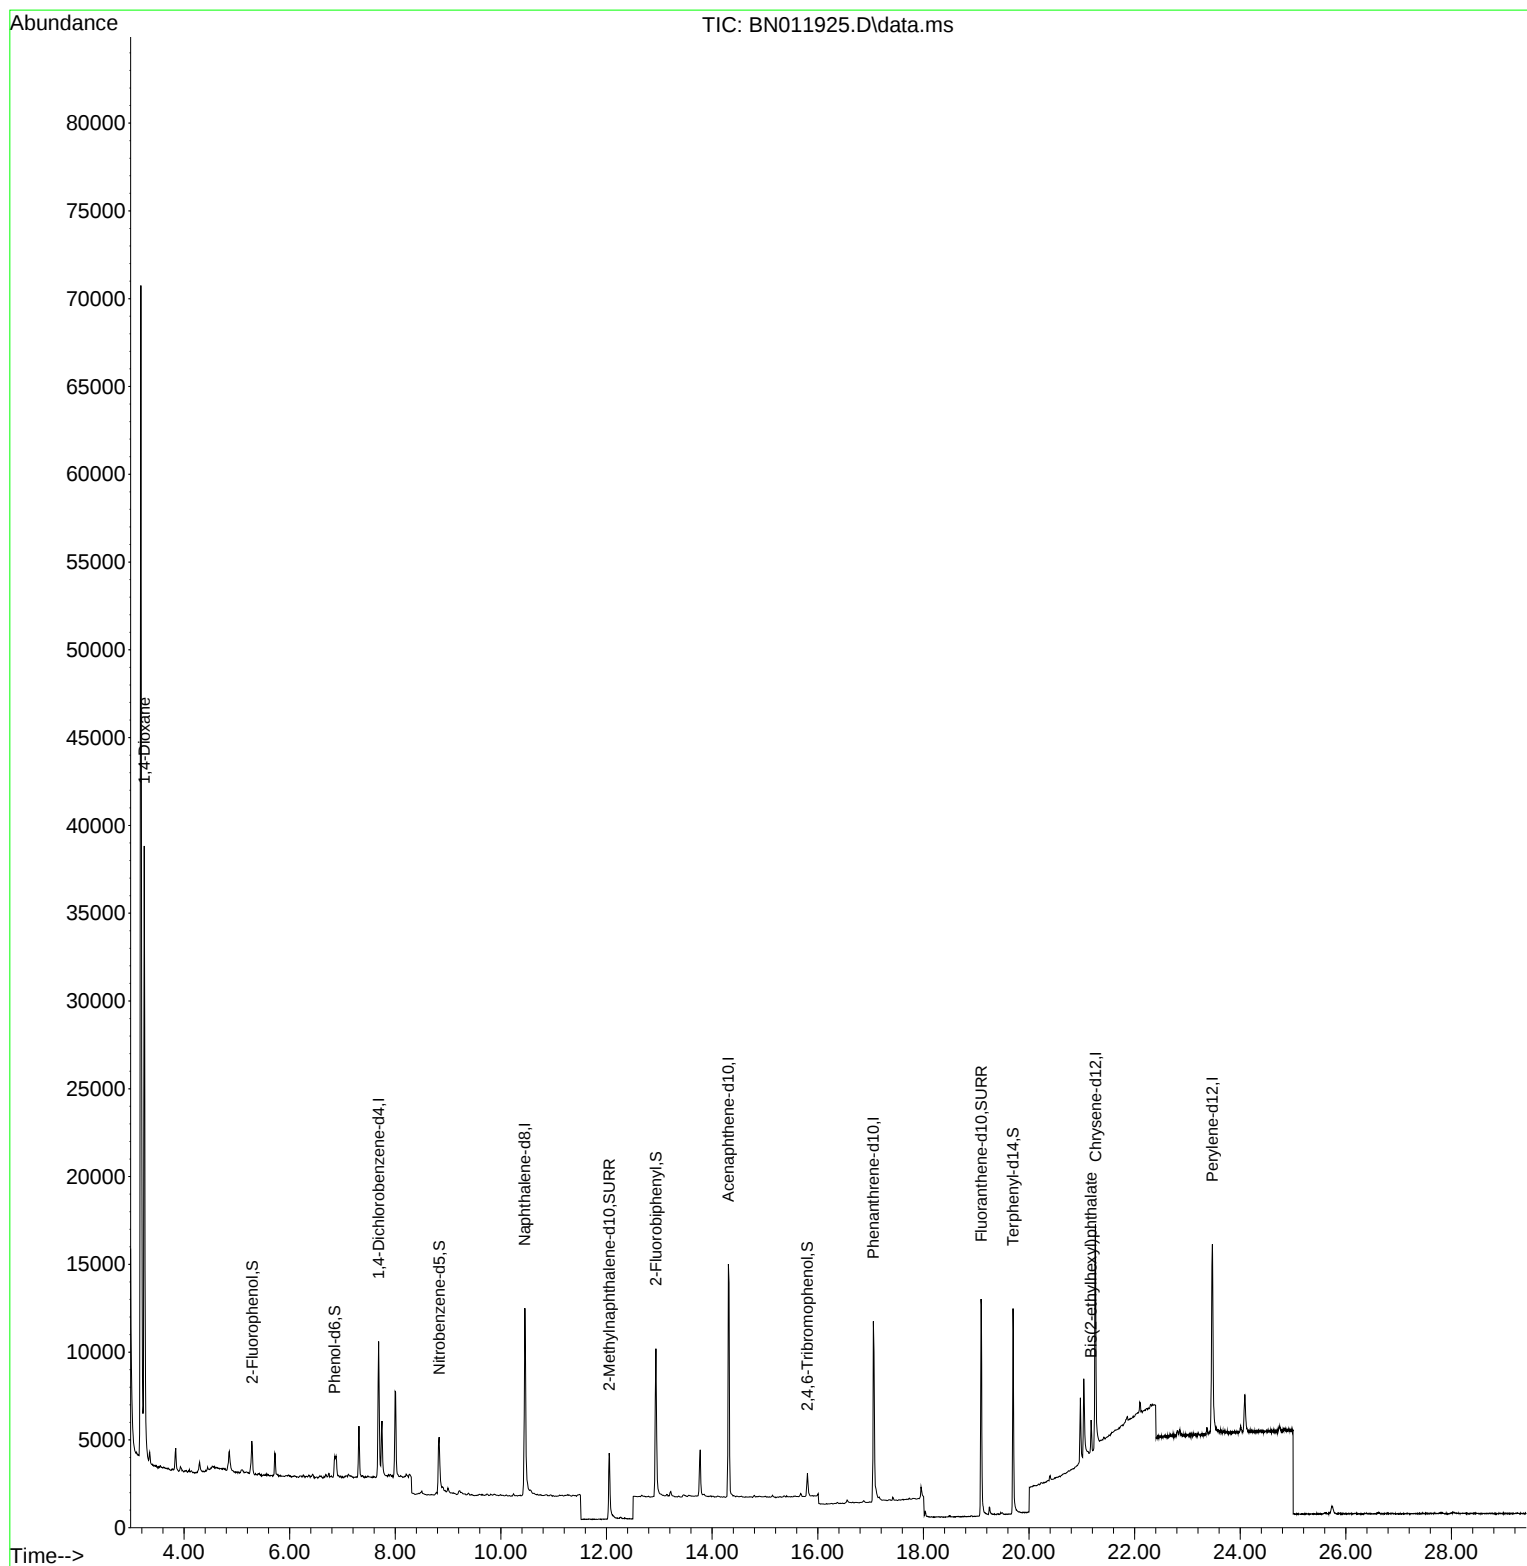


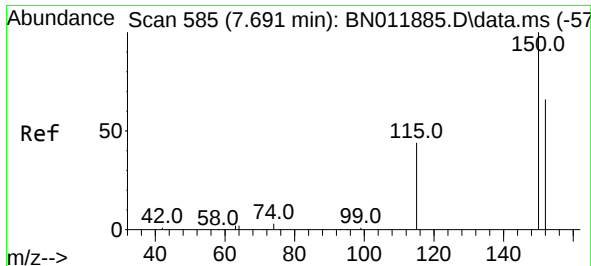

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.683 min Scan# 584
 Delta R.T. -0.008 min
 Lab File: BN011925.D
 Acq: 24 Sep 2020 21:59




Instrument :
 BNA_N
 ClientSampleId :
 RE104D1-20200917


Tgt Ion:152 Resp: 3915
 Ion Ratio Lower Upper
 152 100
 150 156.9 118.3 177.5
 115 74.6 51.3 76.9

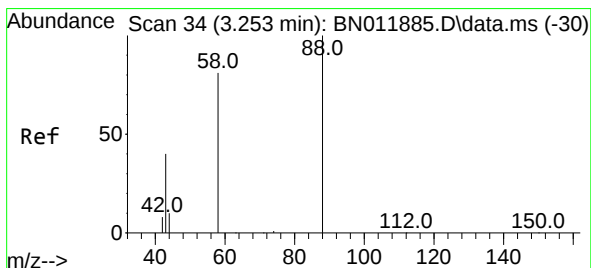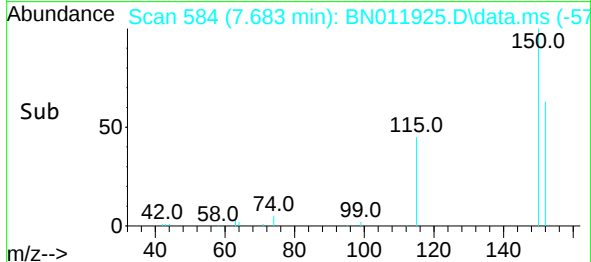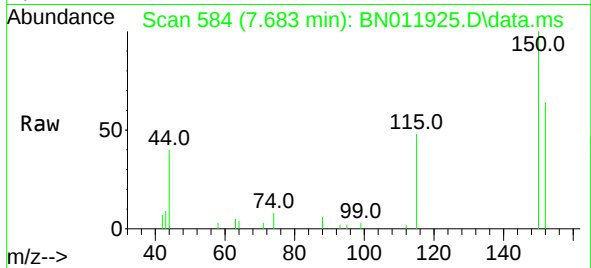

#2
 1,4-Dioxane
 Concen: 2.88 ng
 RT: 3.245 min Scan# 33
 Delta R.T. -0.008 min
 Lab File: BN011925.D
 Acq: 24 Sep 2020 21:59

Tgt Ion: 88 Resp: 19605
 Ion Ratio Lower Upper
 88 100
 58 82.0 63.3 94.9
 43 39.8 33.0 49.4


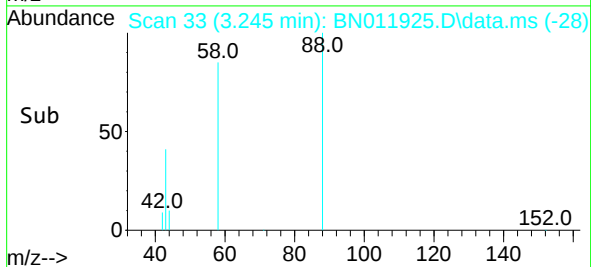

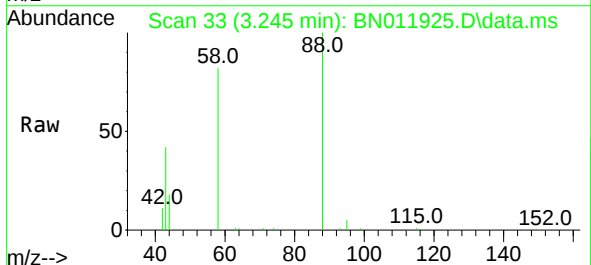


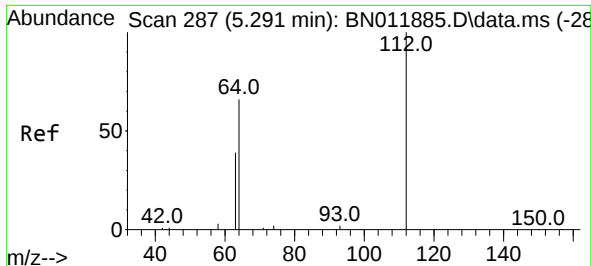

#4
2-Fluorophenol
Concen: 0.09 ng
RT: 5.291 min Scan# 287
Delta R.T. 0.000 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59




Instrument :
BNA_N
ClientSampleId :
RE104D1-20200917


Tgt Ion:	112	Resp:	1302
Ion	Ratio	Lower	Upper
112	100		
64	68.1	49.0	73.6
63	39.0	31.8	47.6

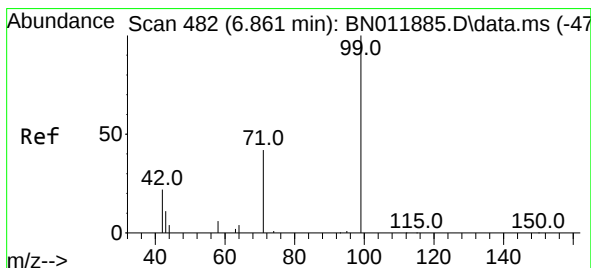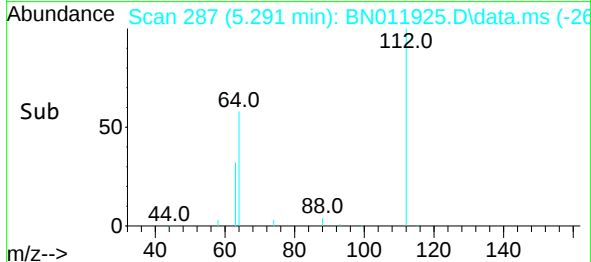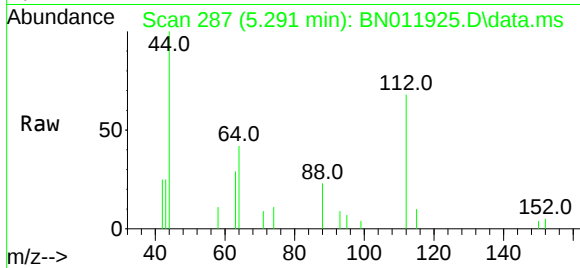

#5
Phenol-d6
Concen: 0.05 ng
RT: 6.853 min Scan# 481
Delta R.T. -0.008 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59

Tgt Ion:	99	Resp:	925
Ion	Ratio	Lower	Upper
99	100		
42	40.0	23.4	35.0
71	53.2	38.1	57.1


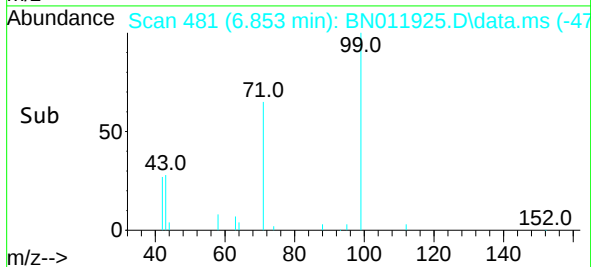

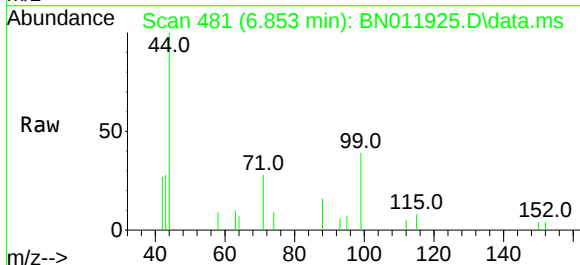


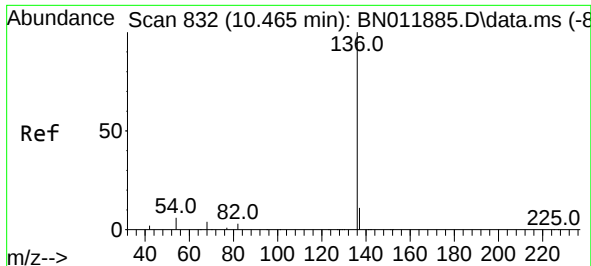

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.453 min Scan# 831
Delta R.T. -0.012 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59




Instrument :
BNA_N
ClientSampleId :
RE104D1-20200917


Tgt Ion:	136	Resp:	16089
Ion Ratio	Lower	Upper	
136	100		
137	11.5	9.5	14.3
54	10.7	5.6	8.4#
68	6.8	3.2	4.8#

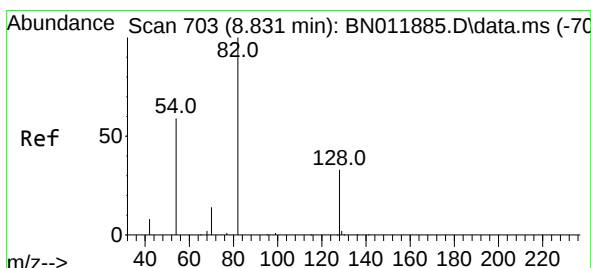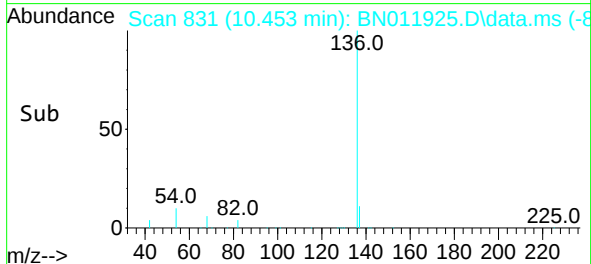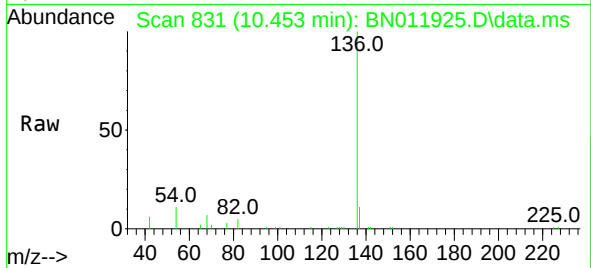

#8
Nitrobenzene-d5
Concen: 0.24 ng
RT: 8.831 min Scan# 703
Delta R.T. 0.000 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59

Tgt Ion:	82	Resp:	3987
Ion Ratio	Lower	Upper	
82	100		
128	38.0	34.2	51.2
54	55.2	43.1	64.7


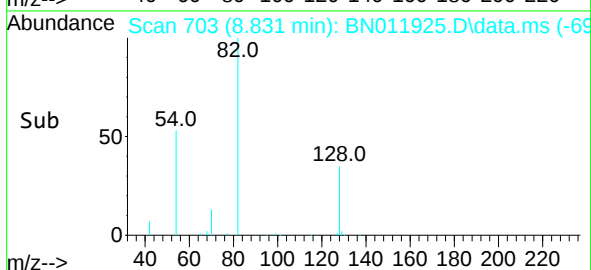

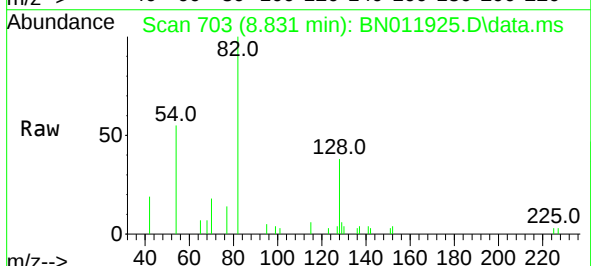


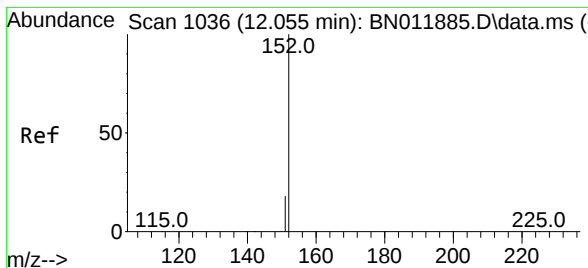

#11
2-Methylnaphthalene-d10
Concen: 0.25 ng
RT: 12.051 min Scan# 1035
Delta R.T. -0.004 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59




Instrument :
BNA_N
ClientSampleId :
RE104D1-20200917


Tgt Ion:152 Resp: 6484
Ion Ratio Lower Upper
152 100
151 20.2 16.7 25.1

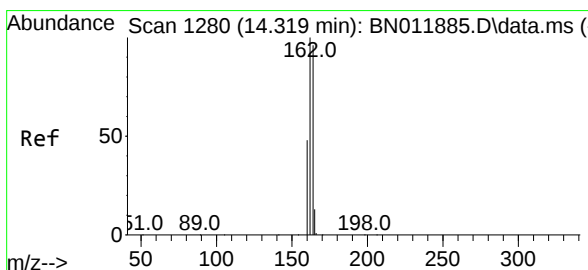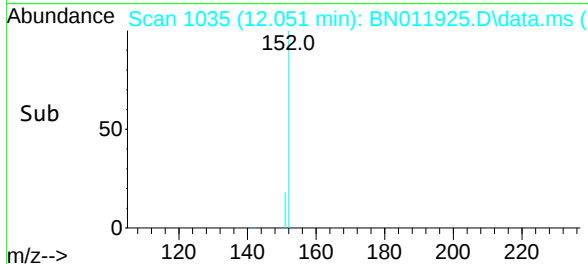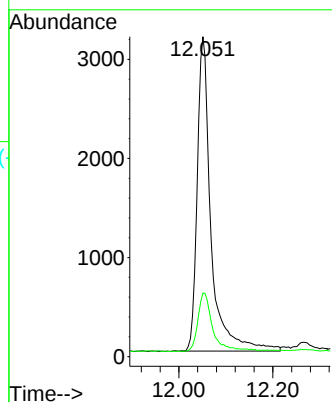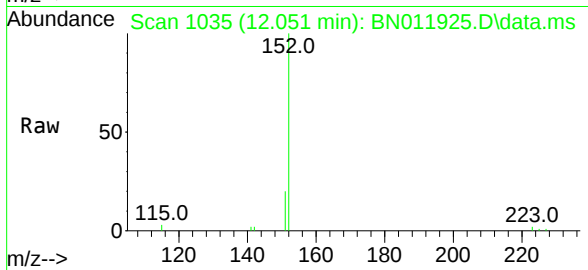

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.306 min Scan# 1279
Delta R.T. -0.012 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59

Tgt Ion:164 Resp: 8914
Ion Ratio Lower Upper
164 100
162 105.0 83.6 125.4
160 51.2 41.2 61.8


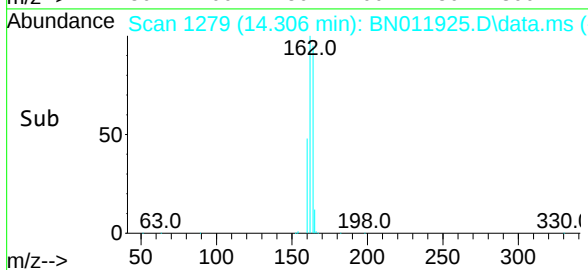
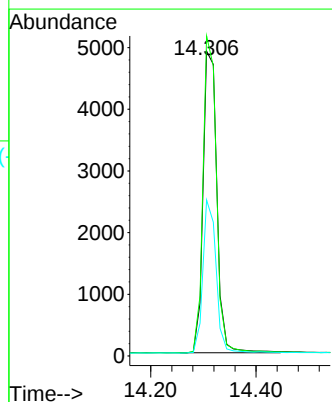
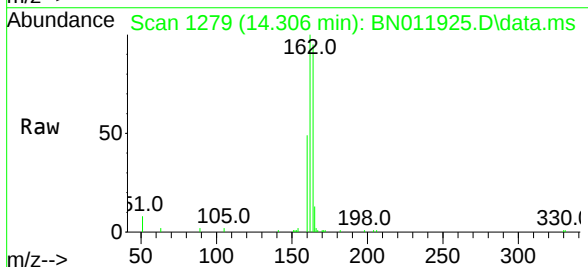


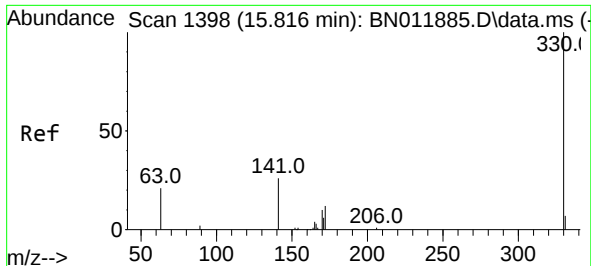

#14
2,4,6-Tribromophenol
Concen: 0.23 ng
RT: 15.803 min Scan# 1397
Delta R.T. -0.013 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59




Instrument :
BNA_N
ClientSampleId :
RE104D1-20200917


Tgt Ion:330 Resp: 1007
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 52.8 33.7 50.5#

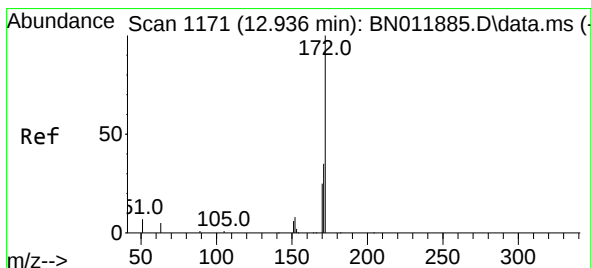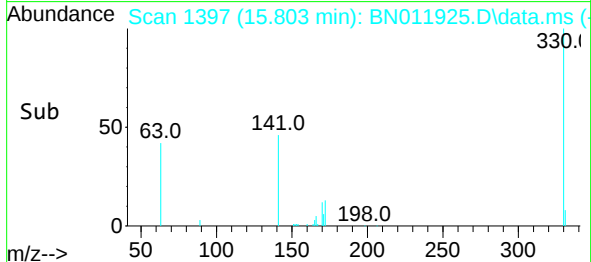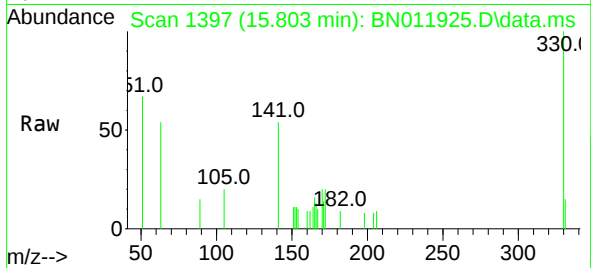

#15
2-Fluorobiphenyl
Concen: 0.25 ng
RT: 12.936 min Scan# 1171
Delta R.T. 0.000 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59

Tgt Ion:172 Resp: 8318
Ion Ratio Lower Upper
172 100
171 35.3 27.4 41.2
170 24.8 17.8 26.6


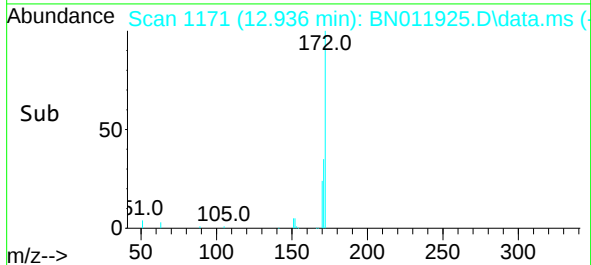

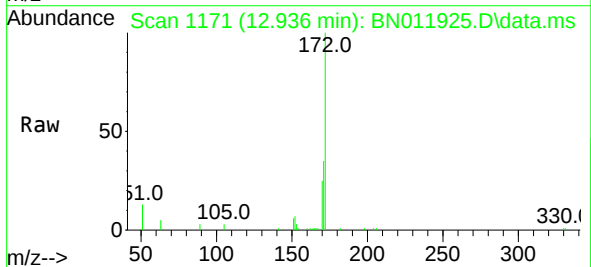


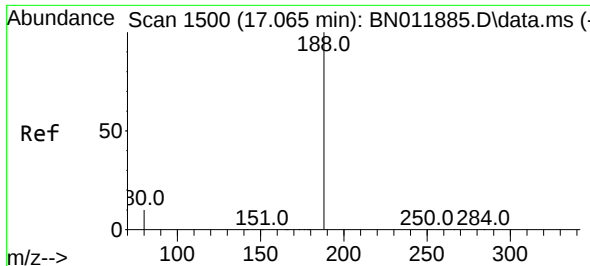

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.053 min Scan# 1499
Delta R.T. -0.012 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59




Instrument :
BNA_N
ClientSampleId :
RE104D1-20200917


Tgt Ion:188 Resp: 17663
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.6 7.7 11.5#

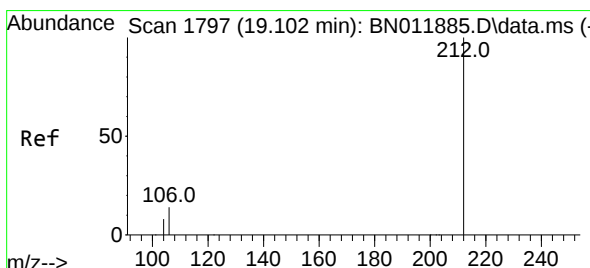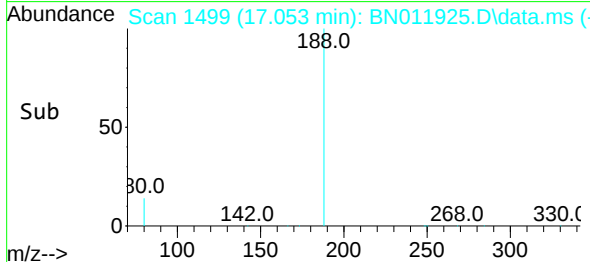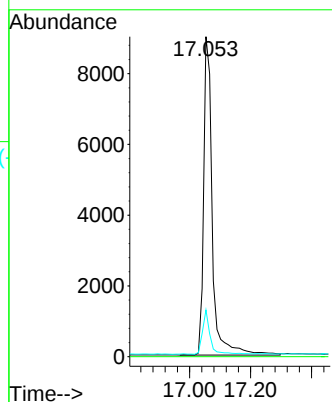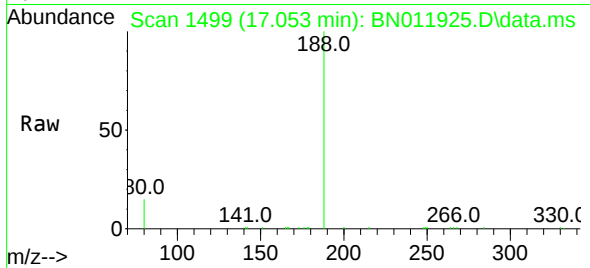

#27
Fluoranthene-d10
Concen: 0.29 ng
RT: 19.097 min Scan# 1796
Delta R.T. -0.005 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59

Tgt Ion:212 Resp: 15260
Ion Ratio Lower Upper
212 100
106 13.9 6.4 9.6#
104 8.4 3.9 5.9#


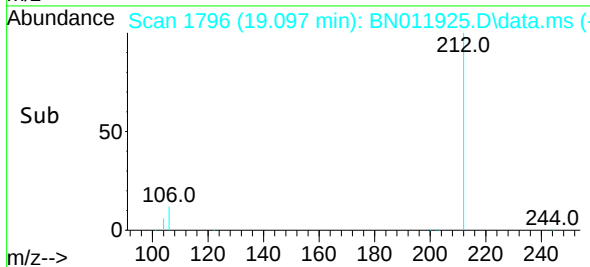
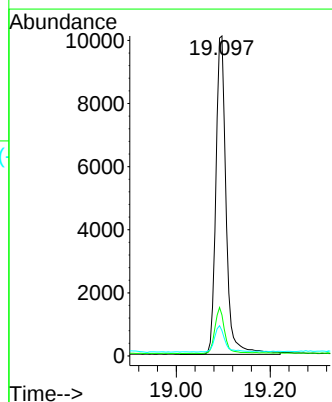
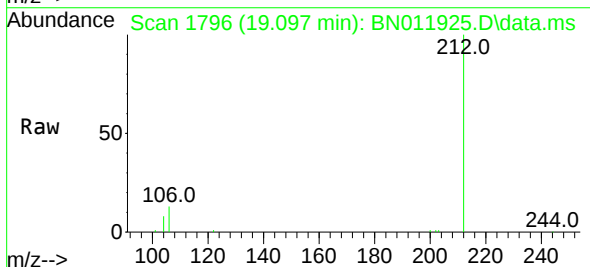


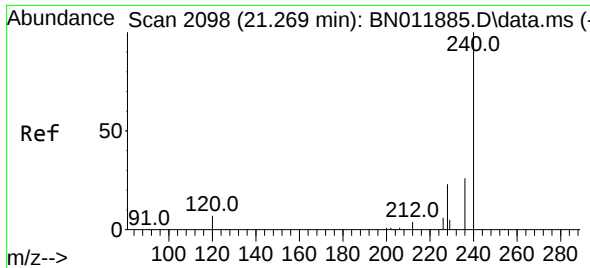

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.259 min Scan# 2097
Delta R.T. -0.010 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59




Instrument :
BNA_N
ClientSampleId :
RE104D1-20200917


Tgt Ion:240 Resp: 15658
Ion Ratio Lower Upper
240 100
120 10.5 3.5 5.3#
236 26.6 20.5 30.7

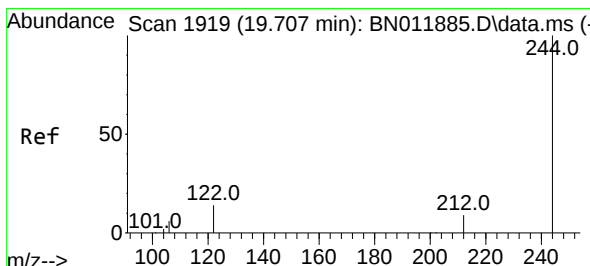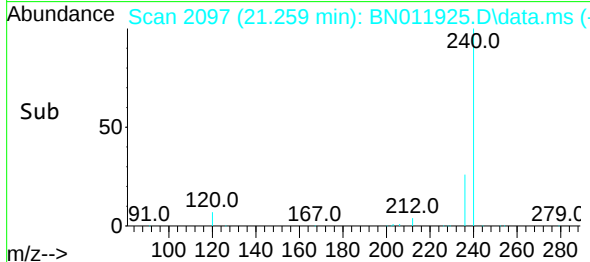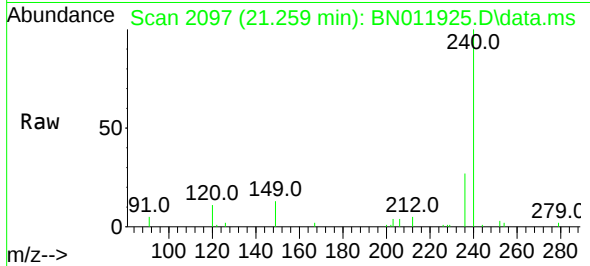

#31
Terphenyl-d14
Concen: 0.36 ng
RT: 19.698 min Scan# 1917
Delta R.T. -0.010 min
Lab File: BN011925.D
Acq: 24 Sep 2020 21:59

Tgt Ion:244 Resp: 12713
Ion Ratio Lower Upper
244 100
212 9.4 7.3 10.9
122 14.7 7.8 11.6#


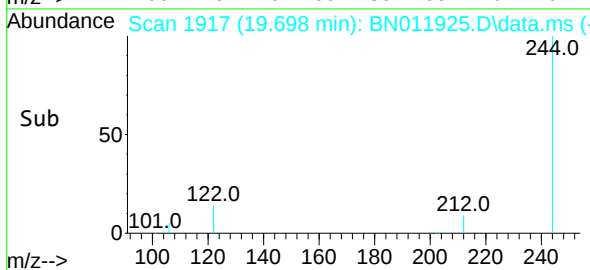

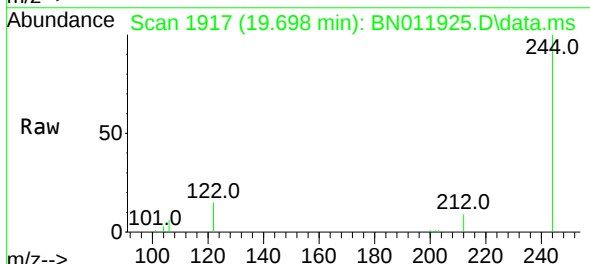


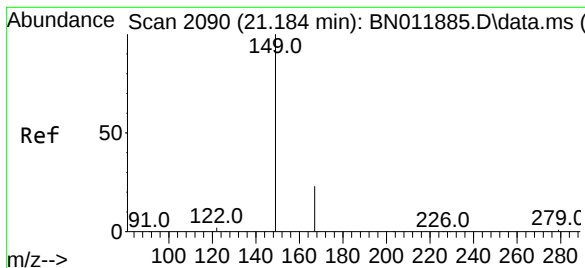

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.05 ng
 RT: 21.174 min Scan# 2089
 Delta R.T. -0.010 min
 Lab File: BN011925.D
 Acq: 24 Sep 2020 21:59

Instrument :
 BNA_N
 ClientSampleId :
 RE104D1-20200917

Tgt Ion:149 Resp: 1867
 Ion Ratio Lower Upper
 149 100
 167 22.3 23.6 35.4#
 279 4.1 4.0 6.0

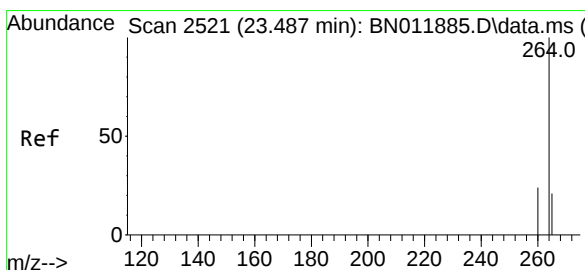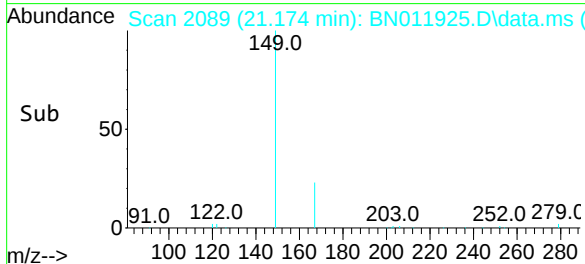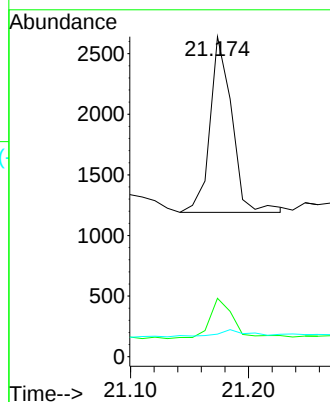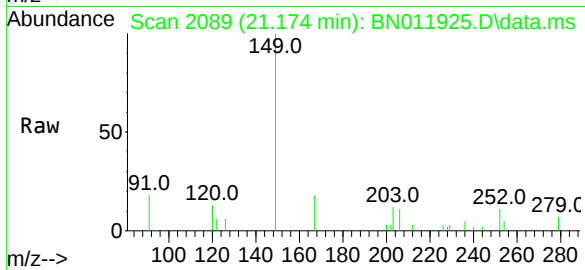

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.470 min Scan# 2516
 Delta R.T. -0.017 min
 Lab File: BN011925.D
 Acq: 24 Sep 2020 21:59

Tgt Ion:264 Resp: 15870
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.6 29.4
 265 61.7 38.6 58.0#

