
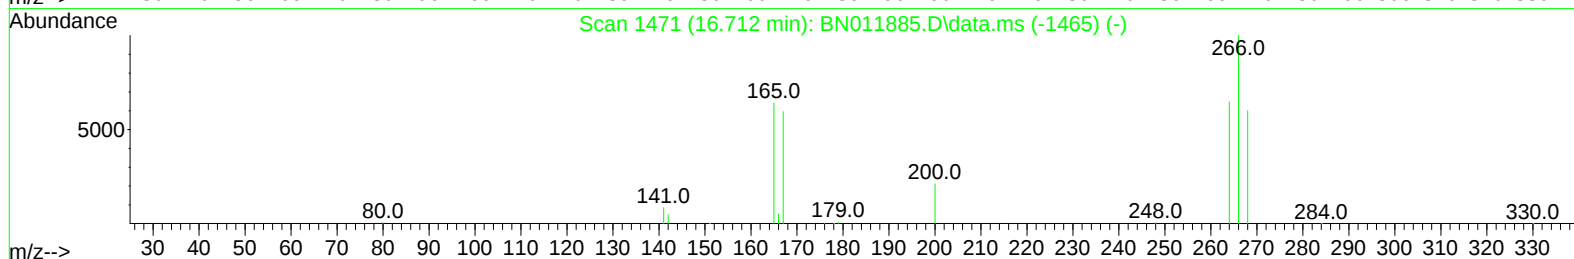
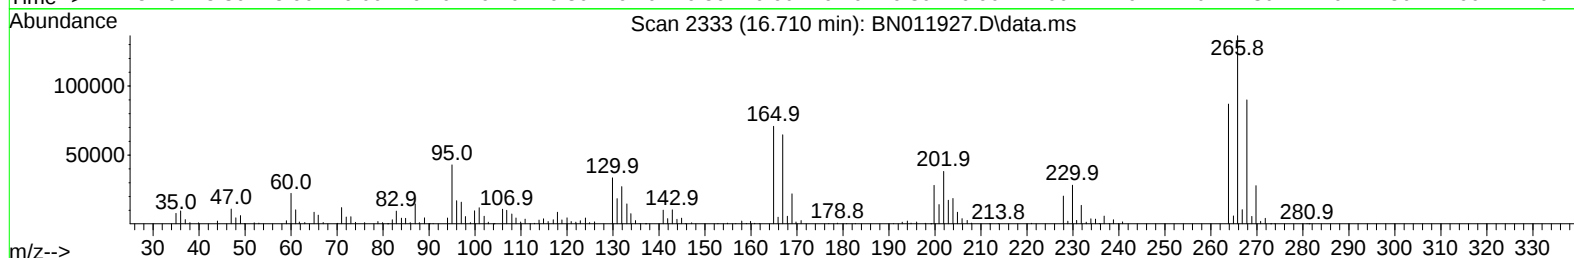


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092420\
Data File : BN011927.D
Acq On : 25 Sep 2020 00:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 00:58:49 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 18:41:41 2020
Response via : Initial Calibration

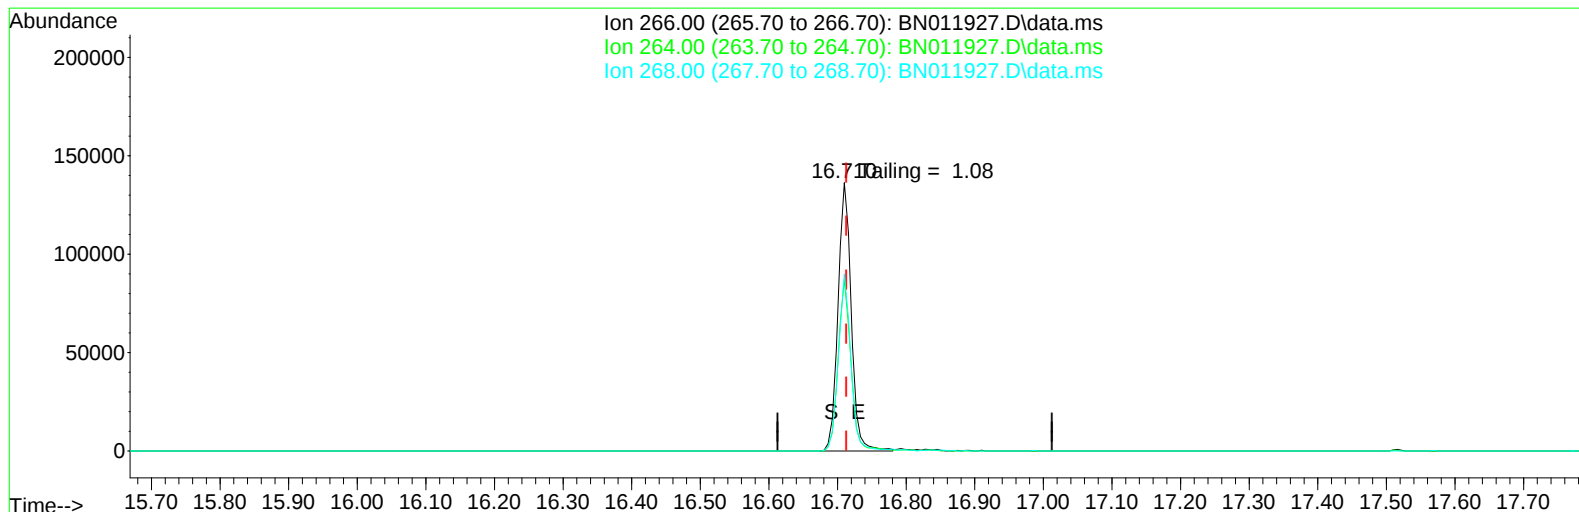

TIC: BN011927.D\data.ms

(24) Pentachlorophenol

16.710min (-0.003) 0.00 ng

response 182679

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.00	62.27
268.00	65.50	63.01
0.00	0.00	0.00