

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092420\
 Data File : BN011919.D
 Acq On : 24 Sep 2020 18:22
 Operator : CG/JU
 Sample : L4125-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CS-31

Quant Time: Sep 25 01:40:25 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 18:41:41 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.683	152	4017	0.40	ng	0.00
7) Naphthalene-d8	10.453	136	16683	0.40	ng	#-0.01
13) Acenaphthene-d10	14.319	164	8887	0.40	ng	0.00
19) Phenanthrene-d10	17.053	188	17318	0.40	ng	#-0.01
29) Chrysene-d12	21.258	240	16163	0.40	ng	#-0.01
36) Perylene-d12	23.477	264	16772	0.40	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	5388	0.38	ng	0.00
5) Phenol-d6	6.853	99	6813	0.38	ng	0.00
8) Nitrobenzene-d5	8.830	82	6751	0.39	ng	0.00
11) 2-Methylnaphthalene-d10	12.051	152	11043	0.42	ng	0.00
14) 2,4,6-Tribromophenol	15.803	330	1824	0.42	ng	-0.01
15) 2-Fluorobiphenyl	12.936	172	14080	0.42	ng	0.00
27) Fluoranthene-d10	19.097	212	22897	0.45	ng	0.00
31) Terphenyl-d14	19.702	244	19403	0.53	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.184	149	2543	0.07	ng	Qvalue # 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092420\
Data File : BN011919.D
Acq On : 24 Sep 2020 18:22
Operator : CG/JU
Sample : L4125-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CS-31

Quant Time: Sep 25 01:40:25 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 18:41:41 2020
Response via : Initial Calibration




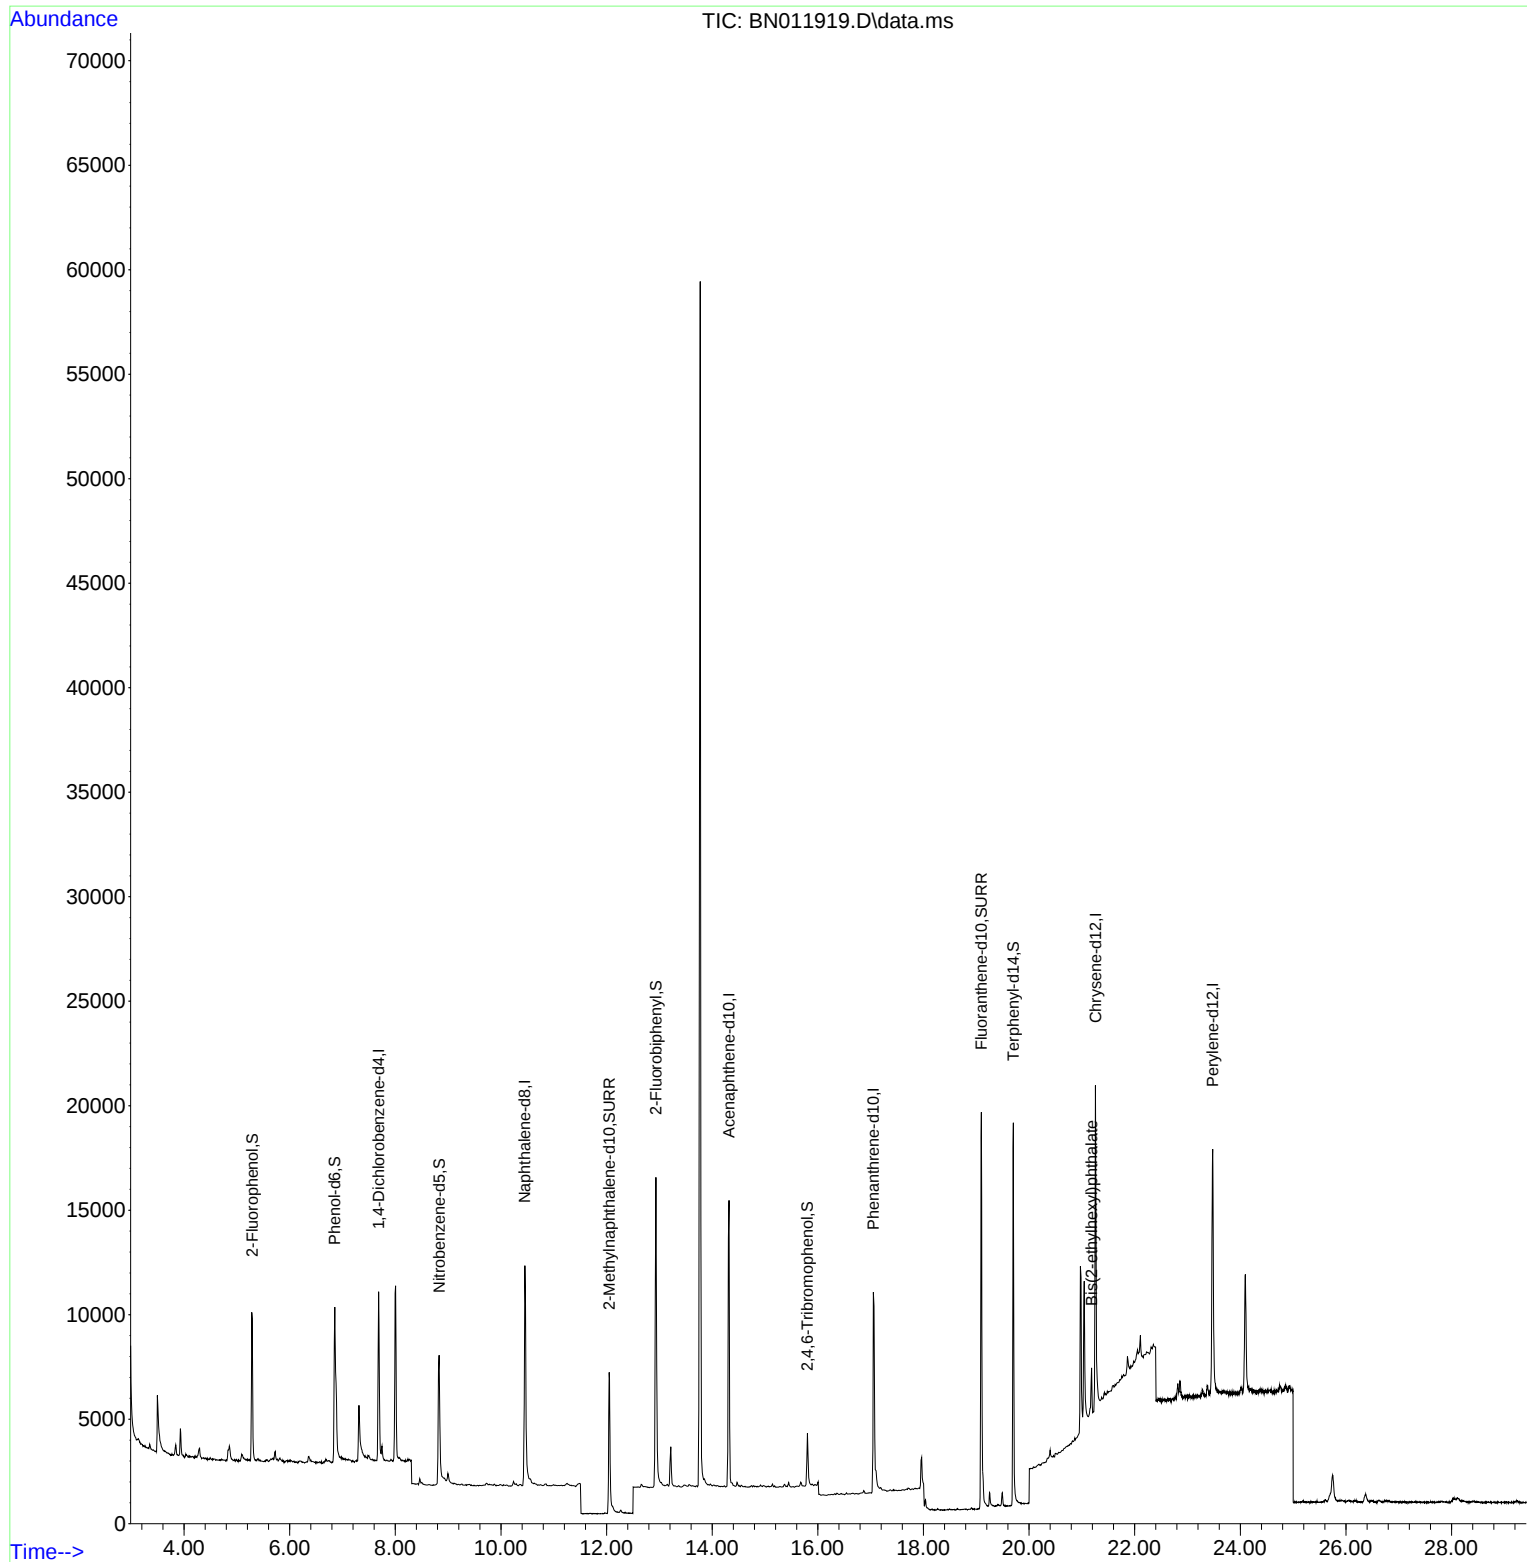




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.683 min Scan# 584
Delta R.T. -0.008 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22




Instrument :
BNA_N
ClientSampleId :
CS-31

Tgt Ion:152 Resp: 4017
Ion Ratio Lower Upper
152 100
150 158.8 118.3 177.5
115 73.8 51.3 76.9

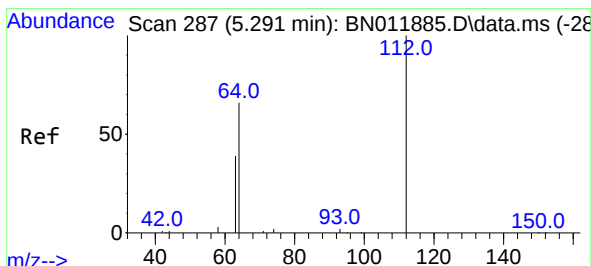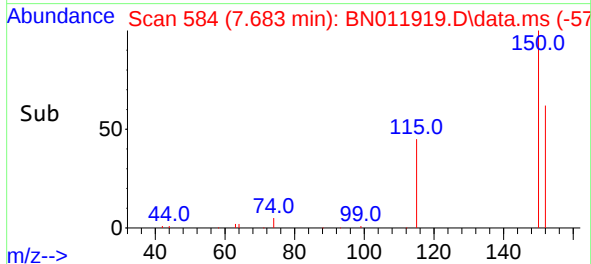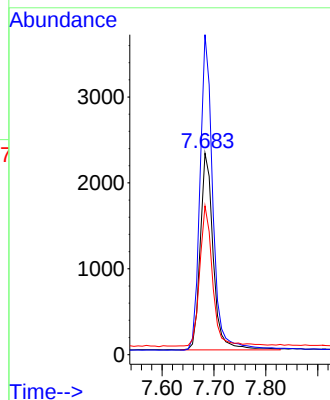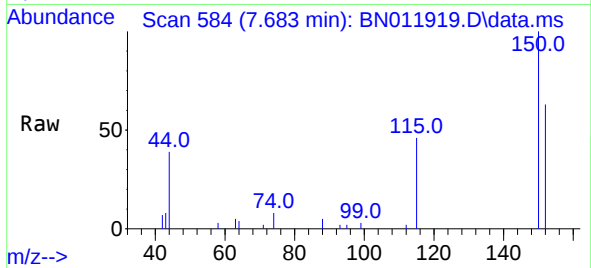

#4
2-Fluorophenol
Concen: 0.38 ng
RT: 5.291 min Scan# 287
Delta R.T. -0.000 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22

Tgt Ion:112 Resp: 5388
Ion Ratio Lower Upper
112 100
64 67.6 49.0 73.6
63 39.7 31.8 47.6

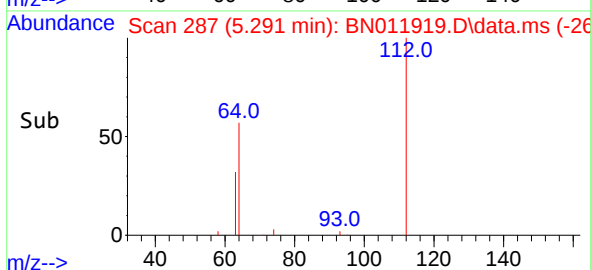
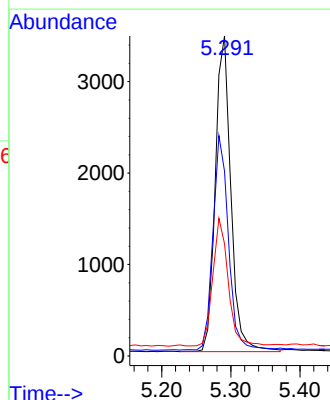
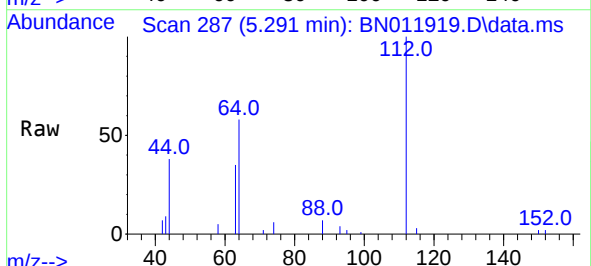




#5
Phenol-d6
Concen: 0.38 ng
RT: 6.853 min Scan# 481
Delta R.T. -0.008 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22




Instrument :
BNA_N
ClientSampleId :
CS-31


Tgt Ion: 99 Resp: 6813
Ion Ratio Lower Upper
99 100
42 30.6 23.4 35.0
71 43.2 38.1 57.1

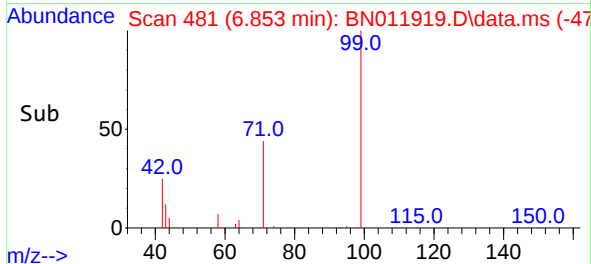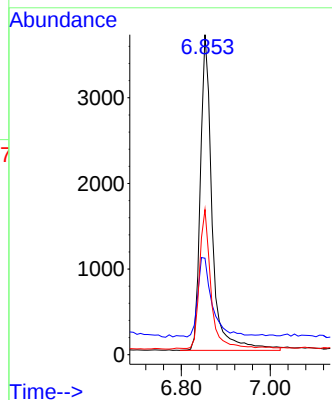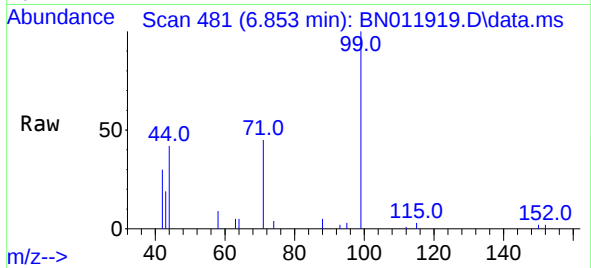

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.453 min Scan# 831
Delta R.T. -0.013 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22

Tgt Ion: 136 Resp: 16683
Ion Ratio Lower Upper
136 100
137 11.5 9.5 14.3
54 11.1 5.6 8.4#
68 7.0 3.2 4.8#


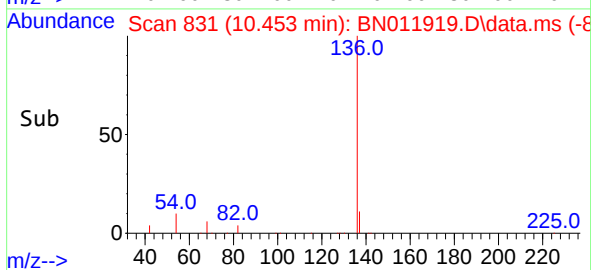
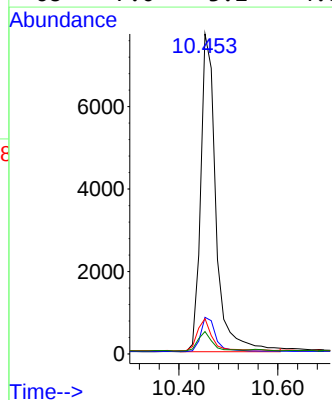
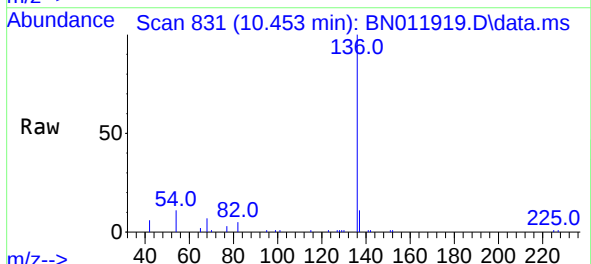


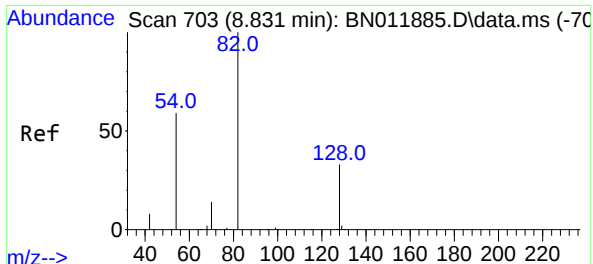

#8
Nitrobenzene-d5
Concen: 0.39 ng
RT: 8.830 min Scan# 703
Delta R.T. -0.000 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22




Instrument :
BNA_N
ClientSampleId :
CS-31


Tgt Ion: 82 Resp: 6751
Ion Ratio Lower Upper
82 100
128 38.6 34.2 51.2
54 55.7 43.1 64.7

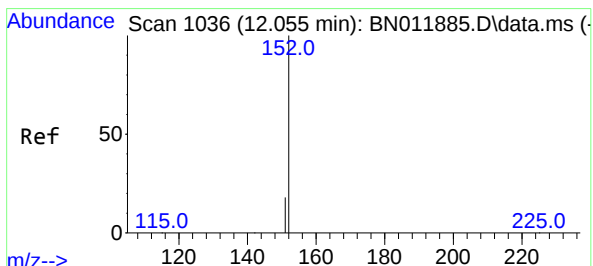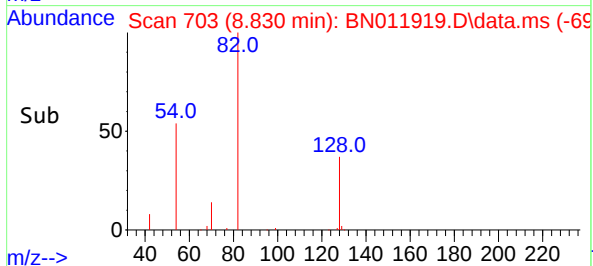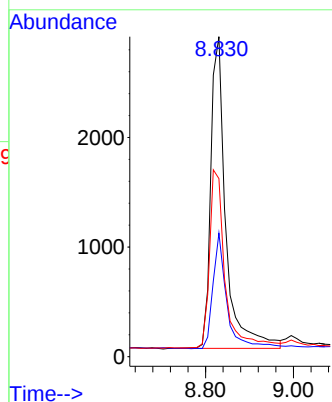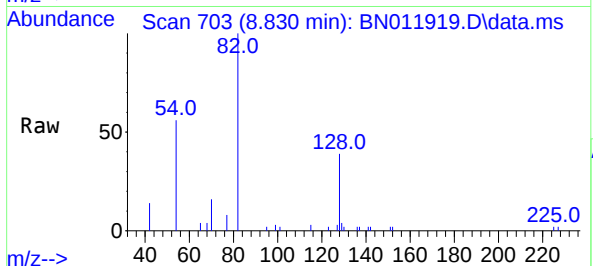

#11
2-Methylnaphthalene-d10
Concen: 0.42 ng
RT: 12.051 min Scan# 1035
Delta R.T. -0.005 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22

Tgt Ion: 152 Resp: 11043
Ion Ratio Lower Upper
152 100
151 20.6 16.7 25.1


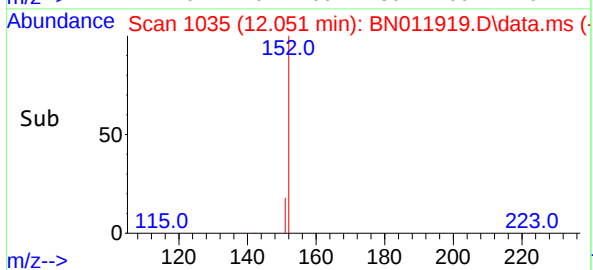
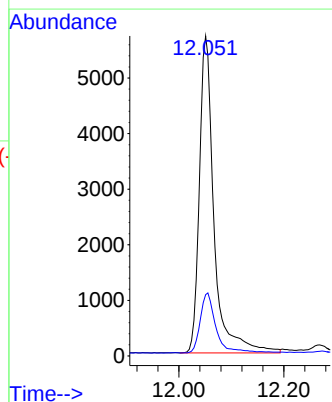
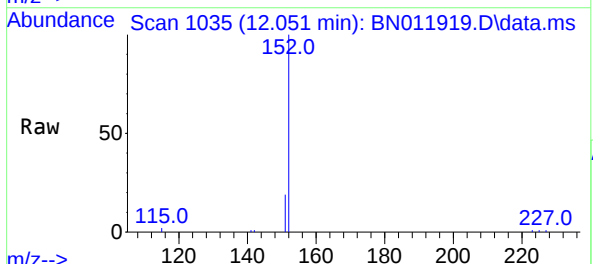


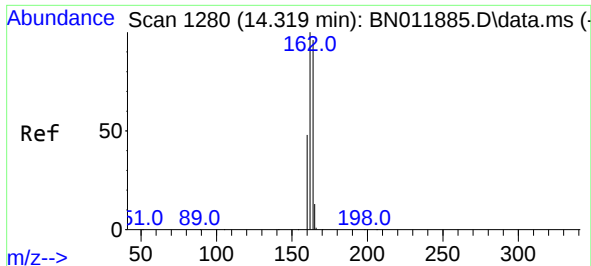

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.319 min Scan# 1280
Delta R.T. -0.000 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22




Instrument :
BNA_N
ClientSampled :
CS-31


Tgt Ion:164 Resp: 8887
Ion Ratio Lower Upper
164 100
162 100.0 83.6 125.4
160 46.2 41.2 61.8

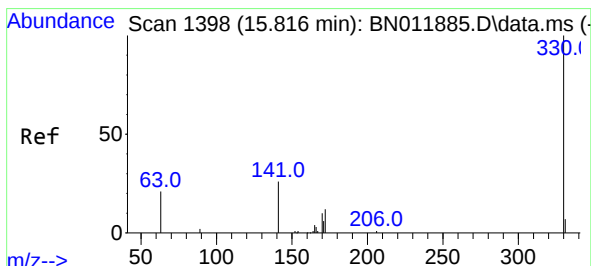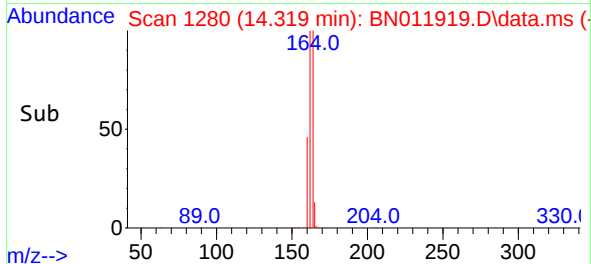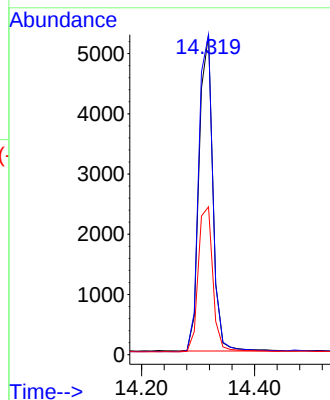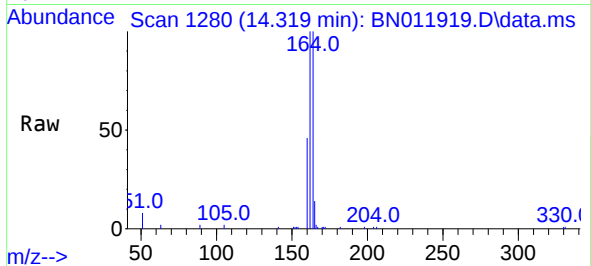

#14
2,4,6-Tribromophenol
Concen: 0.42 ng
RT: 15.803 min Scan# 1397
Delta R.T. -0.013 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22

Tgt Ion:330 Resp: 1824
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 50.3 33.7 50.5


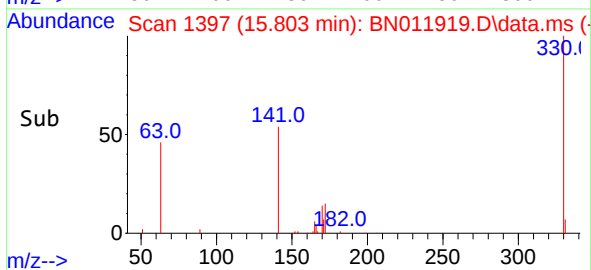
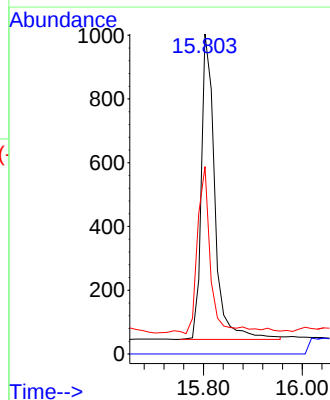
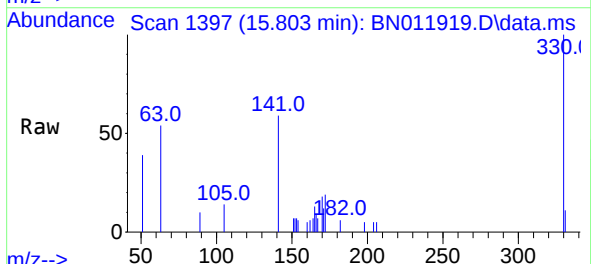


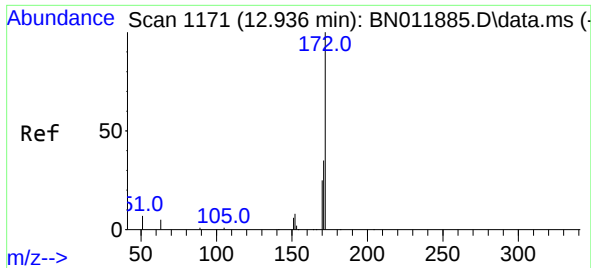

#15
2-Fluorobiphenyl
Concen: 0.42 ng
RT: 12.936 min Scan# 1171
Delta R.T. -0.000 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22




Instrument :
BNA_N
ClientSampleId :
CS-31


Tgt Ion:	172	Resp:	14080
Ion	Ratio	Lower	Upper
172	100		
171	36.2	27.4	41.2
170	24.4	17.8	26.6

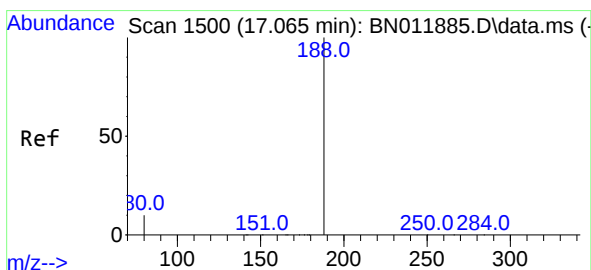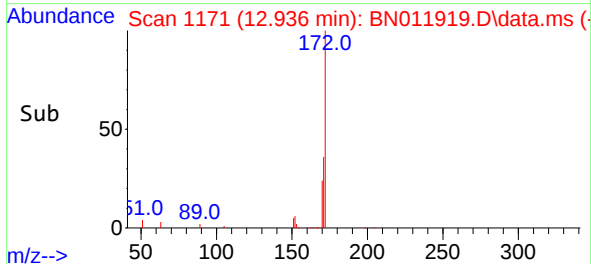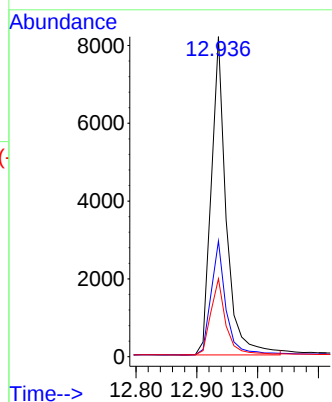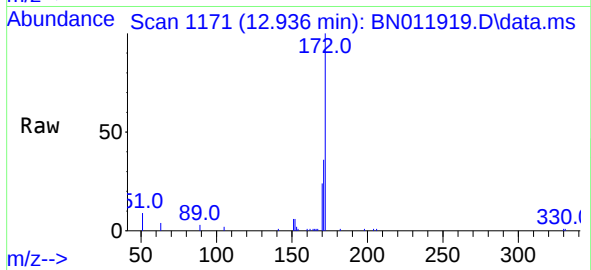

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.053 min Scan# 1499
Delta R.T. -0.012 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22

Tgt Ion:	188	Resp:	17318
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	15.9	7.7	11.5


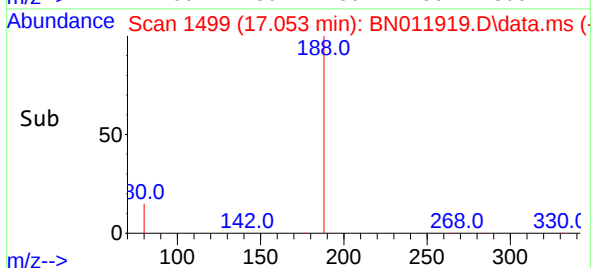
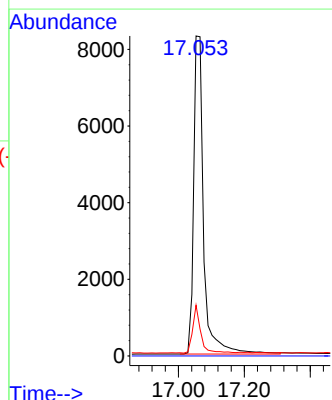
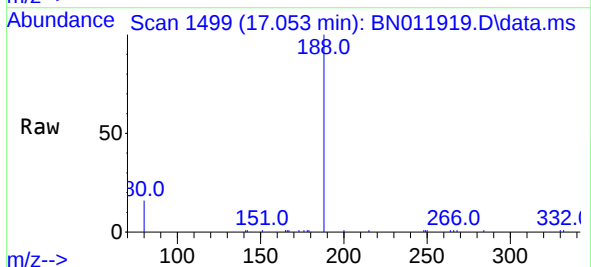


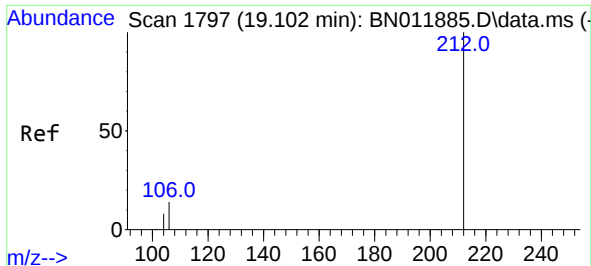

#27
Fluoranthene-d10
Concen: 0.45 ng
RT: 19.097 min Scan# 1796
Delta R.T. -0.005 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22




Instrument :
BNA_N
ClientSampleId :
CS-31


Tgt Ion:212 Resp: 22897
Ion Ratio Lower Upper
212 100
106 13.7 6.4 9.6#
104 9.0 3.9 5.9#

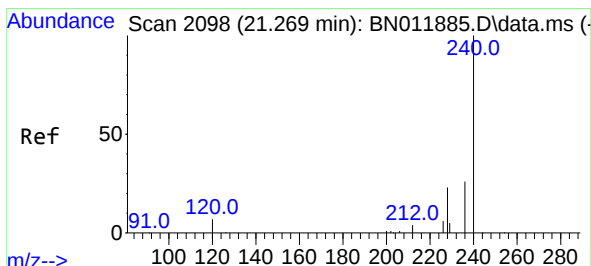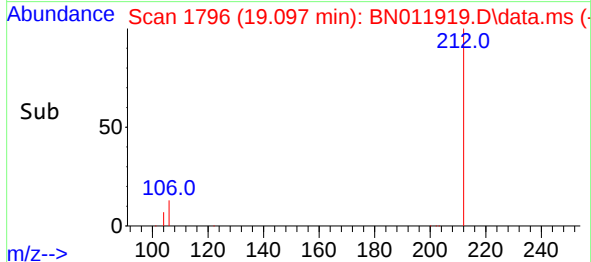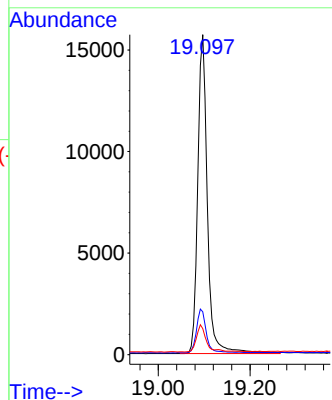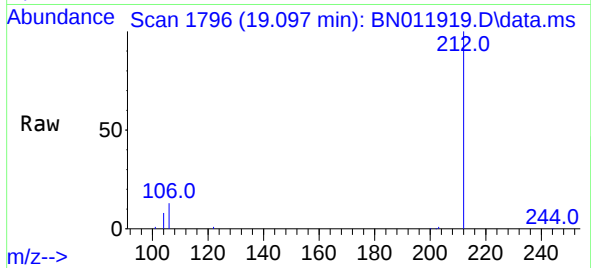

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.258 min Scan# 2097
Delta R.T. -0.011 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22

Tgt Ion:240 Resp: 16163
Ion Ratio Lower Upper
240 100
120 13.6 3.5 5.3#
236 27.3 20.5 30.7


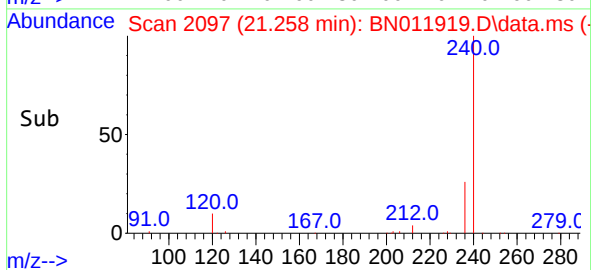
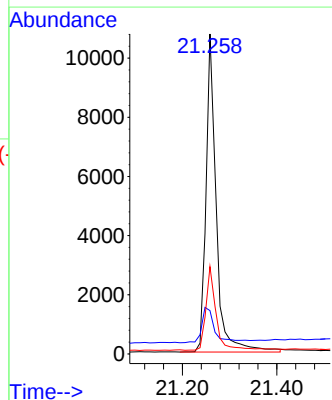
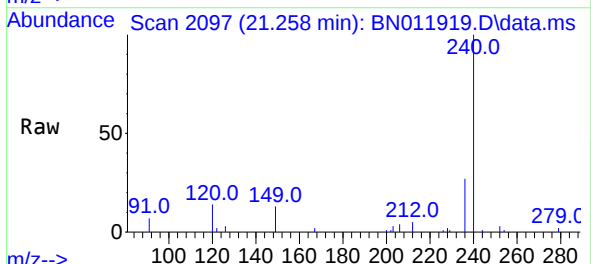


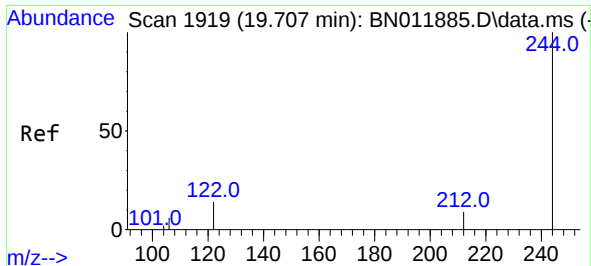

#31
Terphenyl-d14
Concen: 0.53 ng
RT: 19.702 min Scan# 1918
Delta R.T. -0.005 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22




Instrument :
BNA_N
ClientSampleId :
CS-31


Tgt Ion:244 Resp: 19403
Ion Ratio Lower Upper
244 100
212 8.7 7.3 10.9
122 13.0 7.8 11.6#

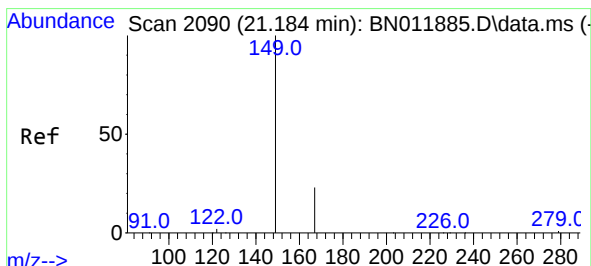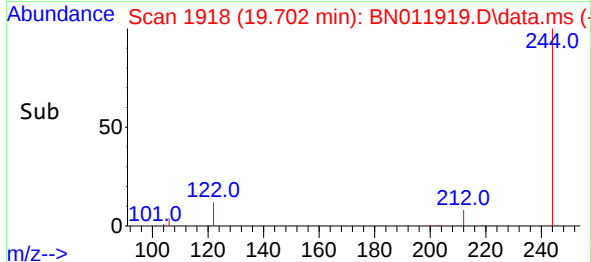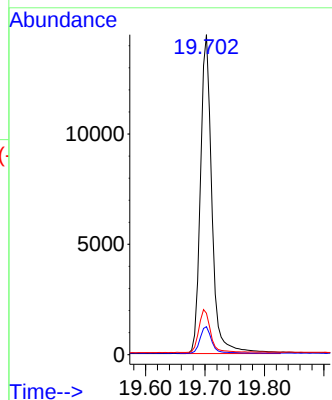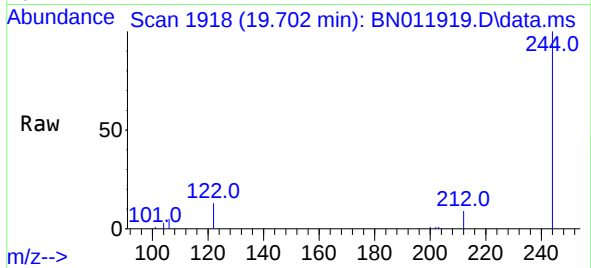

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.07 ng
RT: 21.184 min Scan# 2090
Delta R.T. -0.000 min
Lab File: BN011919.D
Acq: 24 Sep 2020 18:22

Tgt Ion:149 Resp: 2543
Ion Ratio Lower Upper
149 100
167 23.6 23.6 35.4#
279 3.7 4.0 6.0#

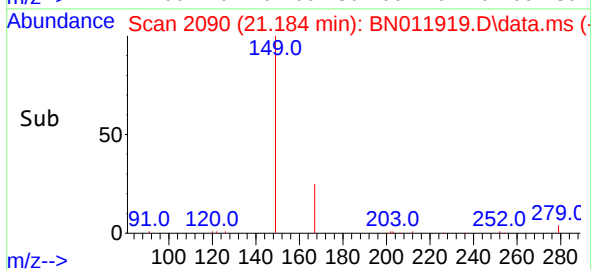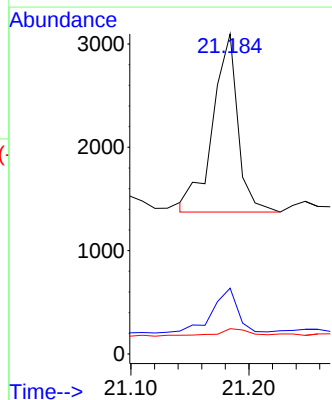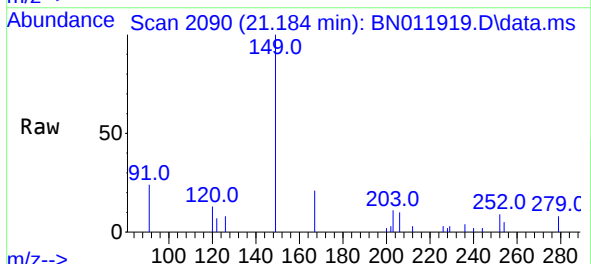

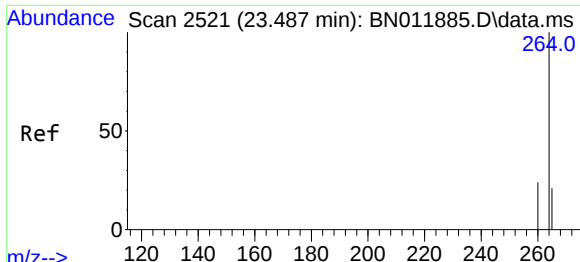

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.477 min Scan# 2518
 Delta R.T. -0.010 min
 Lab File: BN011919.D
 Acq: 24 Sep 2020 18:22

Instrument :
 BNA_N
 ClientSampleId :
 CS-31

Tgt Ion:	264	Resp:	16772
Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.6	29.4
265	60.2	38.6	58.0#

