
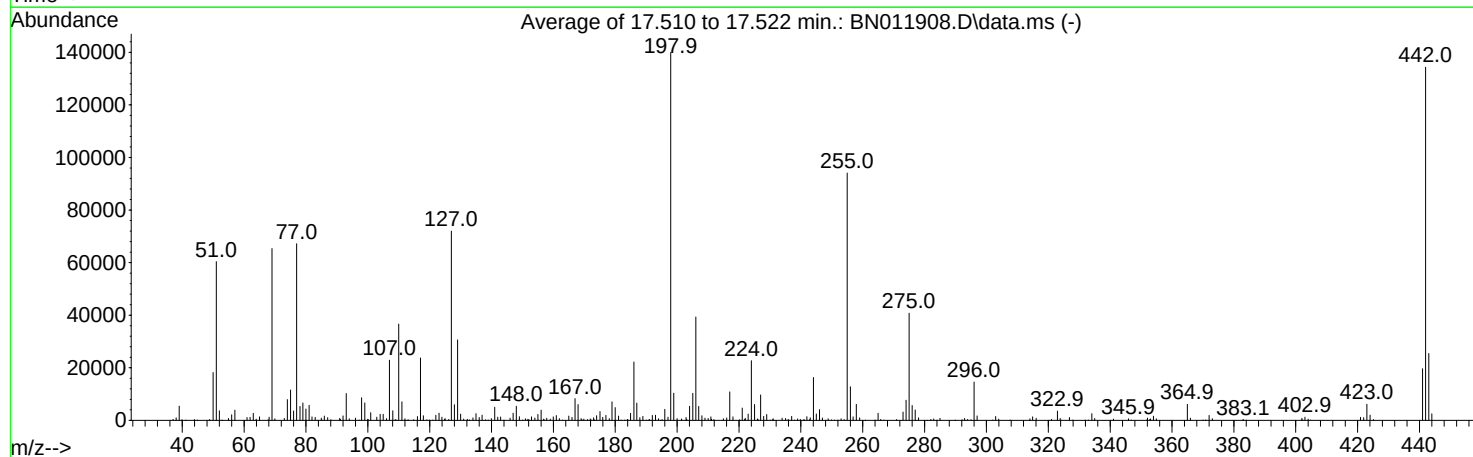


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092420\
 Data File : BN011908.D
 Acq On : 24 Sep 2020 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 23 18:41:41 2020

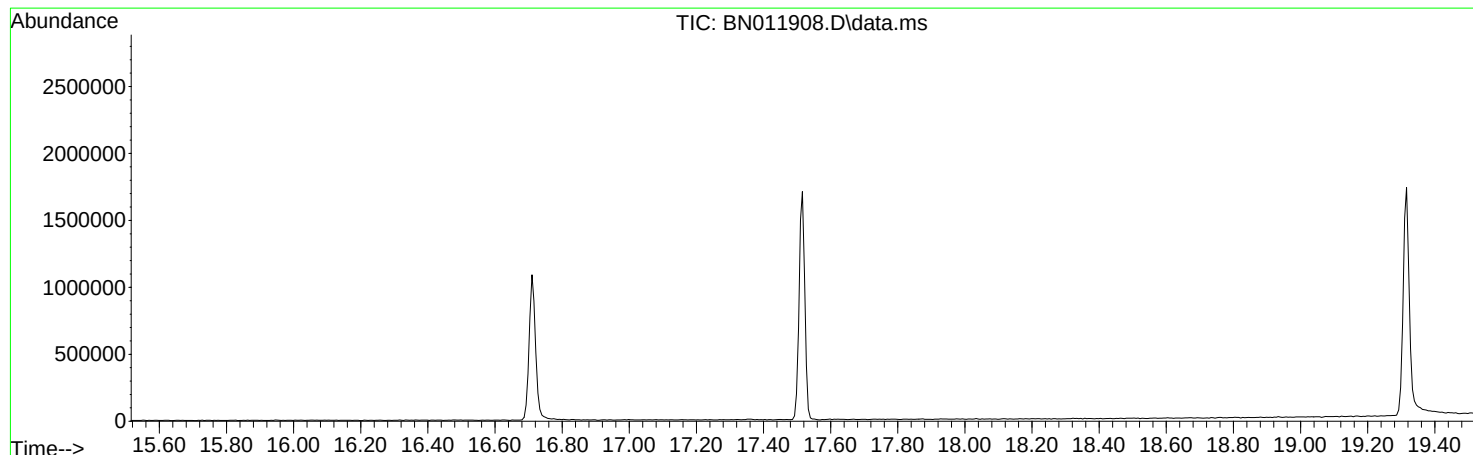

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	60382	PASS
68	69	0.00	2	1.9	1216	PASS
69	198	0.00	100	46.7	65397	PASS
70	69	0.00	2	1.0	629	PASS
127	198	10	80	51.4	71976	PASS
197	198	0.00	2	0.9	1194	PASS
198	198	100	100	100.0	139936	PASS
199	198	5	9	7.4	10352	PASS
275	198	10	60	29.1	40781	PASS
365	198	1	100	4.4	6089	PASS
441	198	0.01	100	14.0	19648	PASS
442	198	50	100	96.0	134336	PASS
443	442	15	24	19.0	25469	PASS