


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092420\
 Data File : BN011927.D
 Acq On : 25 Sep 2020 00:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 25 11:18:41 2020

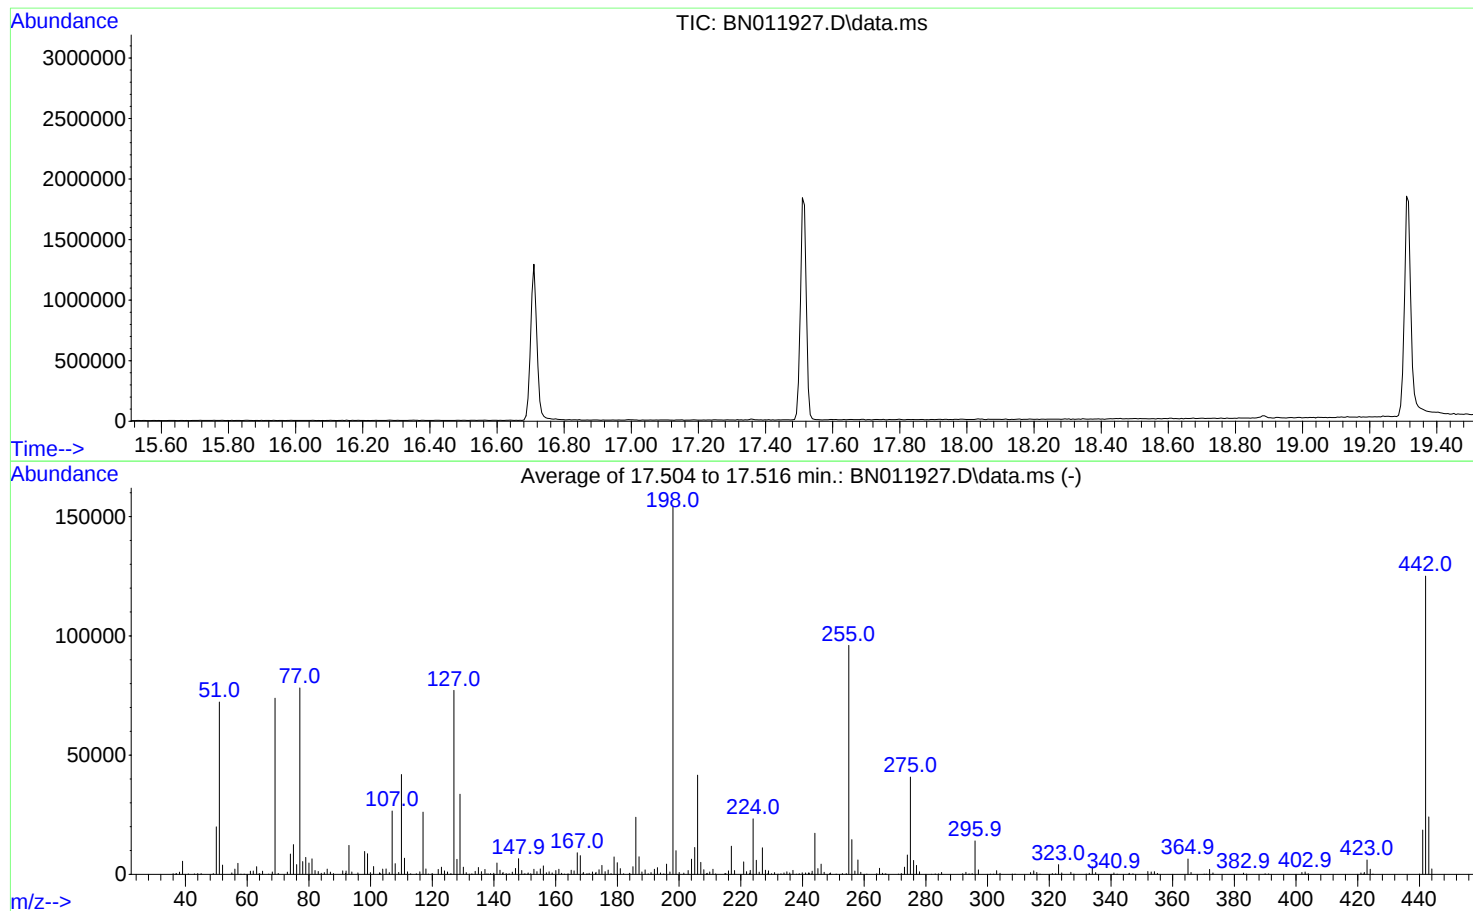

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	72261	PASS
68	69	0.00	2	1.4	1025	PASS
69	198	0.00	100	47.9	73885	PASS
70	69	0.00	2	0.6	427	PASS
127	198	10	80	50.0	77152	PASS
197	198	0.00	2	0.6	981	PASS
198	198	100	100	100.0	154253	PASS
199	198	5	9	6.5	9965	PASS
275	198	10	60	26.4	40787	PASS
365	198	1	100	4.2	6446	PASS
441	198	0.01	100	12.0	18572	PASS
442	198	50	100	81.1	125077	PASS
443	442	15	24	19.3	24125	PASS