
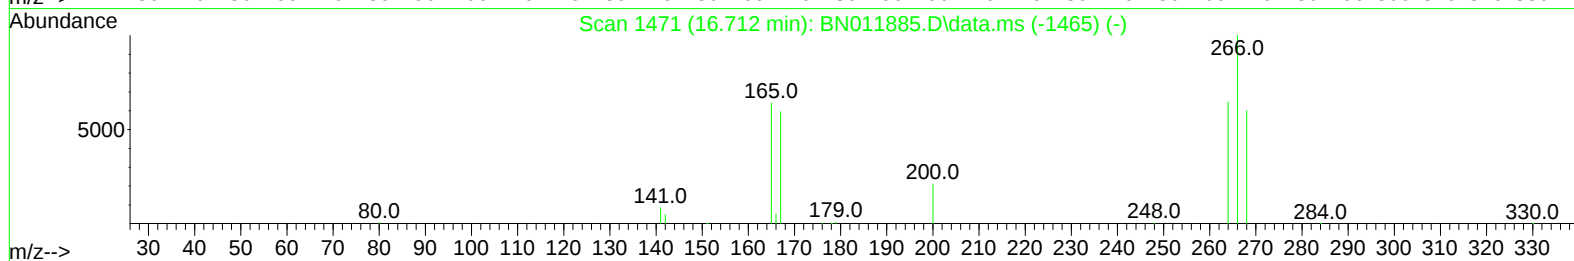
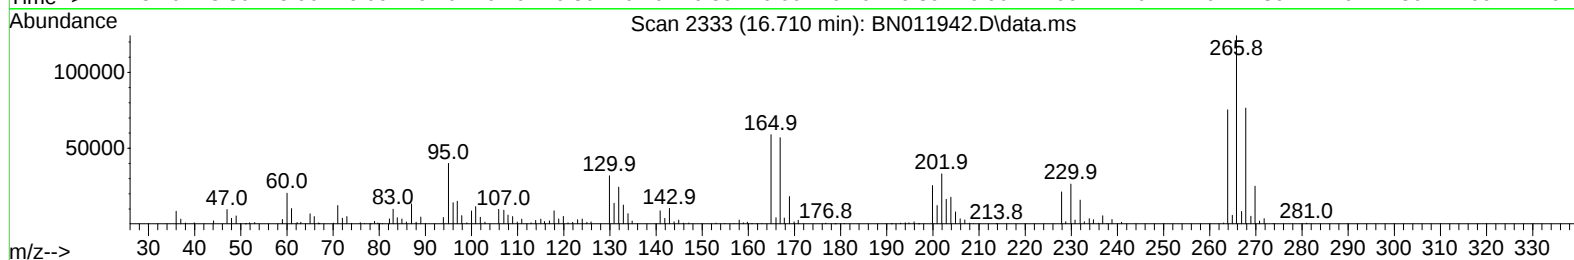


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN092520\  
Data File : BN011942.D  
Acq On : 25 Sep 2020 09:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 06:05:38 2020  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN092320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 25 11:18:41 2020  
Response via : Initial Calibration

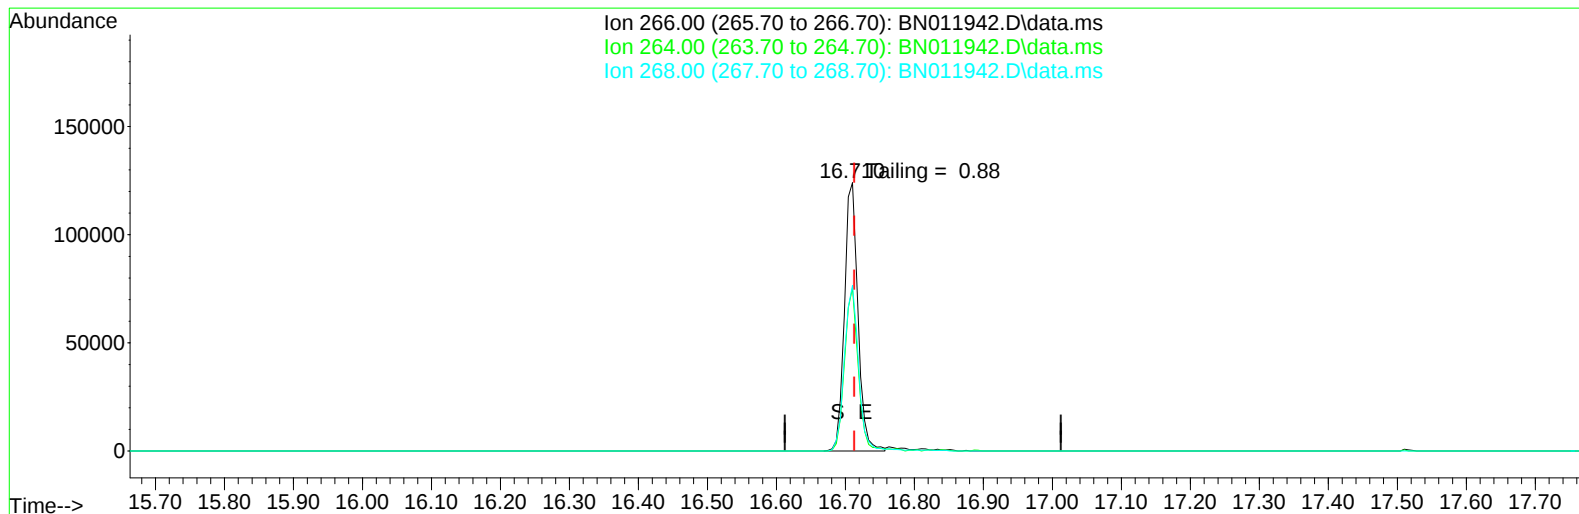

TIC: BN011942.D\data.ms

**(24) Pentachlorophenol**

16.710min (-0.002) 0.00 ng

response 168424

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 266.00 | 100.00 | 100.00 |
| 264.00 | 64.00  | 61.80  |
| 268.00 | 65.50  | 65.48  |
| 0.00   | 0.00   | 0.00   |