
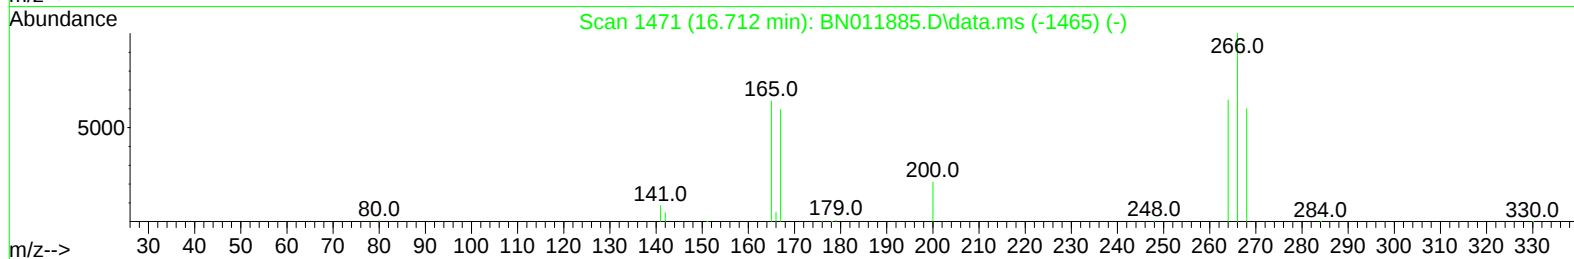
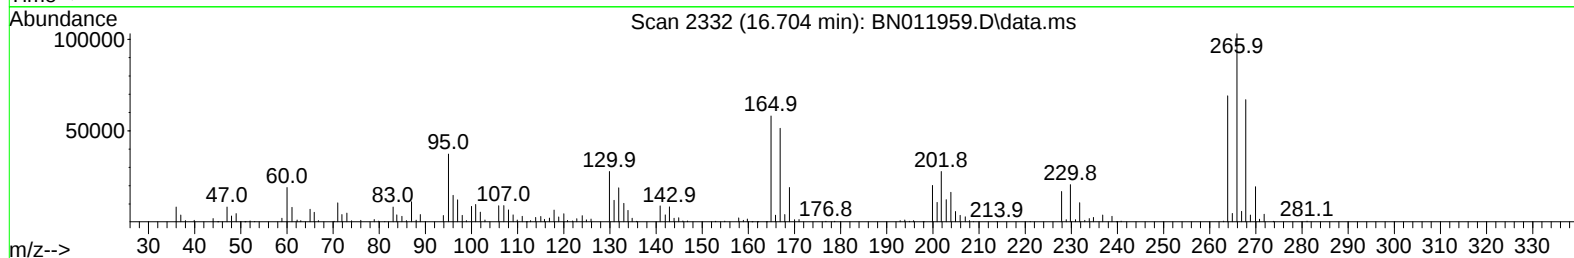


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092520\
Data File : BN011959.D
Acq On : 25 Sep 2020 21:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 06:10:01 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 11:18:41 2020
Response via : Initial Calibration

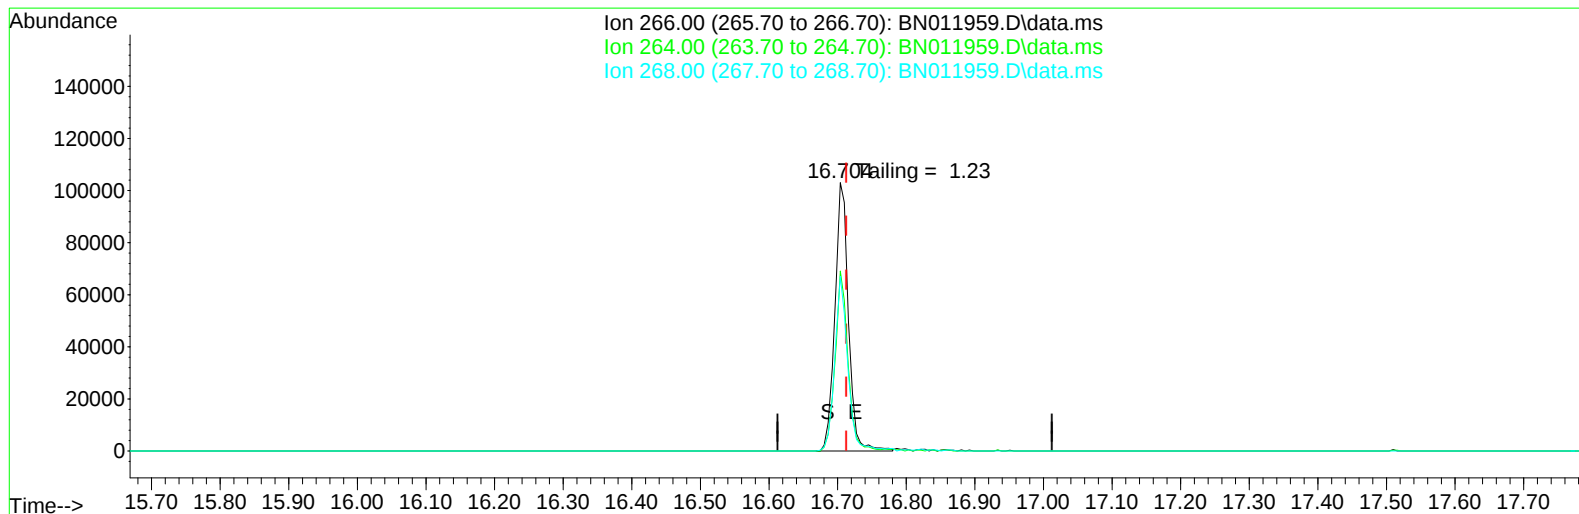

TIC: BN011959.D\data.ms

(24) Pentachlorophenol

16.704min (-0.009) 0.00 ng

response 141768

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.00	63.54
268.00	65.50	62.84
0.00	0.00	0.00