

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092520\
 Data File : BN011974.D
 Acq On : 26 Sep 2020 07:27
 Operator : CG/JU
 Sample : L4119-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DUP05-20200921

Quant Time: Sep 26 08:49:59 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 25 11:18:41 2020
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.683	152	1729	0.40	ng	0.00
7) Naphthalene-d8	10.453	136	7111	0.40	ng	# 0.00
13) Acenaphthene-d10	14.306	164	3917	0.40	ng	0.00
19) Phenanthrene-d10	17.053	188	7675	0.40	ng	0.00
29) Chrysene-d12	21.248	240	6792	0.40	ng	#-0.01
36) Perylene-d12	23.460	264	6984	0.40	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.283	112	680	0.11	ng	0.00
5) Phenol-d6	6.853	99	429	0.06	ng	0.00
8) Nitrobenzene-d5	8.818	82	2180	0.30	ng	0.00
11) 2-Methylnaphthalene-d10	12.042	152	3218	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.803	330	531	0.28	ng	0.00
15) 2-Fluorobiphenyl	12.923	172	4180	0.28	ng	-0.01
27) Fluoranthene-d10	19.087	212	7387	0.33	ng	0.00
31) Terphenyl-d14	19.693	244	6577	0.42	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.245	88	1633	0.54	ng	# 88
34) Bis(2-ethylhexyl)phtha...	21.174	149	787	0.05	ng	# 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092520\
Data File : BN011974.D
Acq On : 26 Sep 2020 07:27
Operator : CG/JU
Sample : L4119-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DUP05-20200921

Quant Time: Sep 26 08:49:59 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 11:18:41 2020
Response via : Initial Calibration



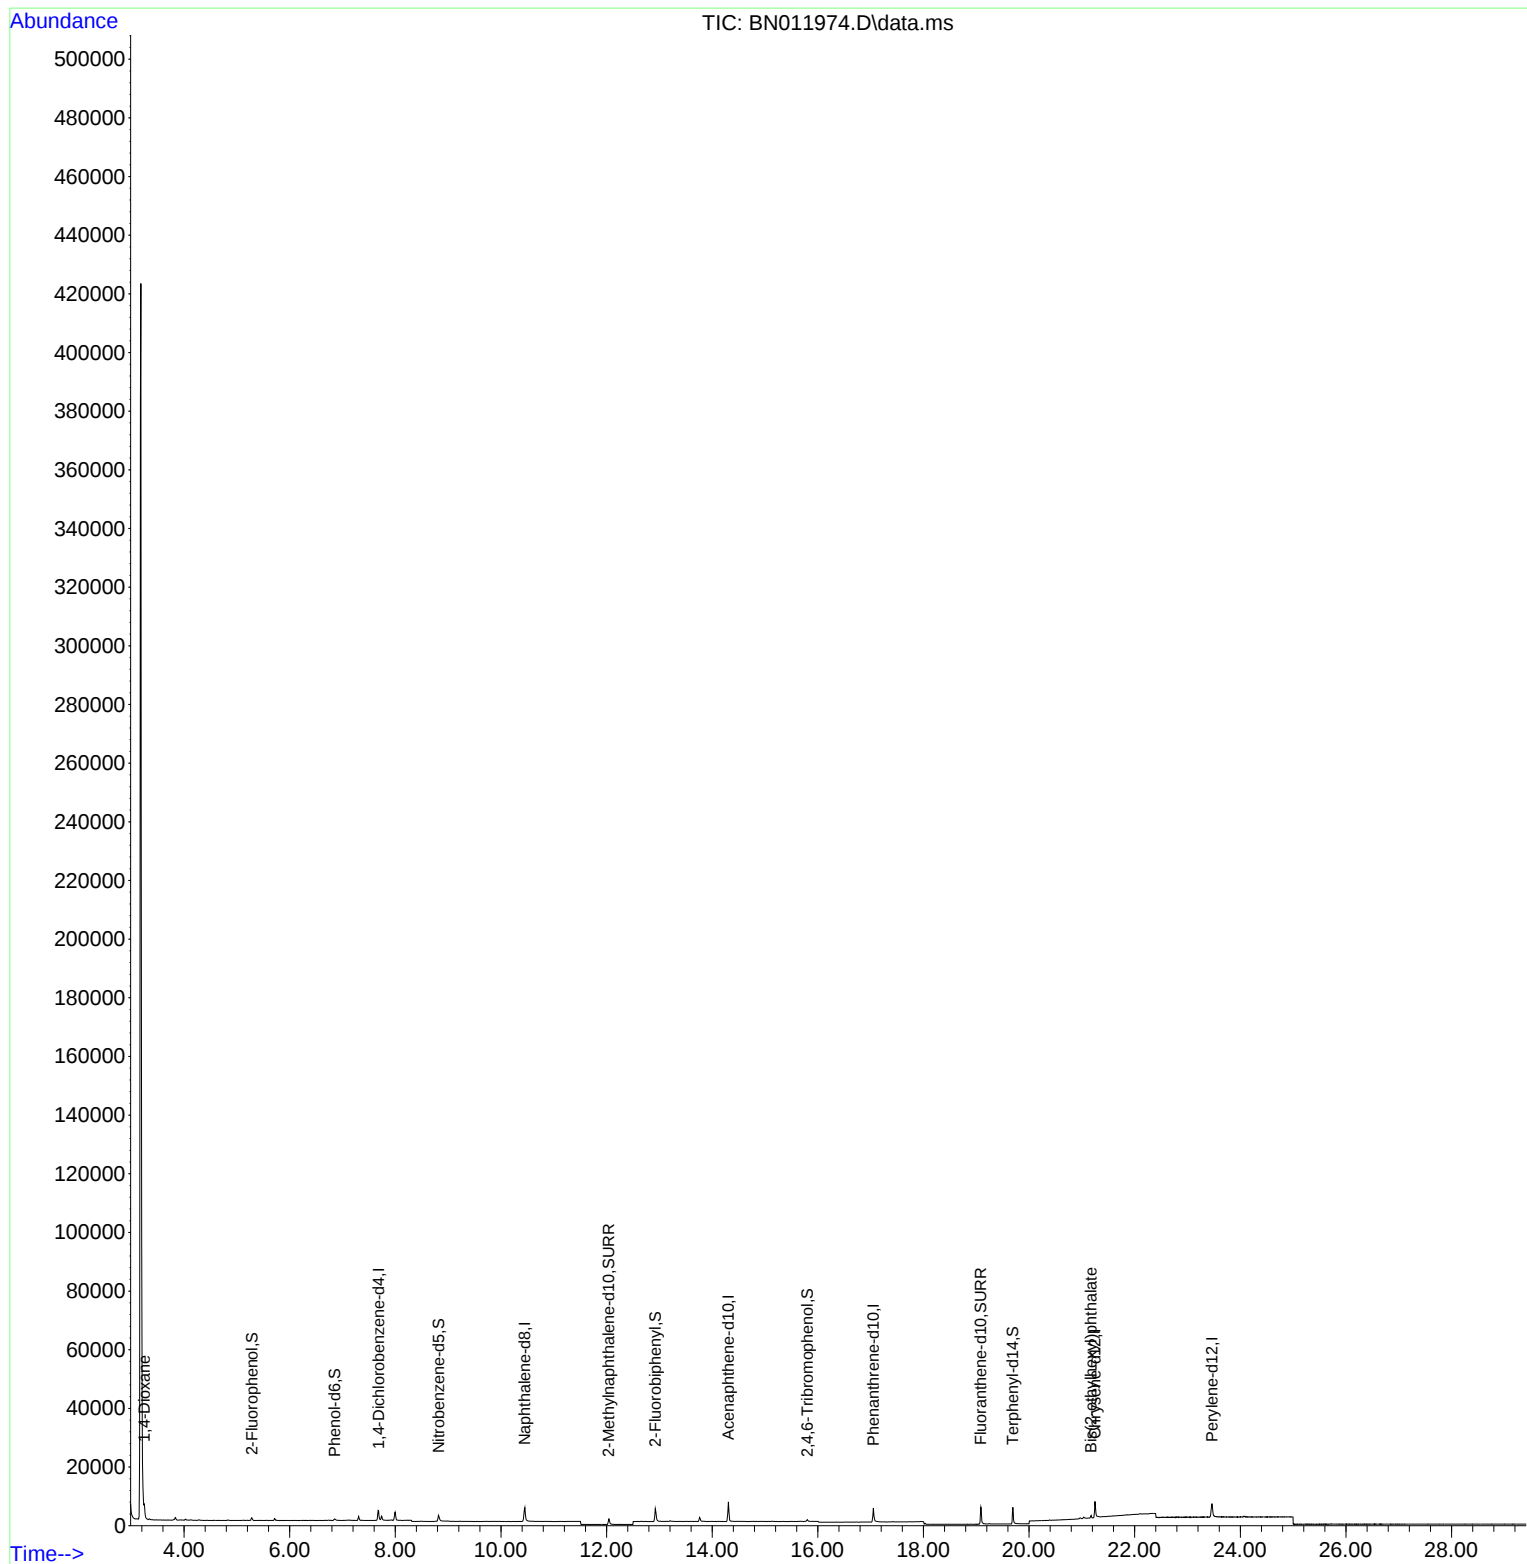




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.683 min Scan# 584
Delta R.T. -0.000 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27




Instrument :
BNA_N
ClientSampleId :
DUP05-20200921

Tgt Ion:152 Resp: 1729
Ion Ratio Lower Upper
152 100
150 149.3 118.3 177.5
115 75.1 51.3 76.9

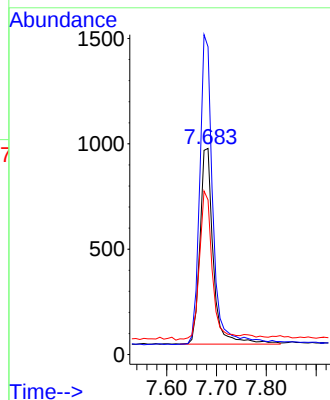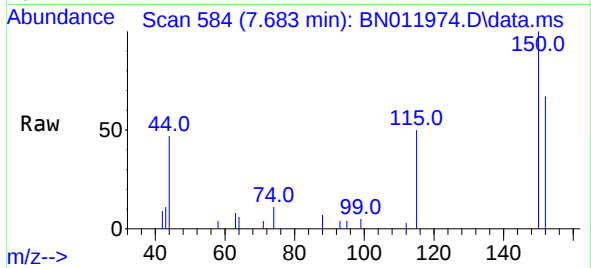


#2
1,4-Dioxane
Concen: 0.54 ng
RT: 3.245 min Scan# 33
Delta R.T. -0.008 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27


Tgt Ion: 88 Resp: 1633
Ion Ratio Lower Upper
88 100
58 86.5 63.3 94.9
43 53.2 33.0 49.4

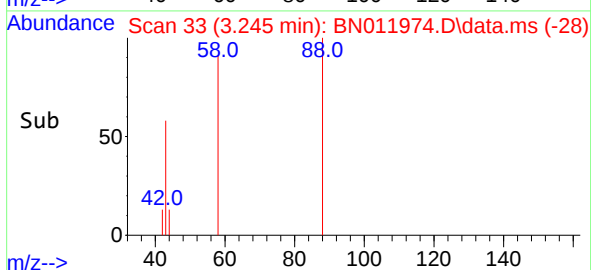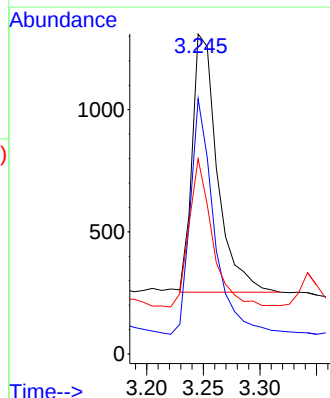


Abundance Scan 287 (5.291 min): BN011885.D\data.ms (-28

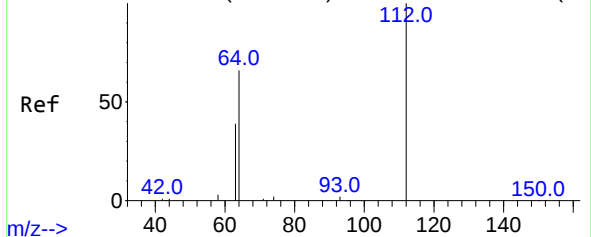

m/z--> Scan 286 (5.283 min): BN011974.D\data.ms

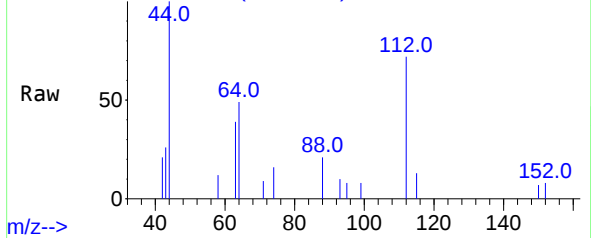


Abundance Scan 286 (5.283 min): BN011974.D\data.ms (-26

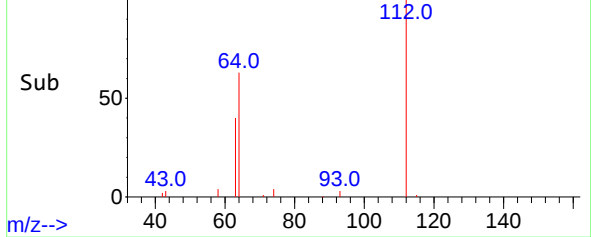


m/z-->


Abundance Scan 482 (6.861 min): BN011885.D\data.ms (-47

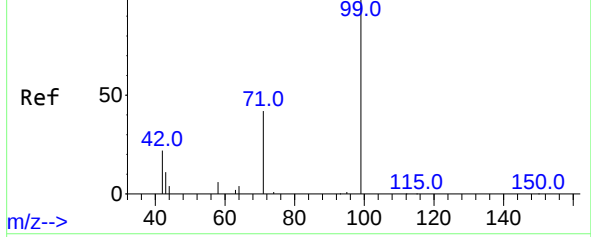

m/z--> Scan 481 (6.853 min): BN011974.D\data.ms

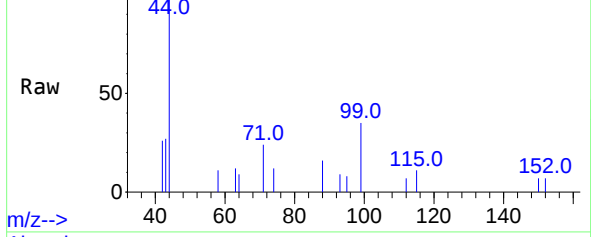

Abundance Scan 481 (6.853 min): BN011974.D\data.ms (-46

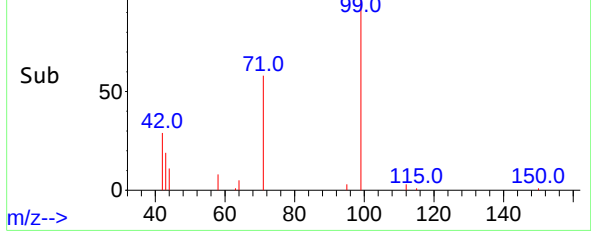

m/z-->

#4

2-Fluorophenol

Concen: 0.11 ng

RT: 5.283 min Scan# 286

Delta R.T. 0.000 min

Lab File: BN011974.D

Acq: 26 Sep 2020 07:27

Tgt Ion: 112 Resp: 680


Ion Ratio Lower Upper

112 100

64 71.3 49.0 73.6

63 45.3 31.8 47.6

Abundance

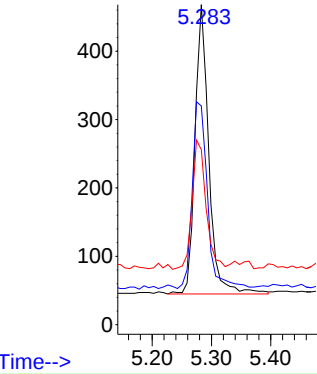

Time-->

#5

Phenol-d6

Concen: 0.06 ng

RT: 6.853 min Scan# 481

Delta R.T. 0.000 min

Lab File: BN011974.D

Acq: 26 Sep 2020 07:27

Tgt Ion: 99 Resp: 429


Ion Ratio Lower Upper

99 100

42 39.2 23.4 35.0#

71 60.6 38.1 57.1#

Abundance

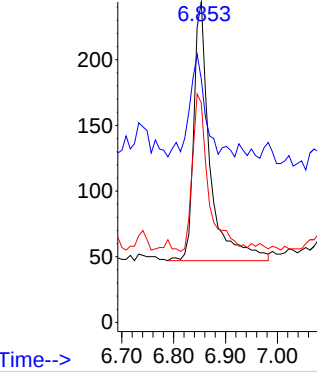


Time-->

Instrument :

BNA_N

ClientSampleId :





DUP05-20200921

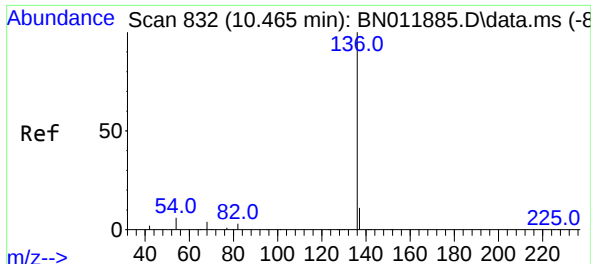

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.453 min Scan# 831
Delta R.T. 0.000 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27




Instrument :
BNA_N
ClientSampleId :
DUP05-20200921

Tgt Ion:	136	Resp:	7111
Ion	Ratio	Lower	Upper
136	100		
137	12.0	9.5	14.3
54	9.3	5.6	8.4#
68	5.5	3.2	4.8#

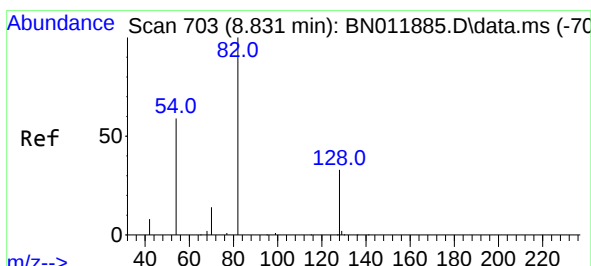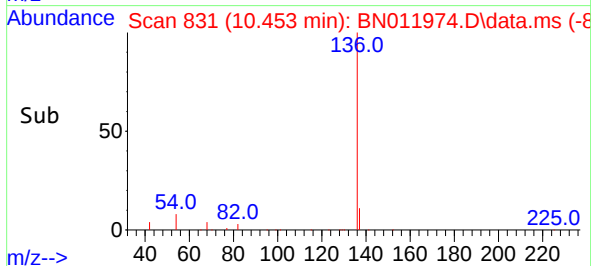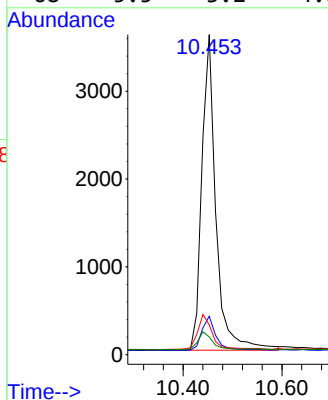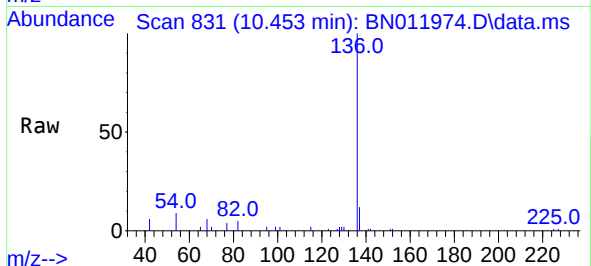

#8
Nitrobenzene-d5
Concen: 0.30 ng
RT: 8.818 min Scan# 702
Delta R.T. 0.000 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27

Tgt Ion:	82	Resp:	2180
Ion	Ratio	Lower	Upper
82	100		
128	33.3	34.2	51.2#
54	69.0	43.1	64.7#

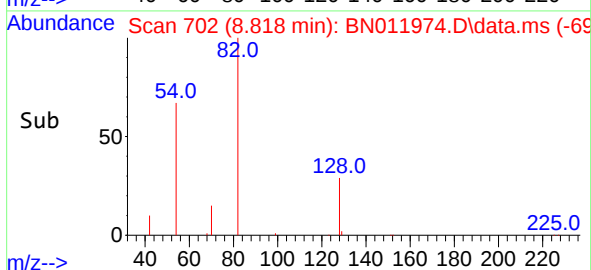
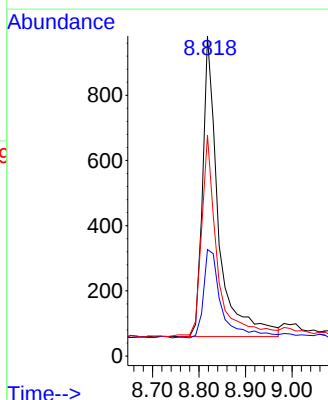





#11
2-Methylnaphthalene-d10
Concen: 0.29 ng
RT: 12.042 min Scan# 1033
Delta R.T. -0.004 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27




Instrument :
BNA_N
ClientSampleId :
DUP05-20200921

Tgt Ion:152 Resp: 3218
Ion Ratio Lower Upper
152 100
151 20.0 16.7 25.1

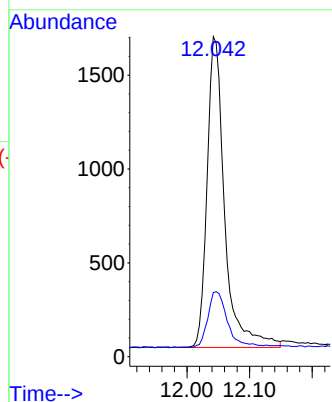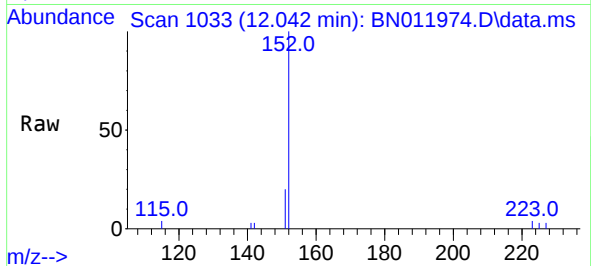

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.306 min Scan# 1279
Delta R.T. 0.000 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27

Tgt Ion:164 Resp: 3917
Ion Ratio Lower Upper
164 100
162 103.5 83.6 125.4
160 50.6 41.2 61.8


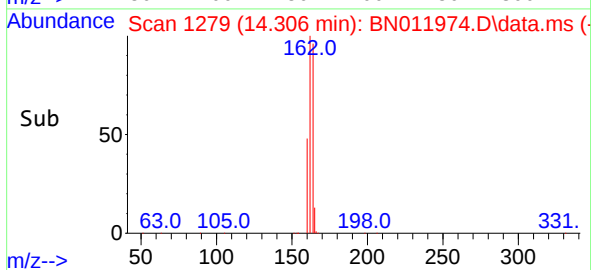
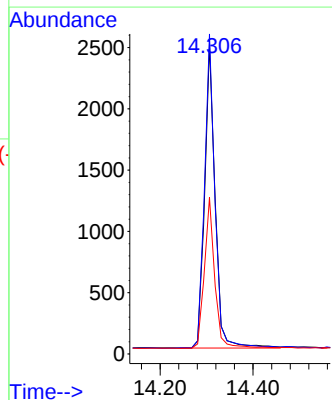





#14
2,4,6-Tribromophenol
Concen: 0.28 ng
RT: 15.803 min Scan# 1397
Delta R.T. 0.000 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27




Instrument :
BNA_N
ClientSampleId :
DUP05-20200921

Tgt Ion:330 Resp: 531
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 51.0 33.7 50.5#

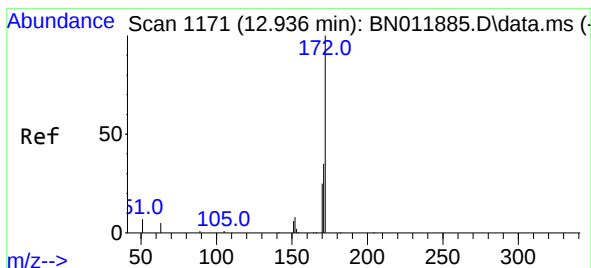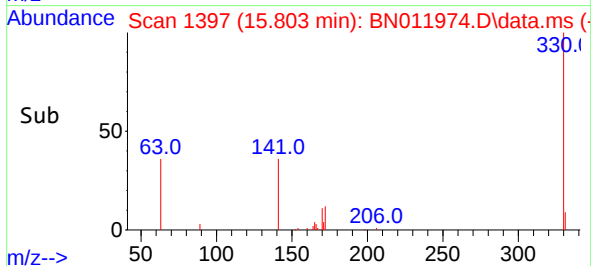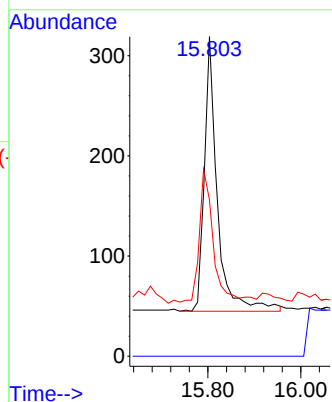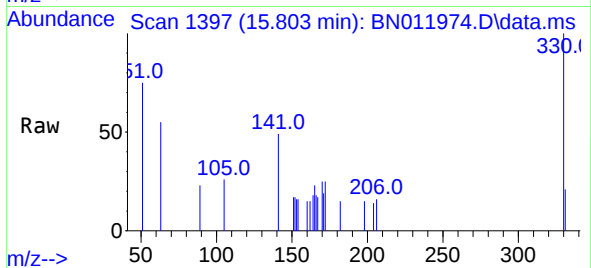

#15
2-Fluorobiphenyl
Concen: 0.28 ng
RT: 12.923 min Scan# 1170
Delta R.T. -0.013 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27

Tgt Ion:172 Resp: 4180
Ion Ratio Lower Upper
172 100
171 36.3 27.4 41.2
170 26.6 17.8 26.6

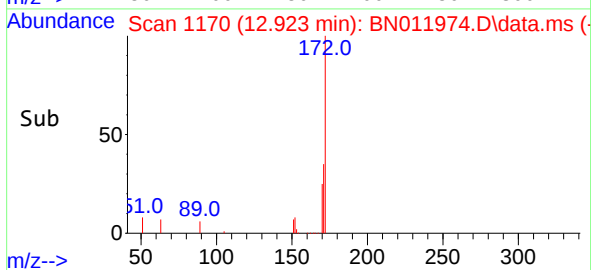
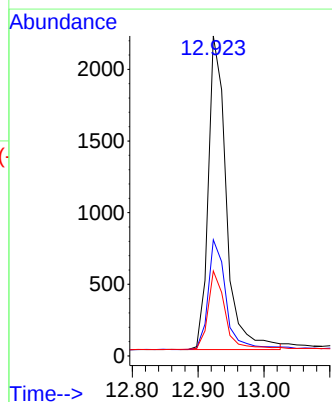
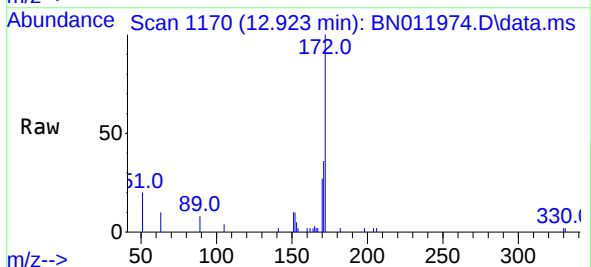




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.053 min Scan# 1499
Delta R.T. 0.000 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27




Instrument :
BNA_N
ClientSampleId :
DUP05-20200921

Tgt Ion:188 Resp: 7675
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.0 7.7 11.5

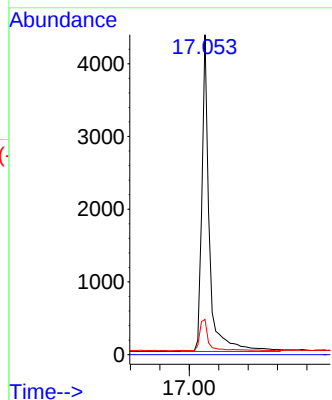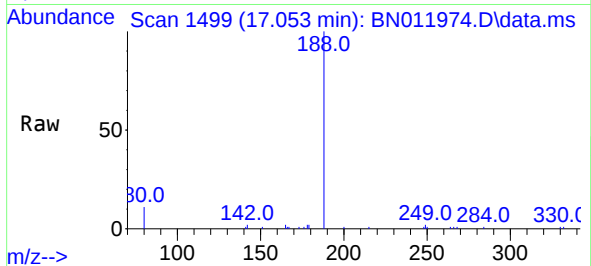

#27
Fluoranthene-d10
Concen: 0.33 ng
RT: 19.087 min Scan# 1794
Delta R.T. -0.005 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27

Tgt Ion:212 Resp: 7387
Ion Ratio Lower Upper
212 100
106 12.9 6.4 9.6#
104 8.5 3.9 5.9#

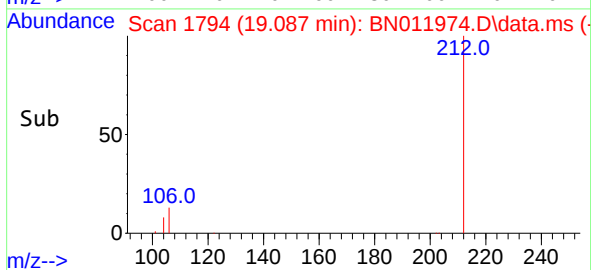
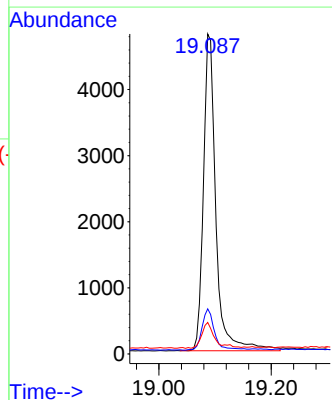





#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.248 min Scan# 2096
Delta R.T. -0.011 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27




Instrument :
BNA_N
ClientSampleId :
DUP05-20200921


Tgt Ion:240 Resp: 6792
Ion Ratio Lower Upper
240 100
120 15.7 3.5 5.3#
236 27.7 20.5 30.7

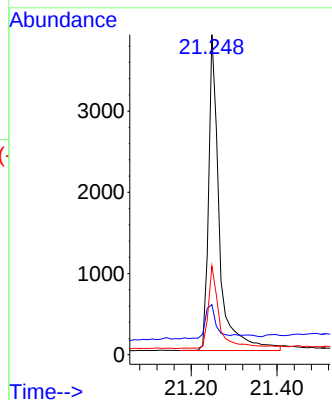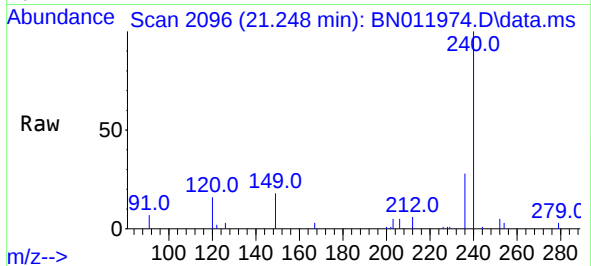

#31
Terphenyl-d14
Concen: 0.42 ng
RT: 19.693 min Scan# 1916
Delta R.T. -0.005 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27

Tgt Ion:244 Resp: 6577
Ion Ratio Lower Upper
244 100
212 10.7 7.3 10.9
122 15.2 7.8 11.6#


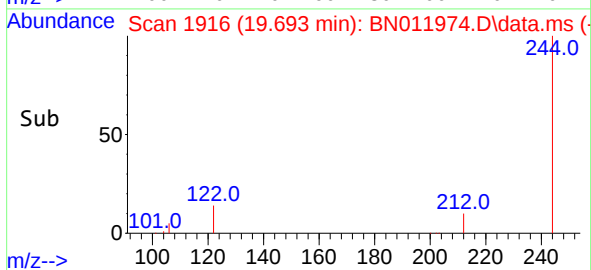
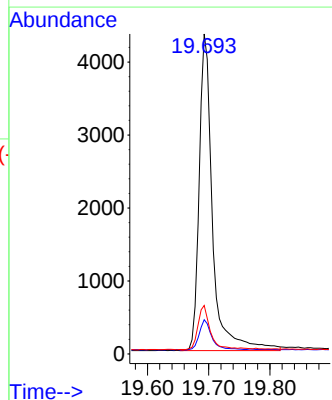



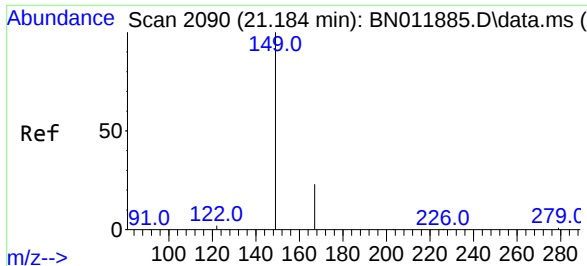

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.05 ng
RT: 21.174 min Scan# 2089
Delta R.T. 0.000 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27

Instrument :
BNA_N
ClientSampleId :
DUP05-20200921

Tgt Ion:149 Resp: 787
Ion Ratio Lower Upper
149 100
167 25.2 23.6 35.4
279 7.9 4.0 6.0#

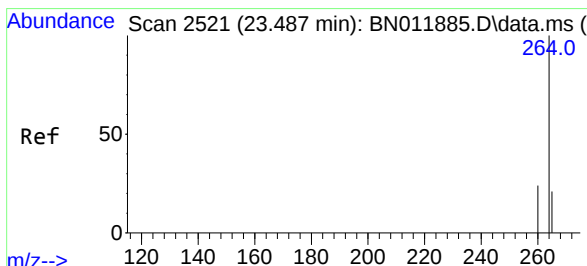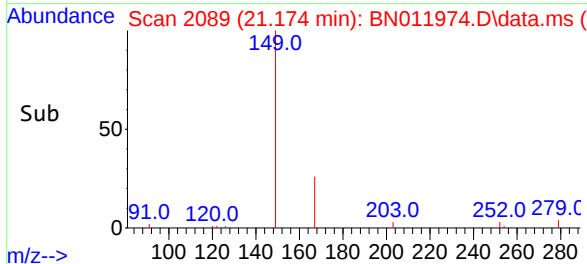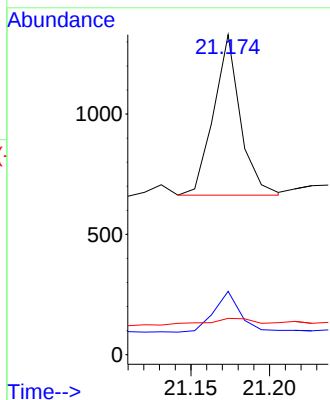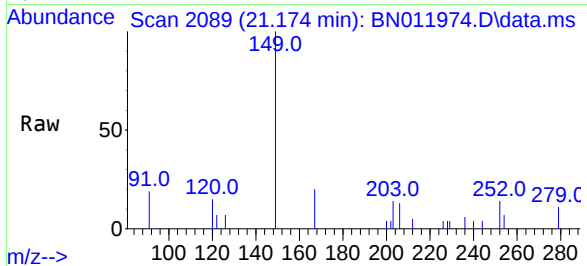

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.460 min Scan# 2513
Delta R.T. -0.010 min
Lab File: BN011974.D
Acq: 26 Sep 2020 07:27

Tgt Ion:264 Resp: 6984
Ion Ratio Lower Upper
264 100
260 24.6 19.6 29.4
265 70.2 38.6 58.0#

