


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092520\
 Data File : BN011942.D
 Acq On : 25 Sep 2020 09:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 25 11:18:41 2020

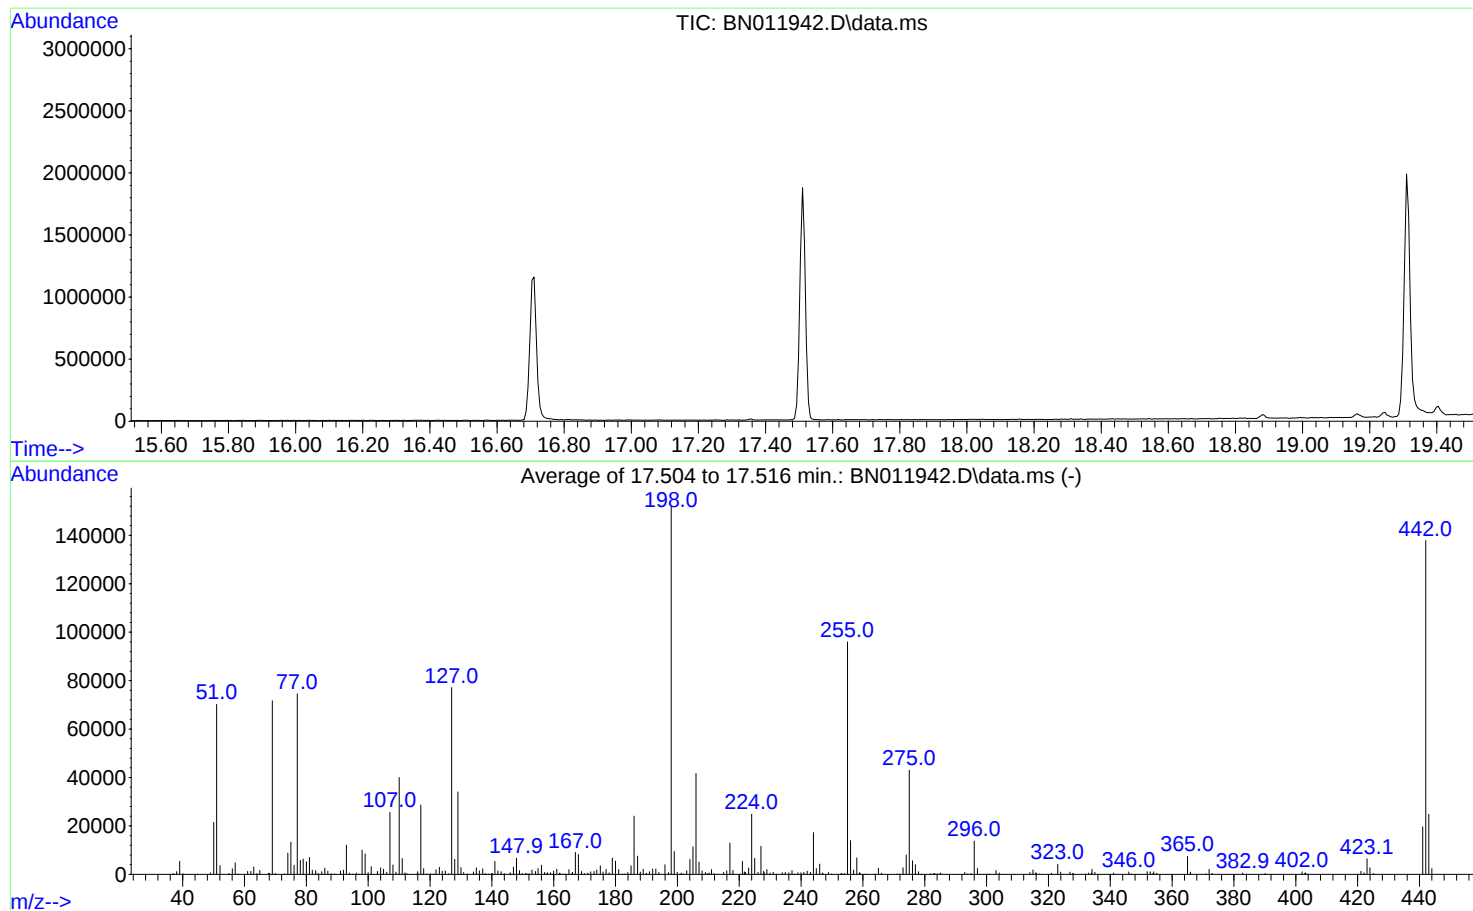

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	70179	PASS
68	69	0.00	2	0.7	472	PASS
69	198	0.00	100	47.2	71707	PASS
70	69	0.00	2	0.6	411	PASS
127	198	10	80	50.8	77120	PASS
197	198	0.00	2	0.5	766	PASS
198	198	100	100	100.0	151893	PASS
199	198	5	9	6.2	9487	PASS
275	198	10	60	28.3	43027	PASS
365	198	1	100	4.9	7419	PASS
441	198	0.01	100	12.9	19610	PASS
442	198	50	100	90.7	137824	PASS
443	442	15	24	18.0	24839	PASS