
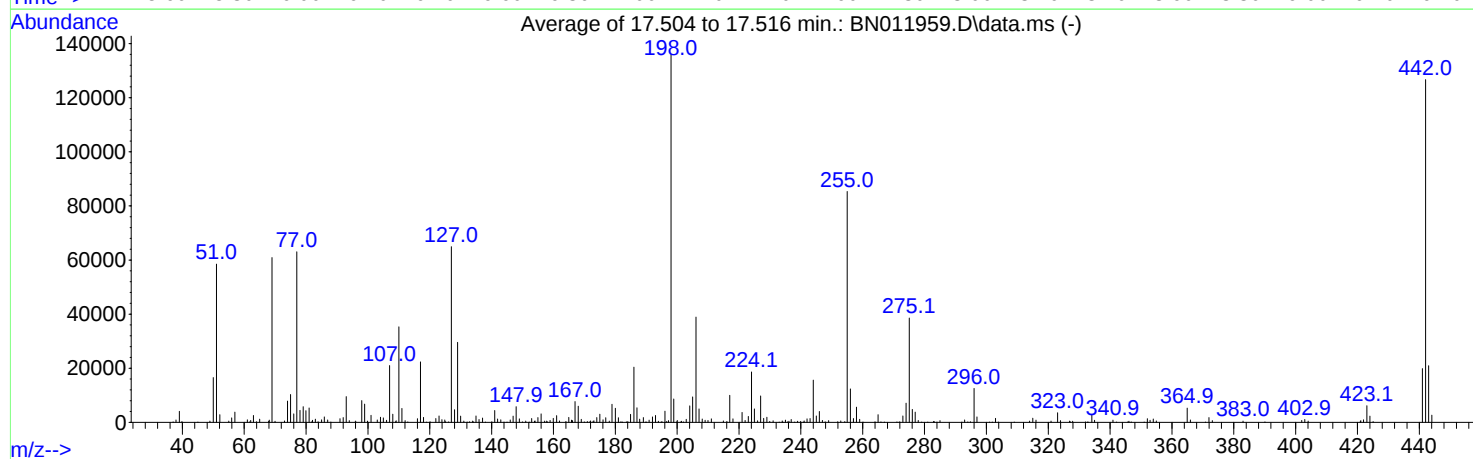


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092520\
 Data File : BN011959.D
 Acq On : 25 Sep 2020 21:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 25 11:18:41 2020

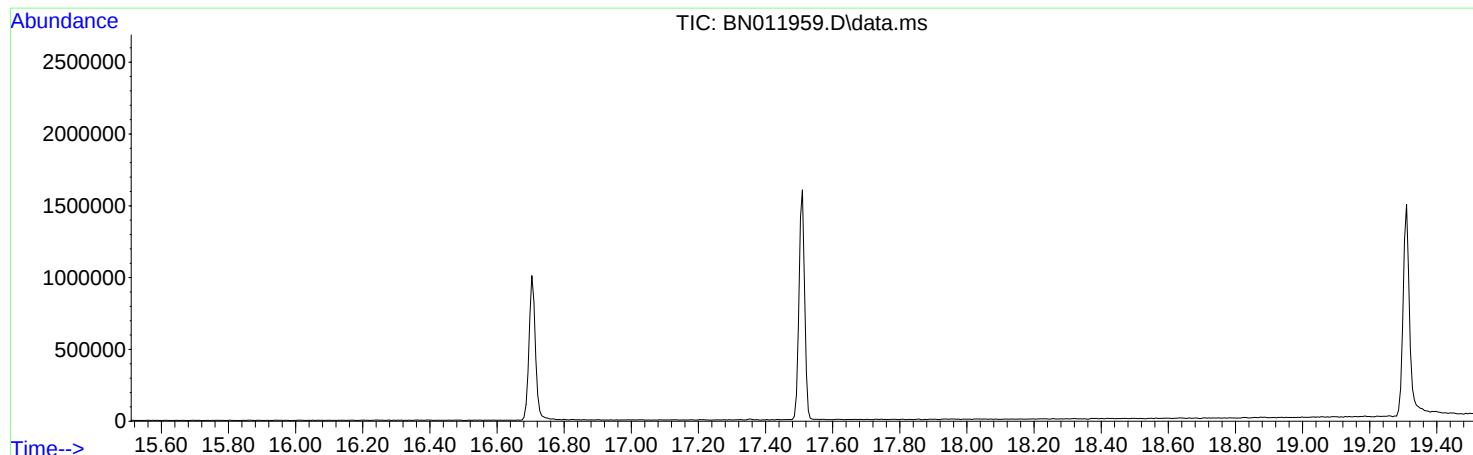

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	58525	PASS
68	69	0.00	2	1.4	835	PASS
69	198	0.00	100	44.8	60928	PASS
70	69	0.00	2	0.6	396	PASS
127	198	10	80	47.8	64949	PASS
197	198	0.00	2	0.5	637	PASS
198	198	100	100	100.0	135976	PASS
199	198	5	9	6.4	8635	PASS
275	198	10	60	28.4	38573	PASS
365	198	1	100	3.9	5242	PASS
441	198	0.01	100	14.6	19865	PASS
442	198	50	100	93.2	126709	PASS
443	442	15	24	16.5	20920	PASS