
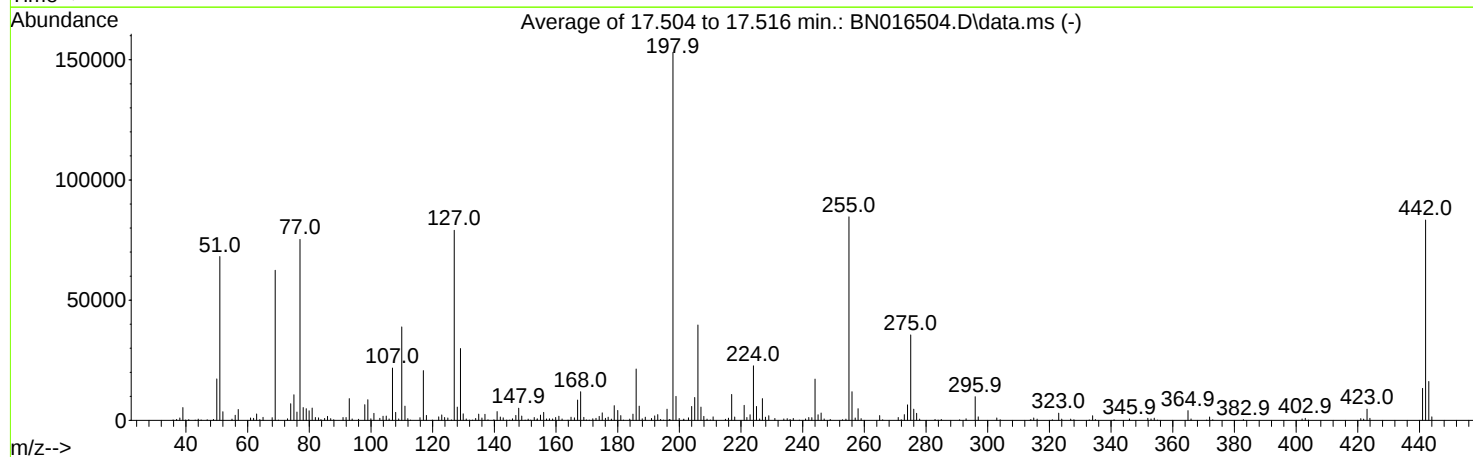


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092521\
 Data File : BN016504.D
 Acq On : 26 Sep 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 03:35:41 2021

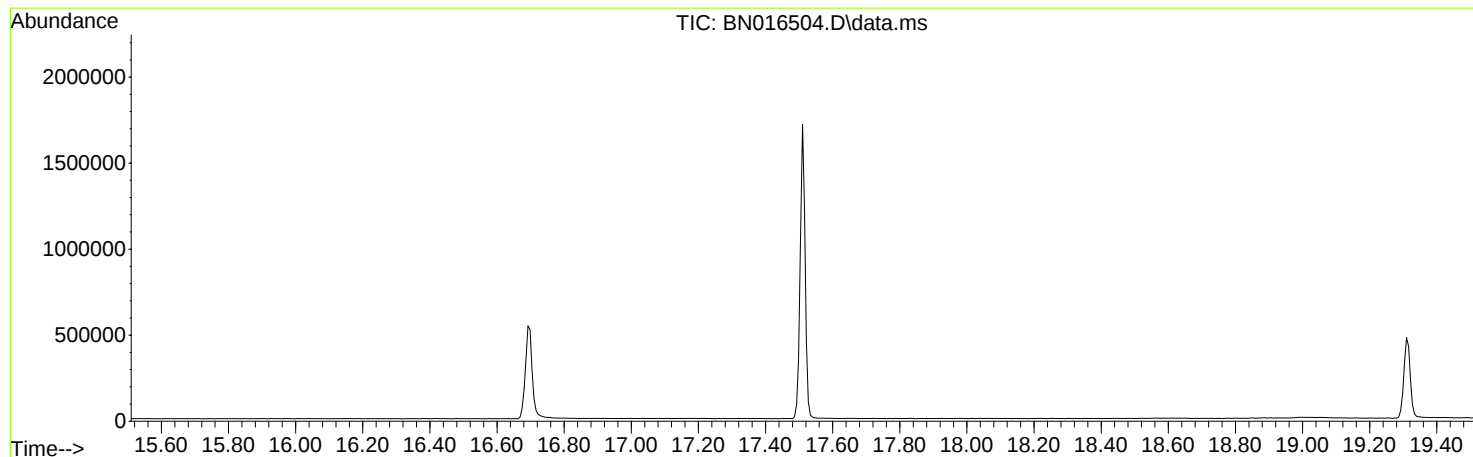




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	68197	PASS
68	69	0.00	2	1.8	1119	PASS
69	198	0.00	100	40.8	62419	PASS
70	69	0.00	2	0.2	132	PASS
127	198	10	80	51.7	79109	PASS
197	198	0.00	2	0.3	407	PASS
198	198	100	100	100.0	153035	PASS
199	198	5	9	6.5	9960	PASS
275	198	10	60	23.2	35565	PASS
365	198	1	100	2.6	4033	PASS
441	198	0.01	100	8.7	13321	PASS
442	442	50	100	100.0	83312	PASS
443	442	15	24	19.4	16191	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092521\
 Data File : BN016504.D
 Acq On : 26 Sep 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 27 07:00:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 13:04:53 2021
 Response via : Initial Calibration

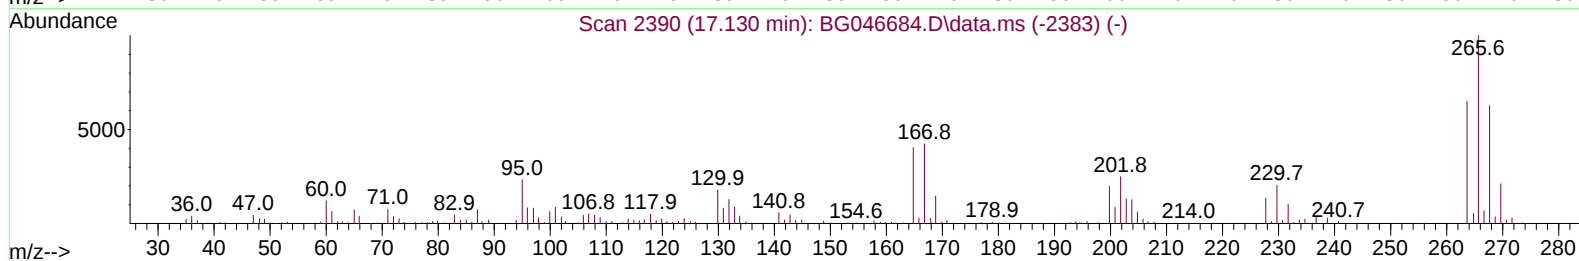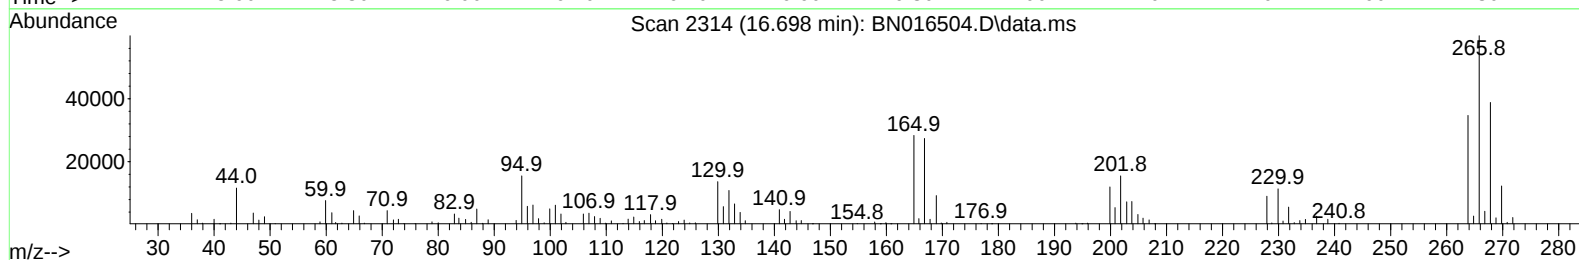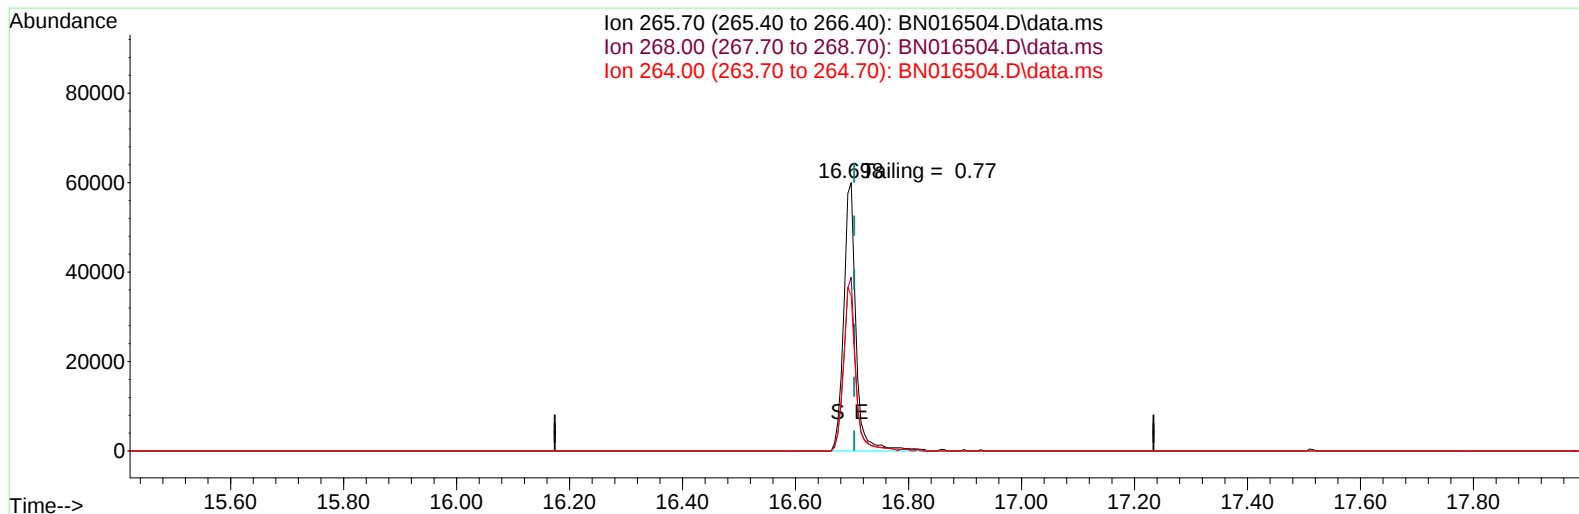

TIC: BN016504.D\data.ms

(70) Pentachlorophenol (C)

16.698min (-0.006) 16224.85 ng




response 88366

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.73
264.00	61.60	57.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092521\
 Data File : BN016504.D
 Acq On : 26 Sep 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 27 07:00:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 13:04:53 2021
 Response via : Initial Calibration

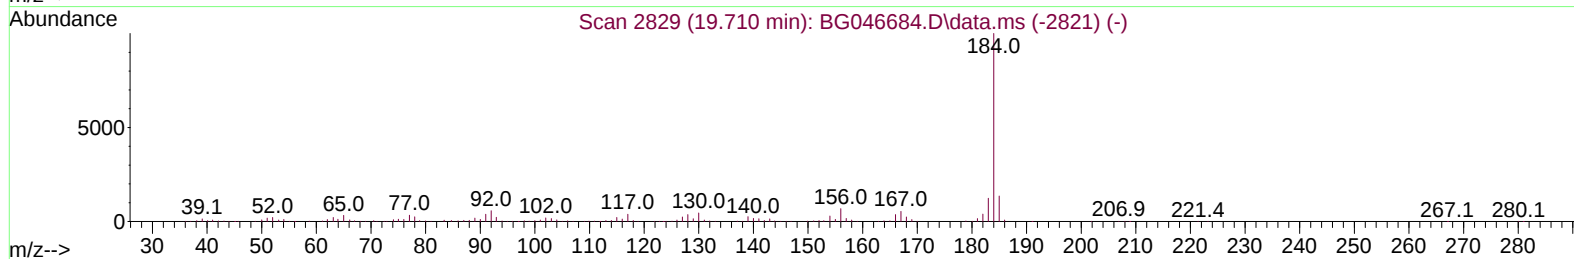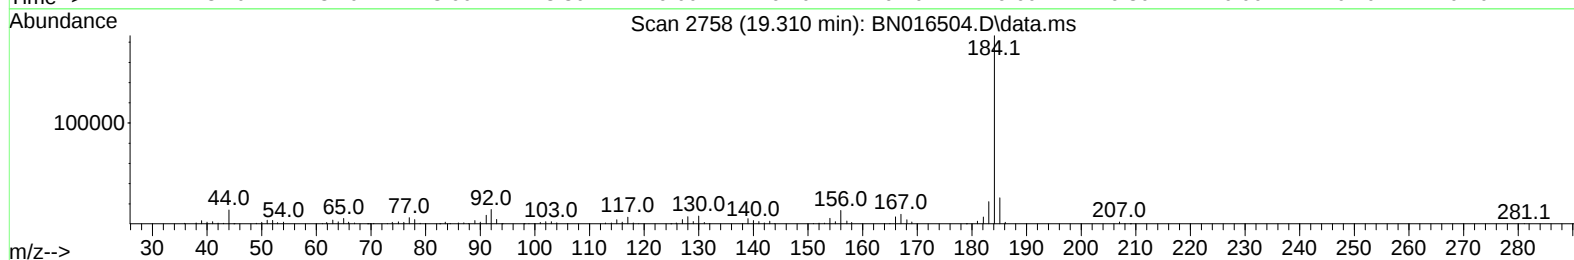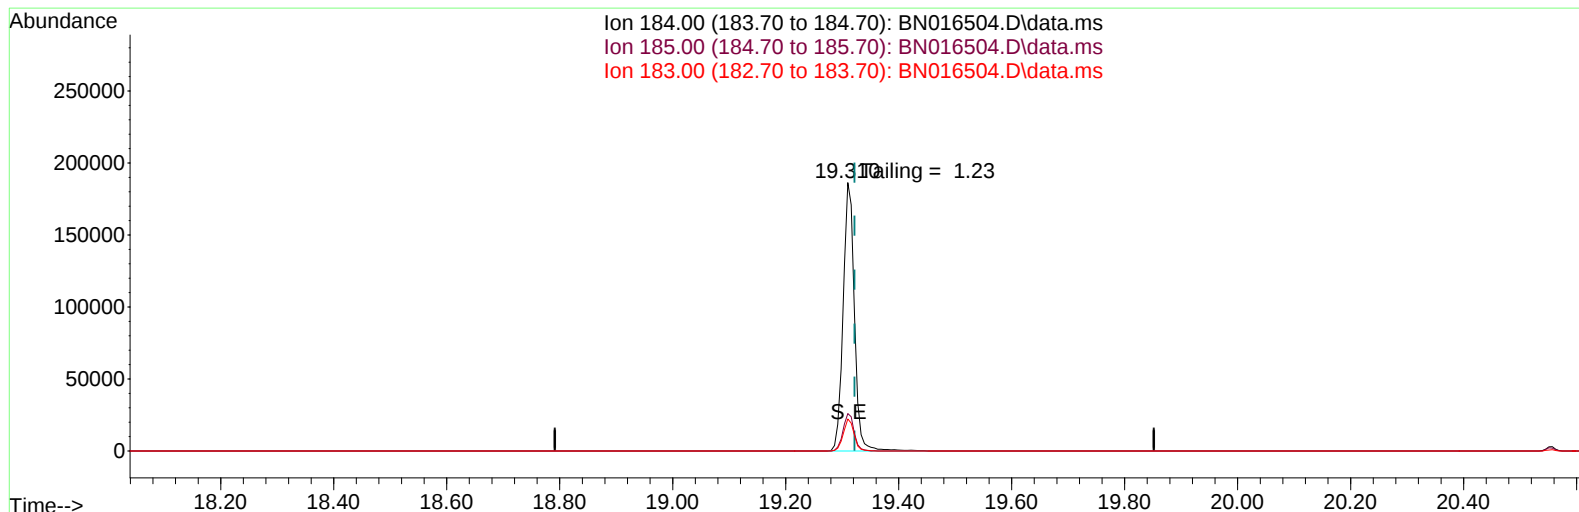

TIC: BN016504.D\data.ms

(77) Benzidine

19.310min (-0.012) 0.00 ng

response 256479

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/25/2021	BNA_N	<u>BN016504.D</u>
Compound Name	Response	Retention Time
DDT	331557	20.557
DDD	10776	20.11
DDE	429	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11205	342762	3.27

Instrument :
BNA_N
ClientSampleId :
DFTPP