
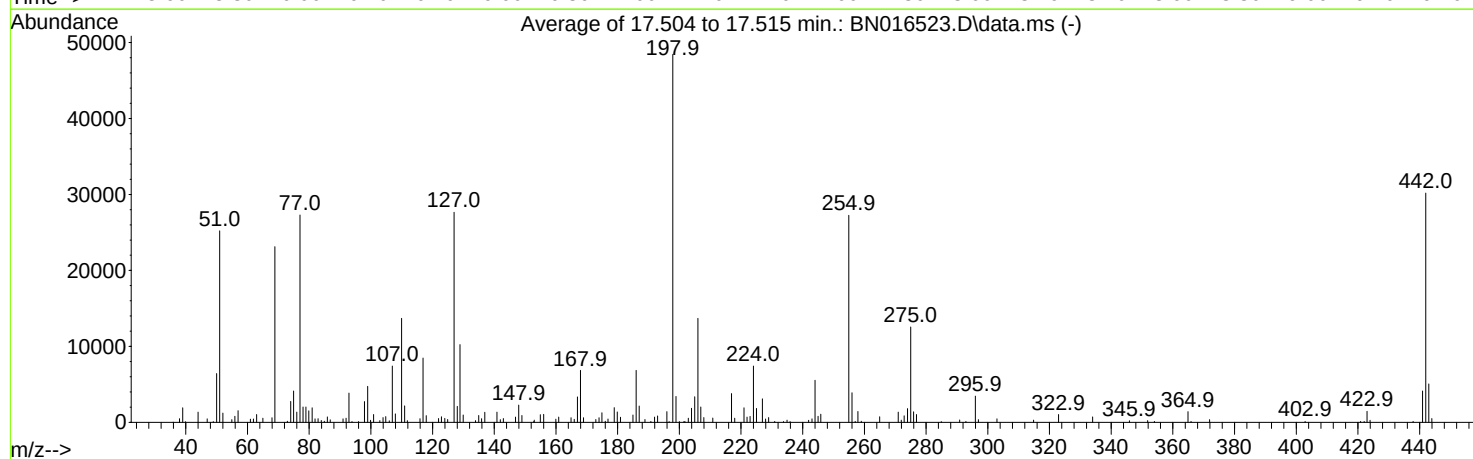


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092521\
 Data File : BN016523.D
 Acq On : 26 Sep 2021 23:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 03:35:41 2021

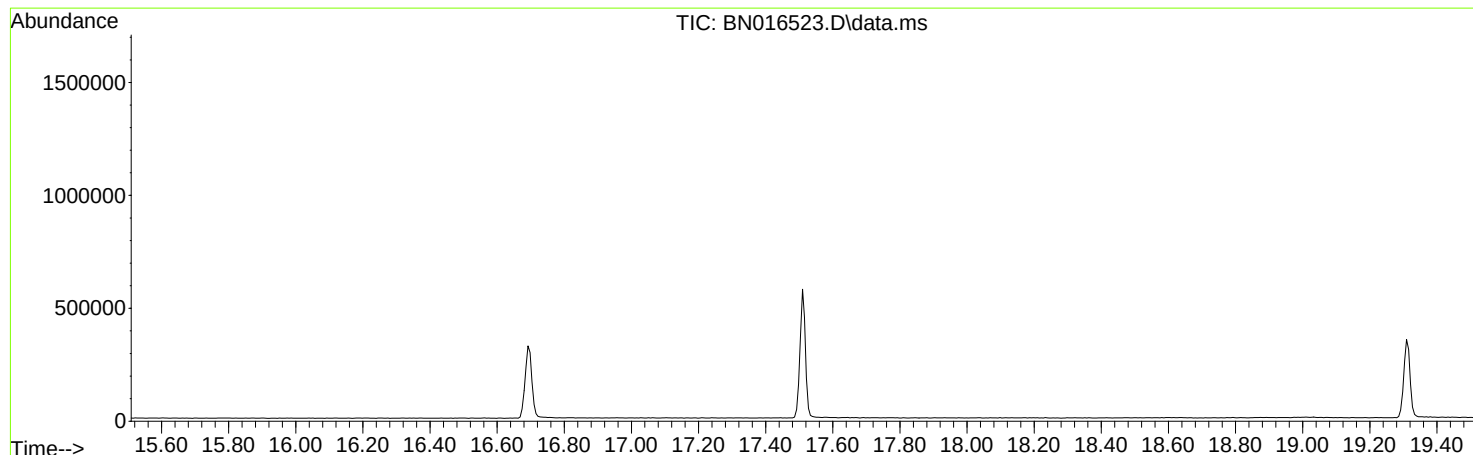

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.1	25216	PASS
68	69	0.00	2	2.6	605	FAIL*
69	198	0.00	100	47.8	23133	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.1	27656	PASS
197	198	0.00	2	0.2	117	PASS
198	198	100	100	100.0	48421	PASS
199	198	5	9	7.0	3410	PASS
275	198	10	60	25.9	12548	PASS
365	198	1	100	2.9	1421	PASS
441	198	0.01	100	8.5	4128	PASS
442	442	50	100	100.0	30189	PASS
443	442	15	24	16.8	5059	PASS