
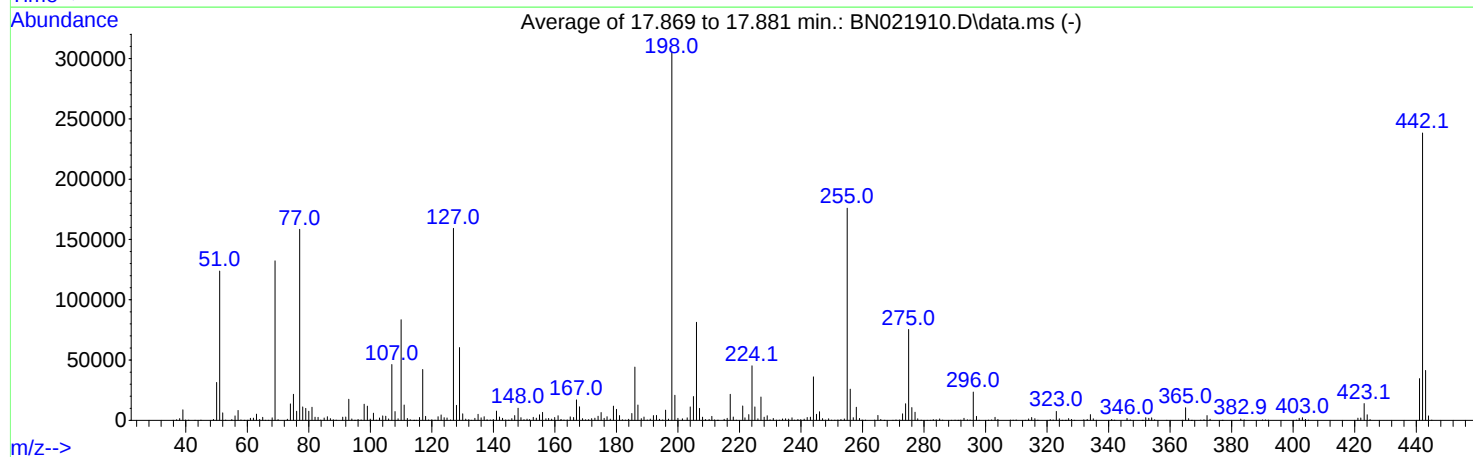


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092622\
 Data File : BN021910.D
 Acq On : 26 Sep 2022 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 04:21:32 2022

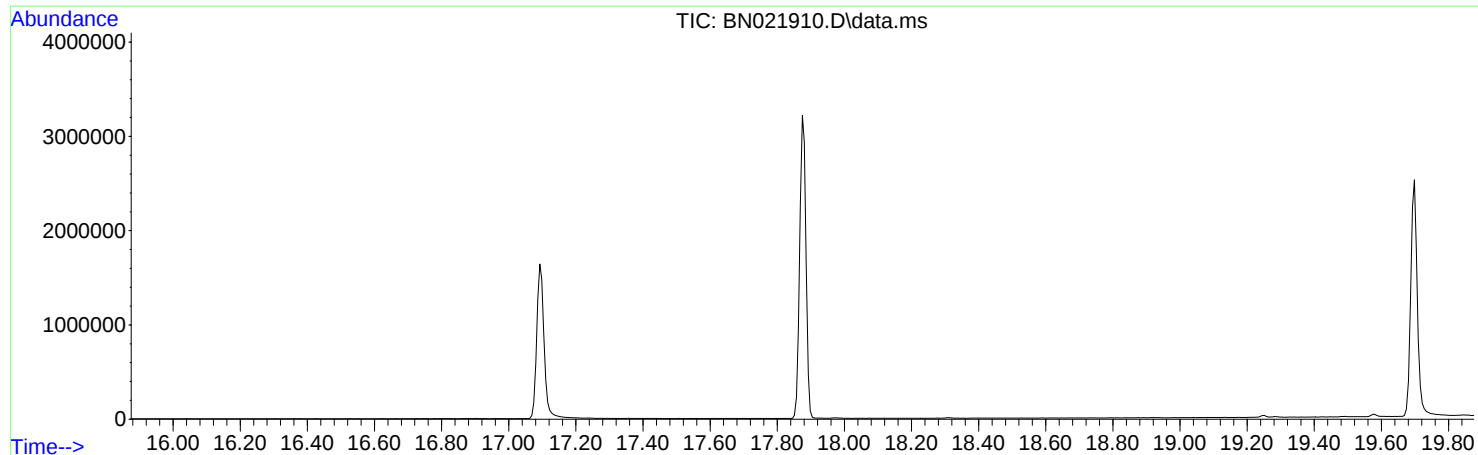




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	123763	PASS
68	69	0.00	2	1.6	2172	PASS
69	198	0.00	100	43.4	132245	PASS
70	69	0.00	2	0.5	666	PASS
127	198	10	80	52.2	159211	PASS
197	198	0.00	2	0.4	1082	PASS
198	198	100	100	100.0	305024	PASS
199	198	5	9	6.8	20779	PASS
275	198	10	60	24.7	75301	PASS
365	198	1	100	3.4	10483	PASS
441	198	0.01	100	11.3	34576	PASS
442	442	50	100	100.0	238280	PASS
443	442	15	24	17.4	41384	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092622\
Data File : BN021910.D
Acq On : 26 Sep 2022 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 26 17:43:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 17:42:56 2022
Response via : Initial Calibration

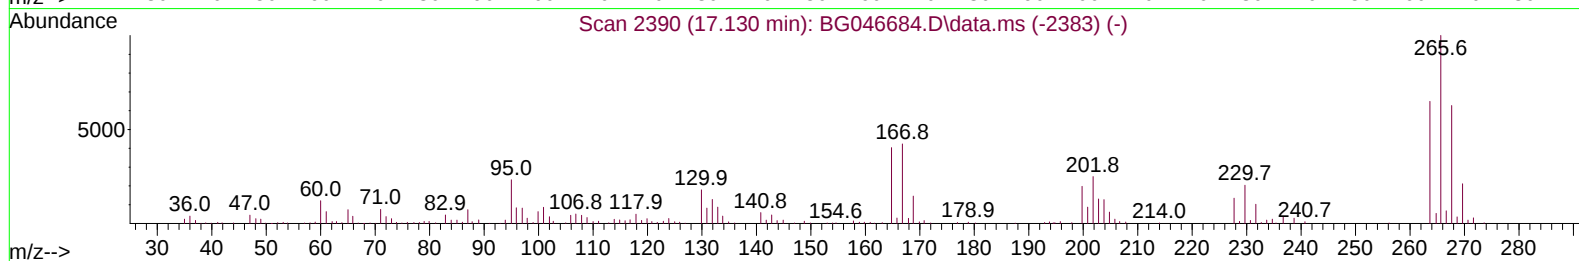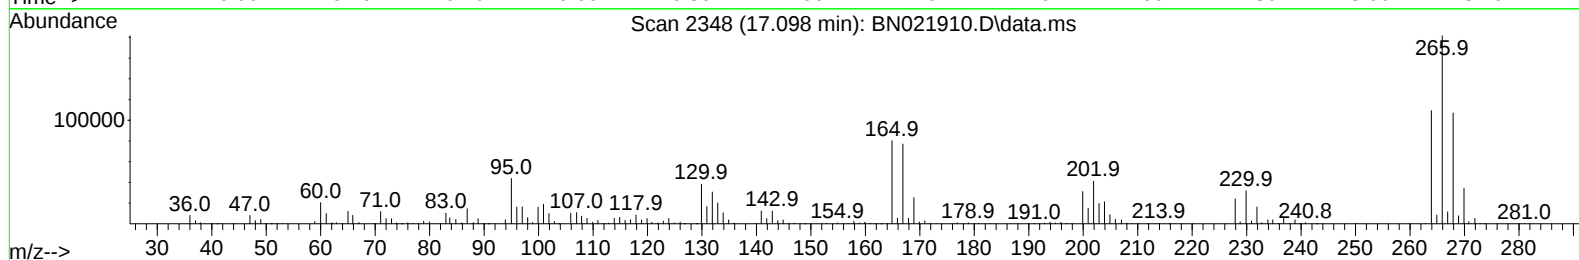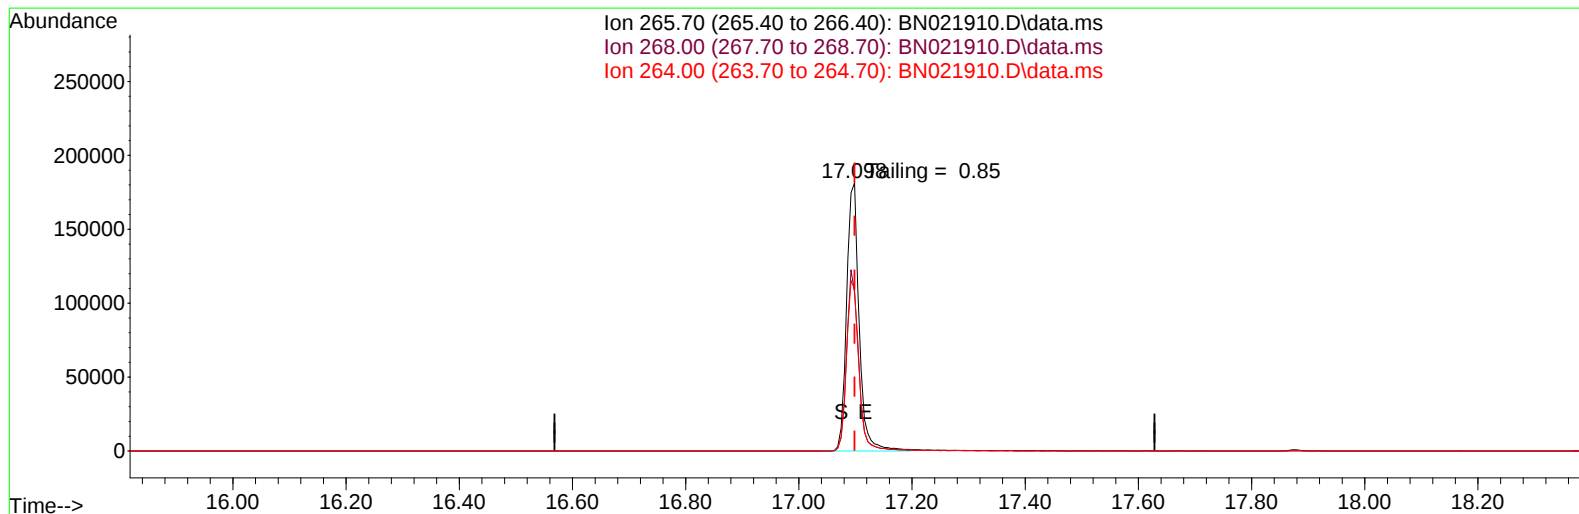

TIC: BN021910.D\data.ms

(70) Pentachlorophenol (C)

17.098min (0.000) 15419.48 ng




response 280255

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.90
264.00	61.60	60.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092622\
Data File : BN021910.D
Acq On : 26 Sep 2022 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 26 17:43:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 17:42:56 2022
Response via : Initial Calibration

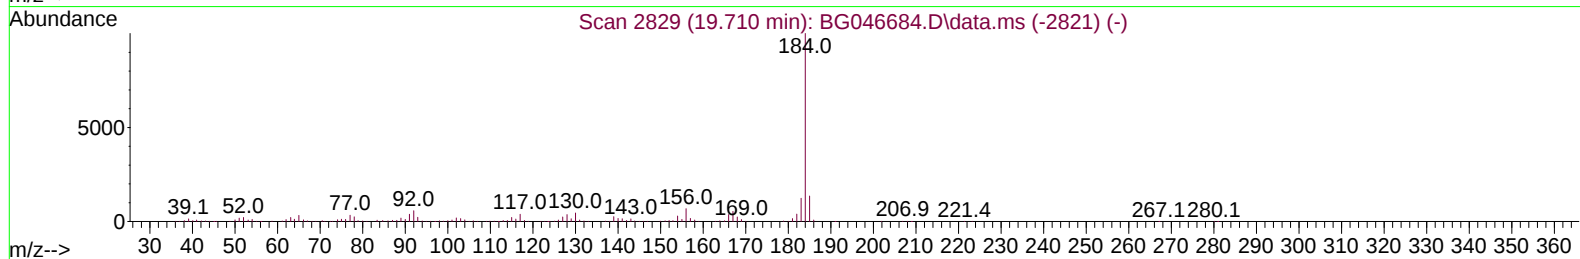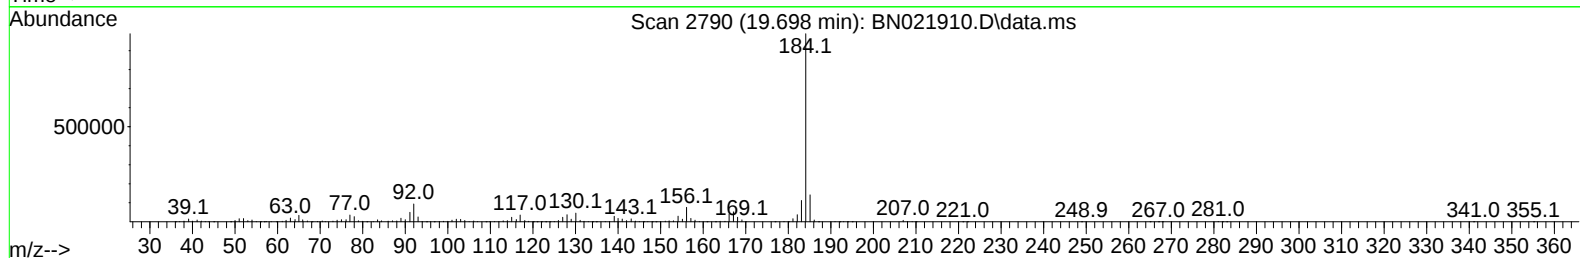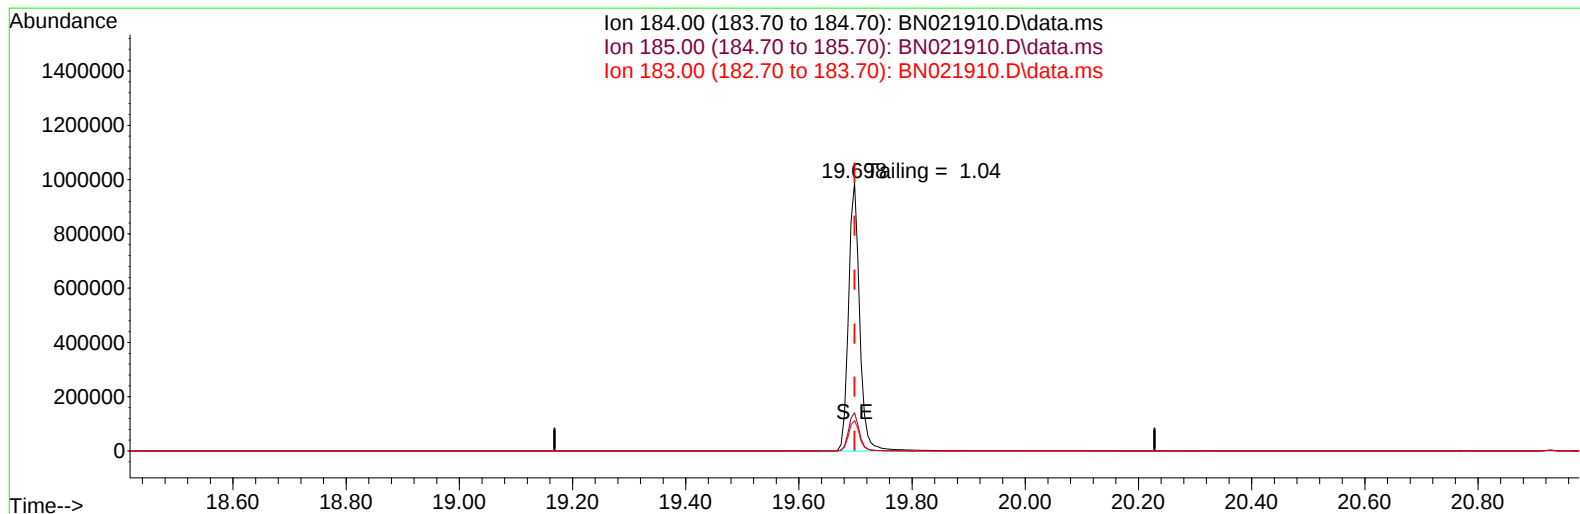

TIC: BN021910.D\data.ms

(77) Benzidine

19.698min (0.000) 0.00 ng

response 1354602

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/26/2022	BNA_N	<u>BN021910.D</u>
Compound Name	Response	Retention Time
DDT	834796	20.92
DDD	59061	20.48
DDE	16238	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
75299	910095	8.27

Instrument :
BNA_N
ClientSampleId :
DFTPP