

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
 Data File : BN021922.D
 Acq On : 26 Sep 2022 17:37
 Operator : CG/JU
 Sample : PB147751BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK751

Quant Time: Sep 27 00:25:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	4035	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	13303	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.703	164	7370	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	14006	0.400	ng/ul	0.00
17) Chrysene-d12	21.650	240	7401	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	6472	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	26396	5.317	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	6081	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	10192	0.370	ng/ul	0.00
Target Compounds						
					Qvalue	
14) Pentachlorophenol	17.109	266	65	0.024	ng/ul	95
20) Pyrene	19.845	202	1346	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.983	252	2209	0.093	ng/ul#	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
Data File : BN021922.D
Acq On : 26 Sep 2022 17:37
Operator : CG/JU
Sample : PB147751BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK751

Quant Time: Sep 27 00:25:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




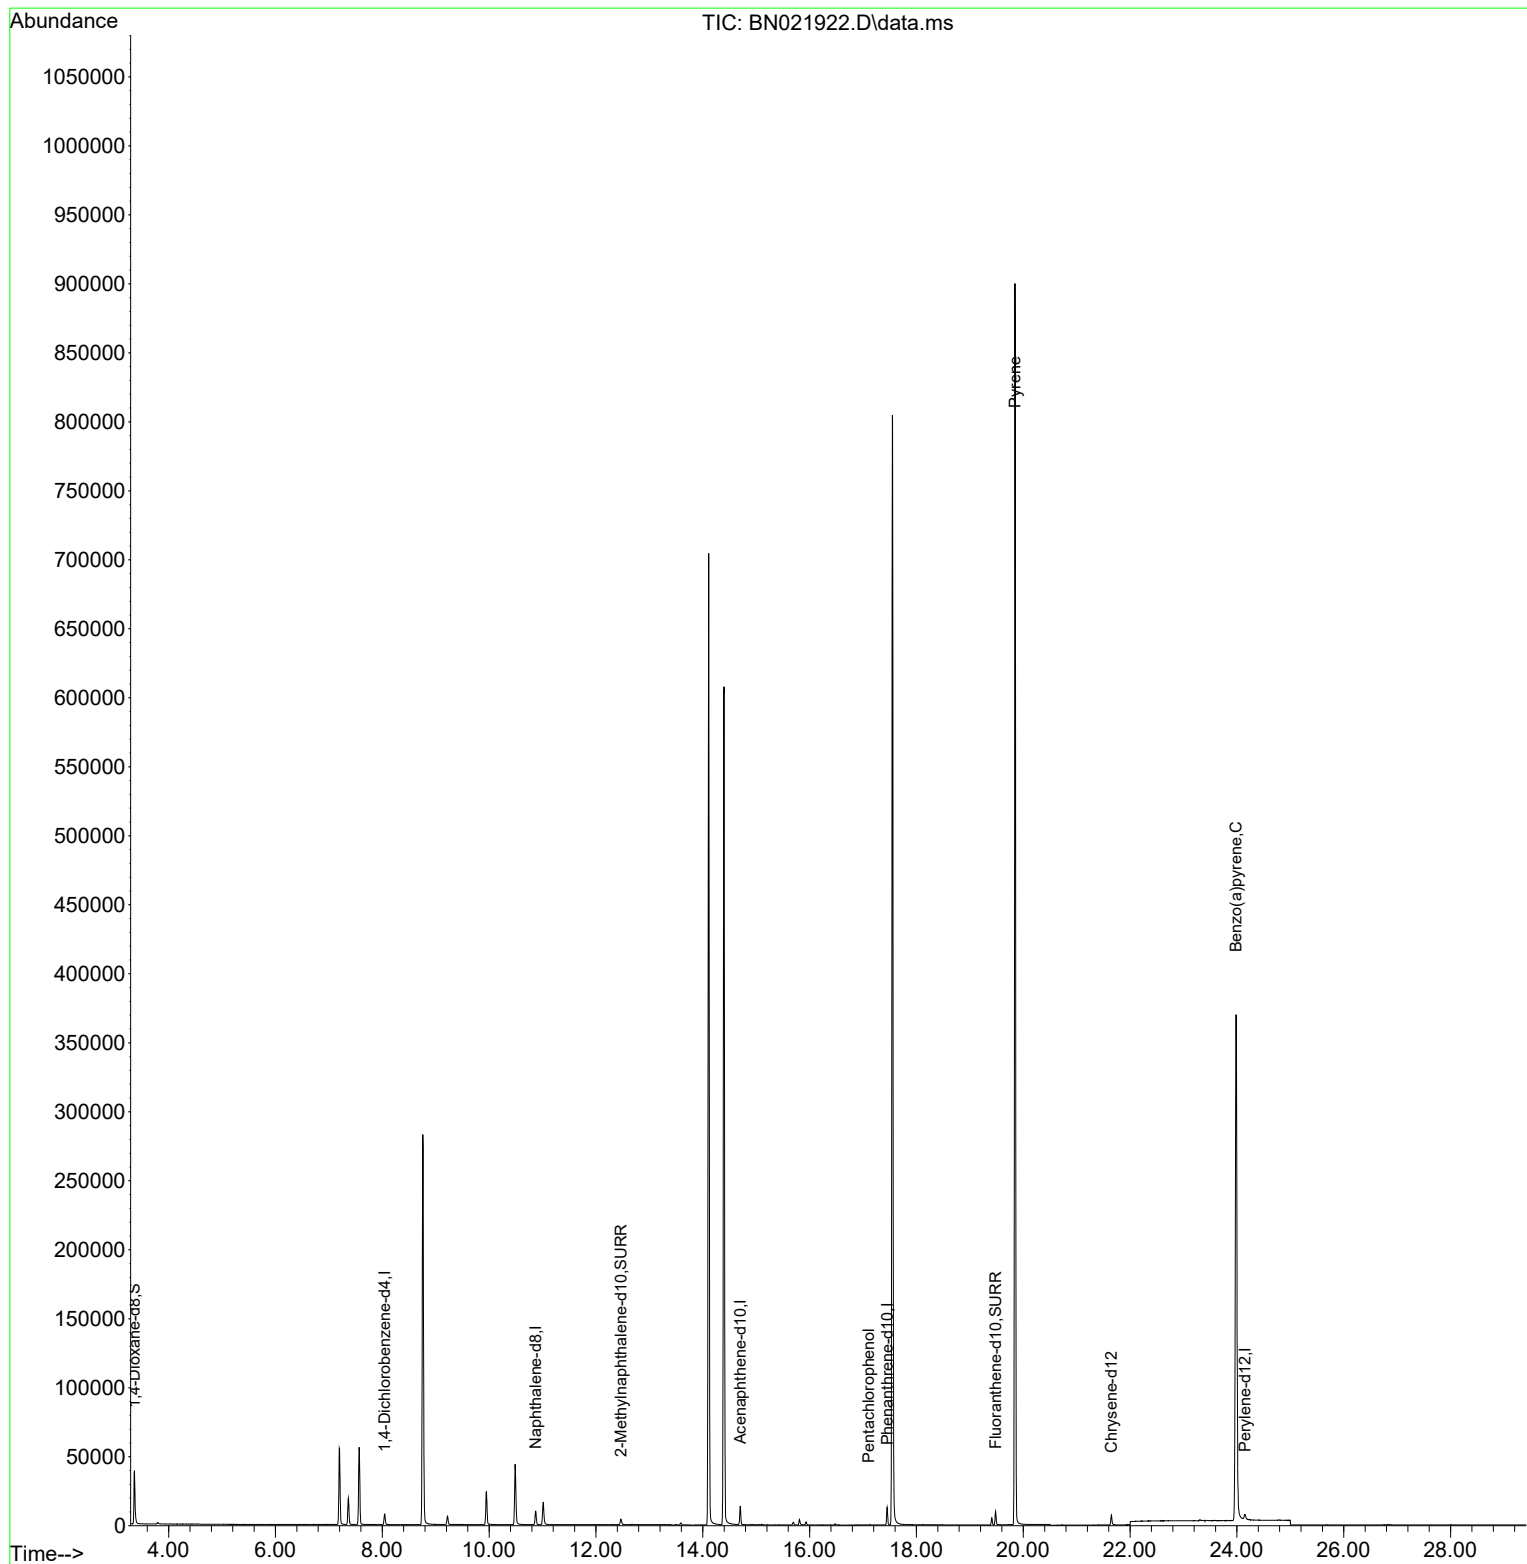


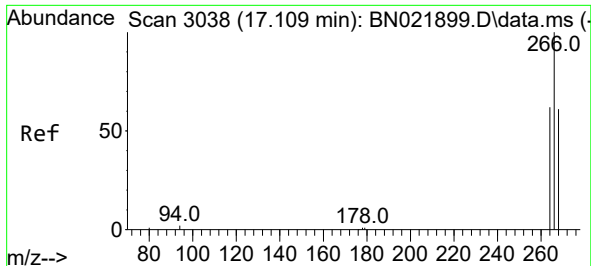

#14
 Pentachlorophenol
 Concen: 0.024 ng/ul
 RT: 17.109 min Scan# 3038
 Delta R.T. -0.000 min
 Lab File: BN021922.D
 Acq: 26 Sep 2022 17:37




Instrument :
 BNA_N
 ClientSampleId :
 SBLK751


Tgt Ion:266 Resp: 65
 Ion Ratio Lower Upper
 266 100
 264 61.5 49.8 74.8
 268 70.8 50.6 75.8

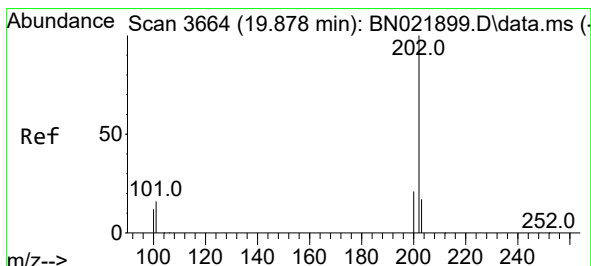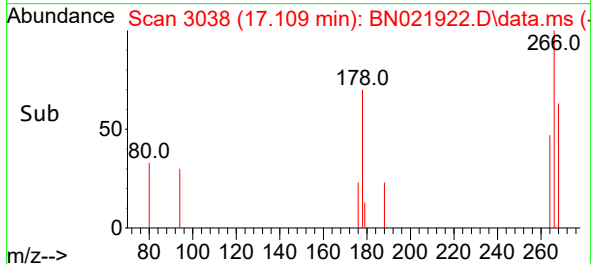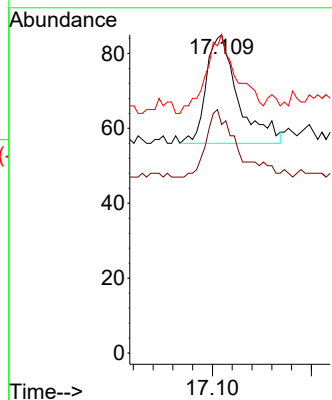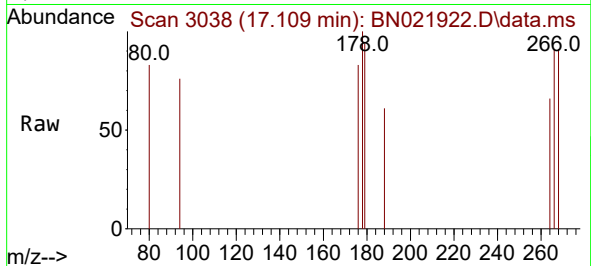

#20
 Pyrene
 Concen: 0.039 ng/ul
 RT: 19.845 min Scan# 3657
 Delta R.T. -0.033 min
 Lab File: BN021922.D
 Acq: 26 Sep 2022 17:37

Tgt Ion:202 Resp: 1346
 Ion Ratio Lower Upper
 202 100
 101 172.0 11.3 16.9#
 100 1258.8 9.0 13.4#

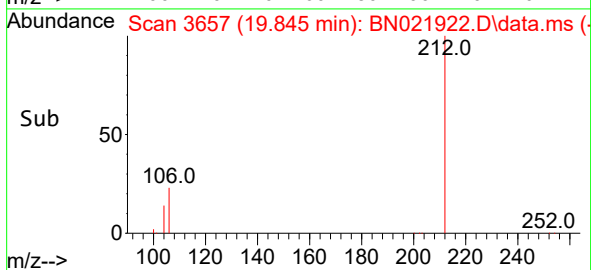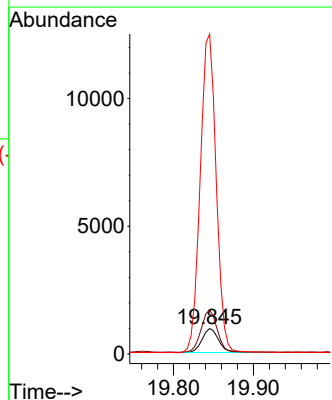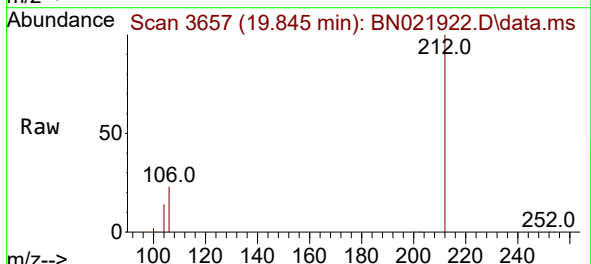

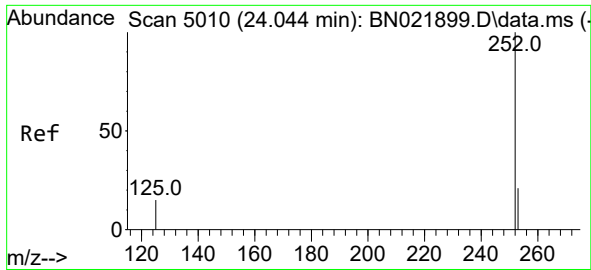

#26

Benzo(a)pyrene

Concen: 0.093 ng/ul

RT: 23.983 min Scan# 4989

Delta R.T. -0.059 min

Lab File: BN021922.D


Acq: 26 Sep 2022 17:37

Instrument :

BNA_N

ClientSampleId :

SBLK751

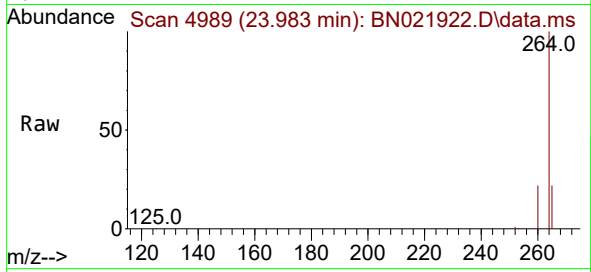

Tgt Ion:252 Resp: 2209

Ion Ratio Lower Upper

252 100

253 61.8 22.1 33.1#

125 61.2 14.7 22.1#

