

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
 Data File : BN021925.D
 Acq On : 26 Sep 2022 19:36
 Operator : CG/JU
 Sample : N4662-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ24

Quant Time: Sep 27 00:26:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	8004	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	26165	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.698	164	14628	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	29345	0.400	ng/ul	0.00
17) Chrysene-d12	21.644	240	17398	0.400	ng/ul	# 0.00
23) Perylene-d12	24.147	264	14353	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	40788	4.142	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.462	152	10665	0.257	ng/ul	-0.01
18) Fluoranthene-d10	19.478	212	24207	0.374	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.397	88	6336	0.627	ng/ul	91
20) Pyrene	19.845	202	2801	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.989	252	4694	0.089	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
Data File : BN021925.D
Acq On : 26 Sep 2022 19:36
Operator : CG/JU
Sample : N4662-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ24

Quant Time: Sep 27 00:26:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




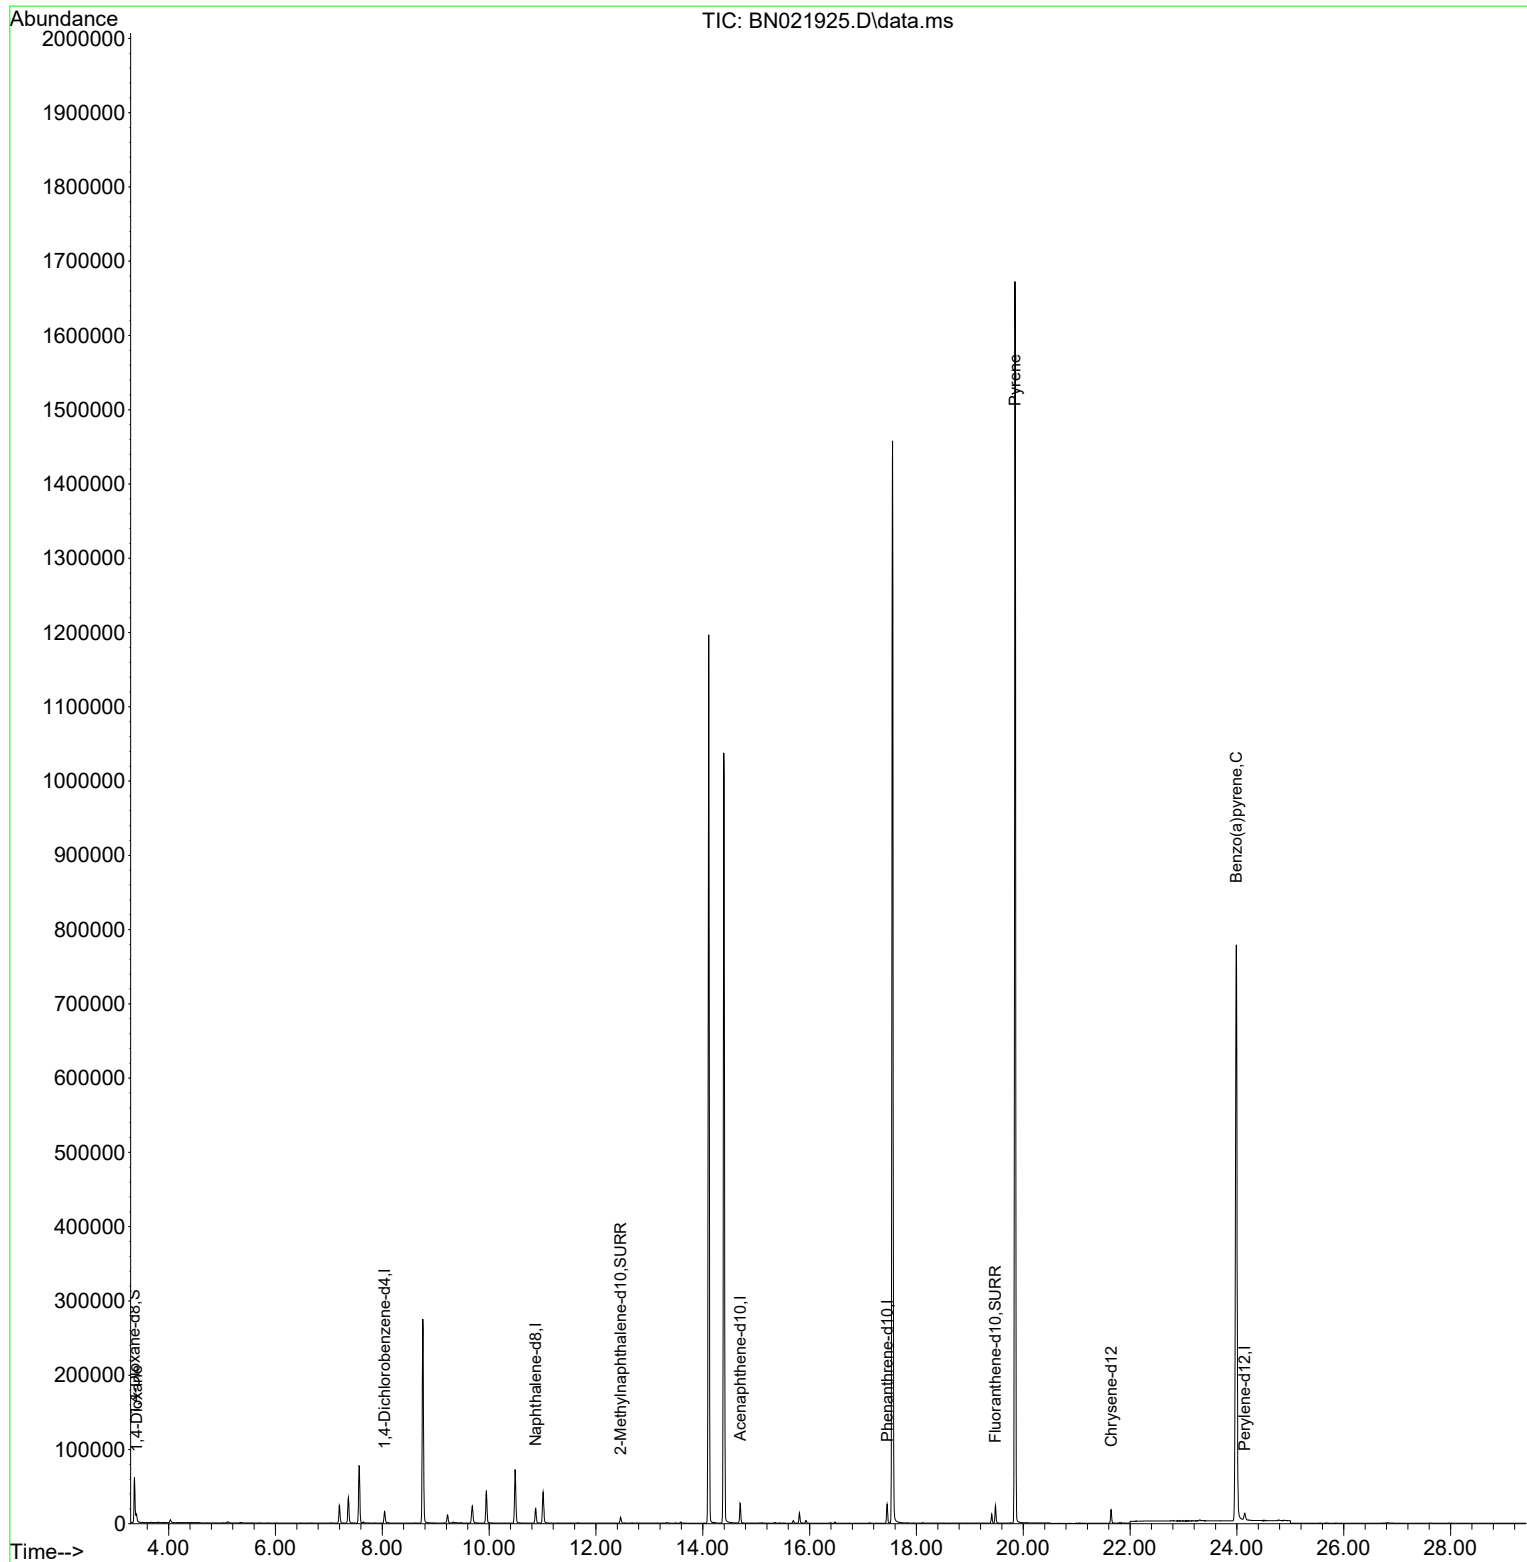


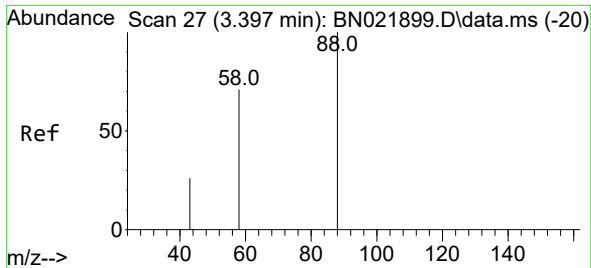

#2
 1,4-Dioxane
 Concen: 0.627 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021925.D
 Acq: 26 Sep 2022 19:36




Instrument :
 BNA_N
 ClientSampleId :
 EXZ24


Tgt Ion: 88 Resp: 6336
 Ion Ratio Lower Upper
 88 100
 43 33.5 31.4 47.0
 58 68.5 49.0 73.6

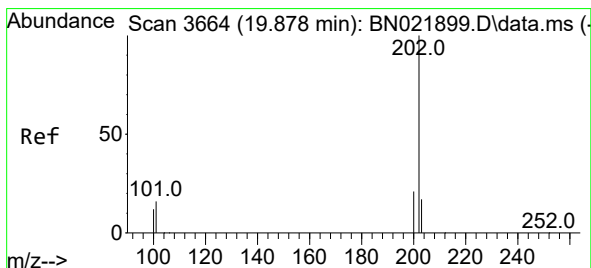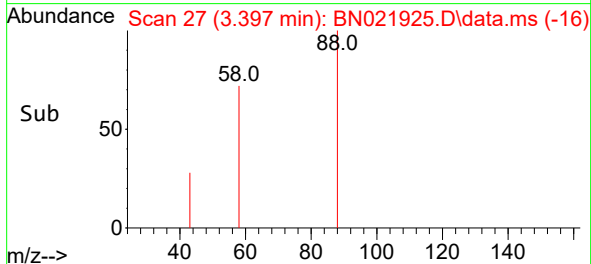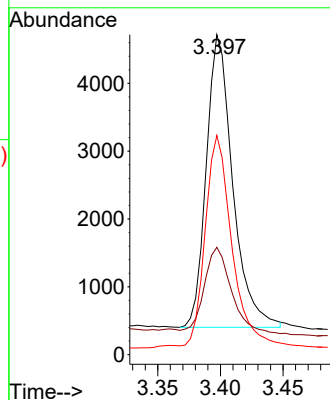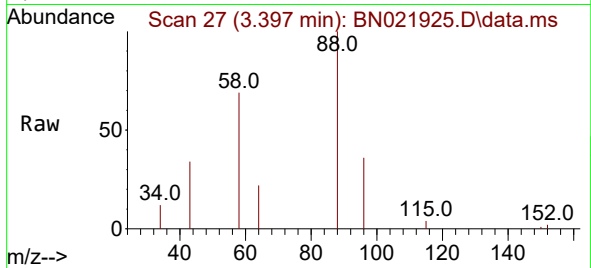

#20
 Pyrene
 Concen: 0.035 ng/ul
 RT: 19.845 min Scan# 3657
 Delta R.T. -0.033 min
 Lab File: BN021925.D
 Acq: 26 Sep 2022 19:36


Tgt Ion: 202 Resp: 2801
 Ion Ratio Lower Upper
 202 100
 101 178.3 11.3 16.9#
 100 1343.6 9.0 13.4#

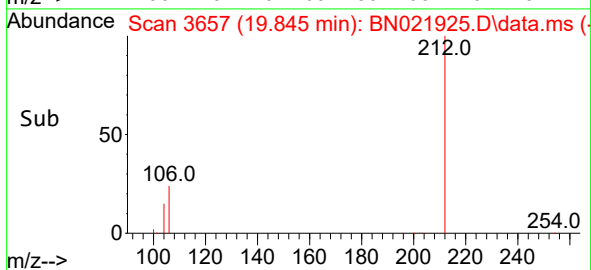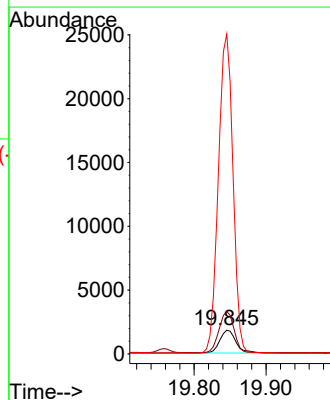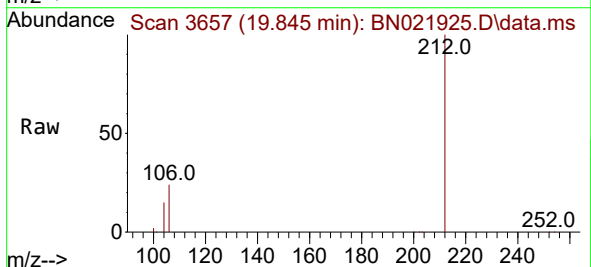

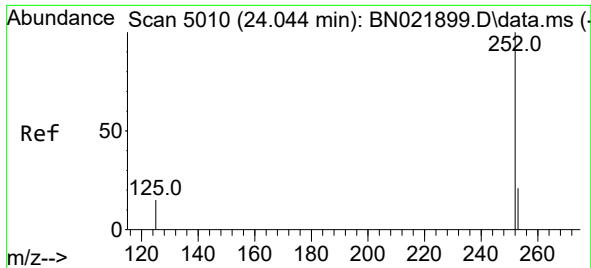

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.989 min Scan# 4991
Delta R.T. -0.053 min
Lab File: BN021925.D
Acq: 26 Sep 2022 19:36

Instrument :
BNA_N
ClientSampleId :
EXZ24

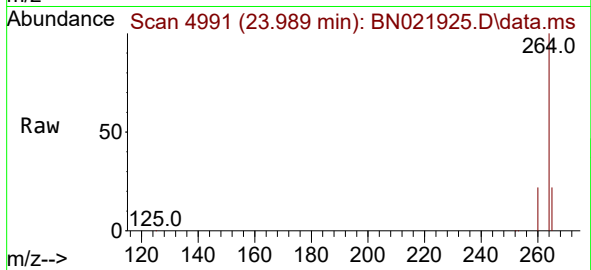

Tgt Ion:252 Resp: 4694
Ion Ratio Lower Upper
252 100
253 46.5 22.1 33.1#
125 45.6 14.7 22.1#

