

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
 Data File : BN021928.D
 Acq On : 26 Sep 2022 21:33
 Operator : CG/JU
 Sample : N4662-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ28

Quant Time: Sep 27 00:26:21 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	6631	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	22171	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.698	164	12507	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	24973	0.400	ng/ul	0.00
17) Chrysene-d12	21.644	240	14504	0.400	ng/ul	0.00
23) Perylene-d12	24.146	264	11959	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	34422	4.219	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.462	152	10632	0.303	ng/ul	-0.01
18) Fluoranthene-d10	19.478	212	23005	0.426	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.397	88	303	0.036	ng/ul#	51
12) Fluorene	15.693	166	3218	0.064	ng/ul#	14
20) Pyrene	19.845	202	2595	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.983	252	4165	0.095	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
Data File : BN021928.D
Acq On : 26 Sep 2022 21:33
Operator : CG/JU
Sample : N4662-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ28

Quant Time: Sep 27 00:26:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




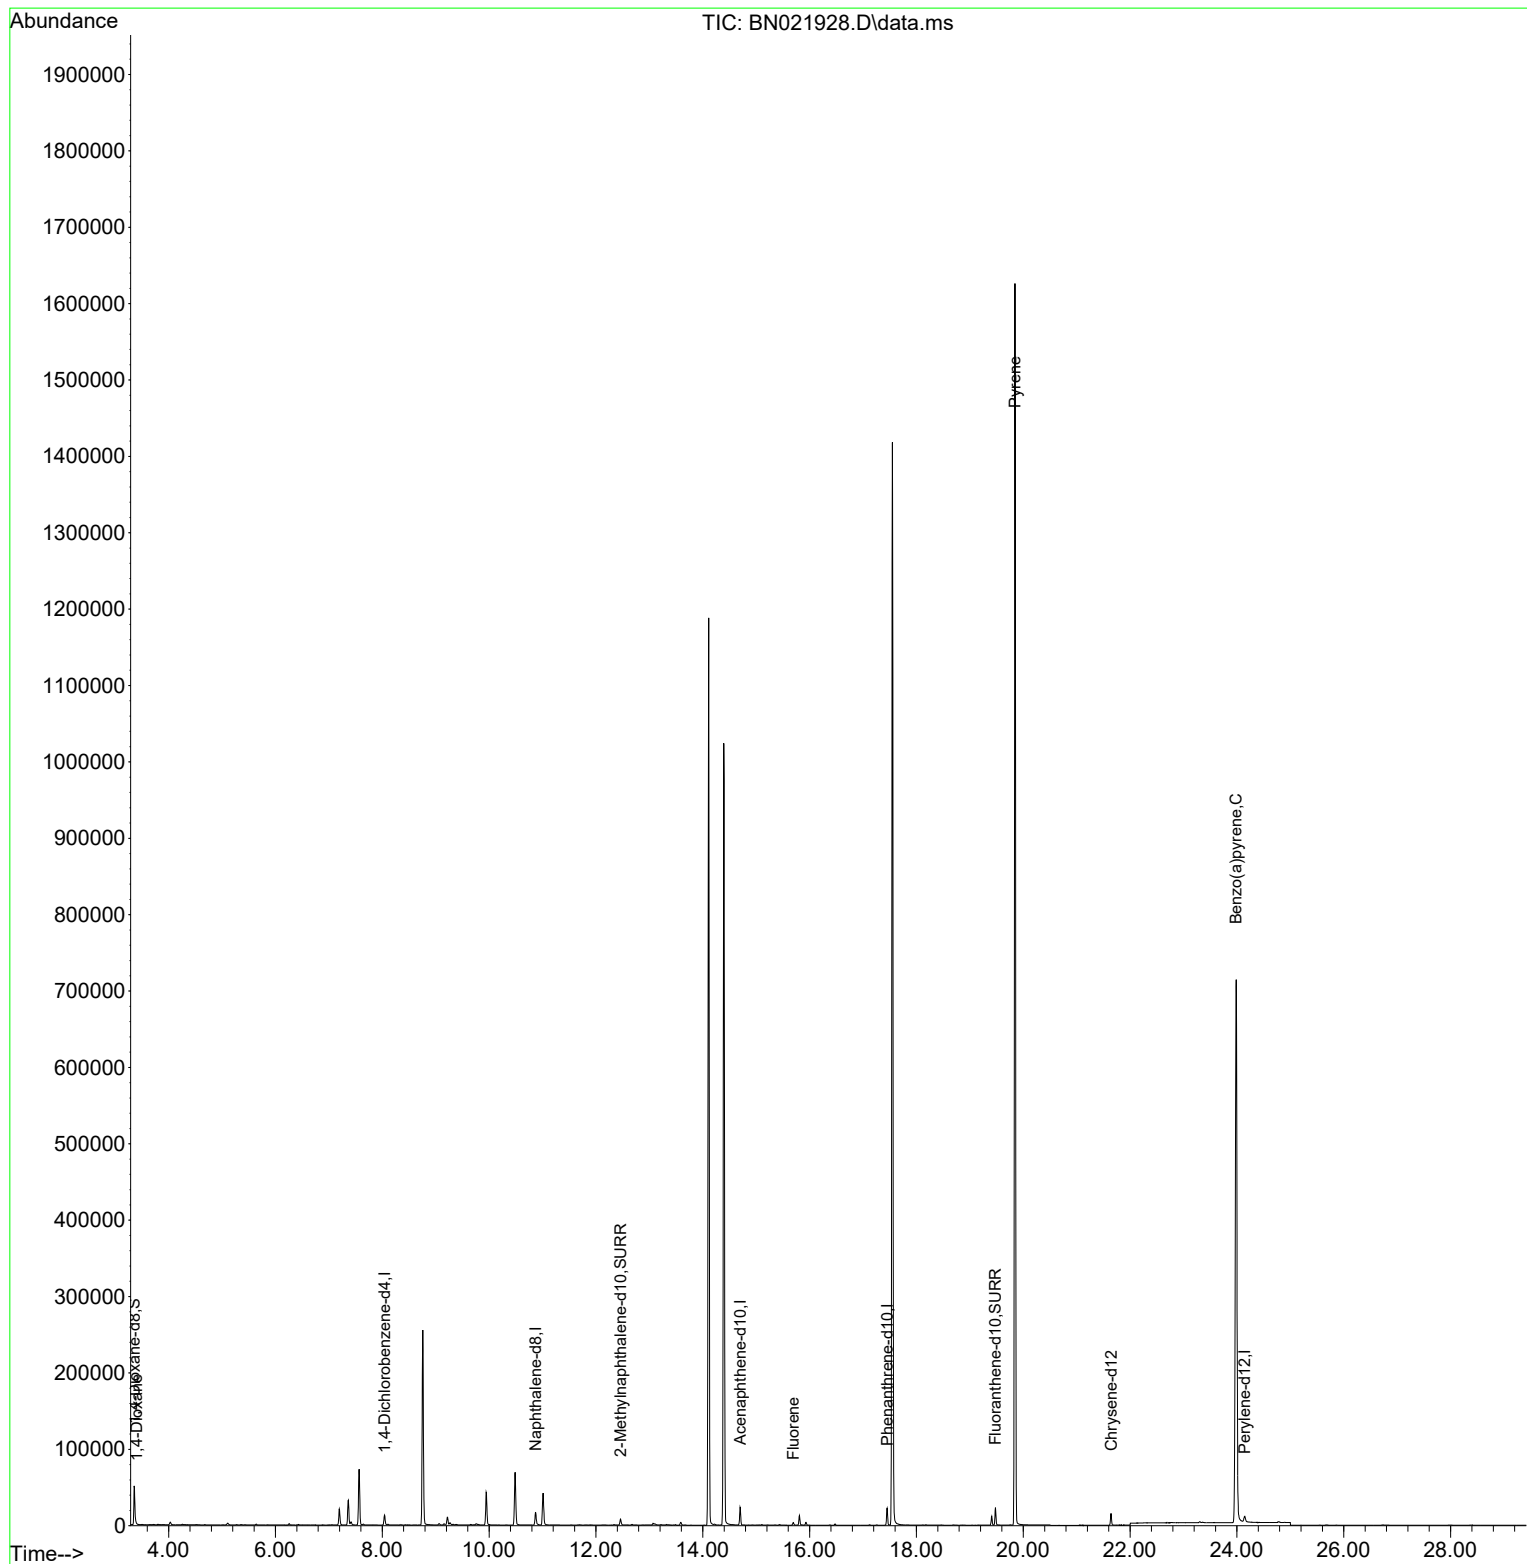


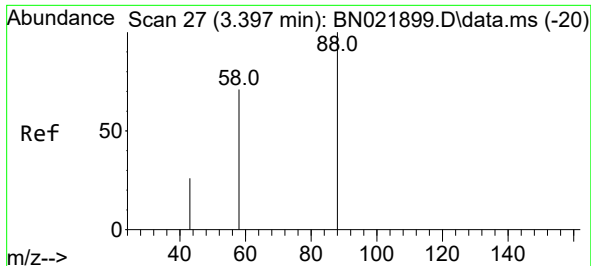

#2
 1,4-Dioxane
 Concen: 0.036 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021928.D
 Acq: 26 Sep 2022 21:33




Instrument :
 BNA_N
 ClientSampleId :
 EXZ28


Tgt Ion: 88 Resp: 303
 Ion Ratio Lower Upper
 88 100
 43 106.6 31.4 47.0#
 58 54.3 49.0 73.6

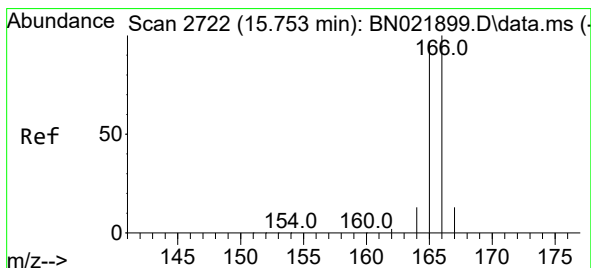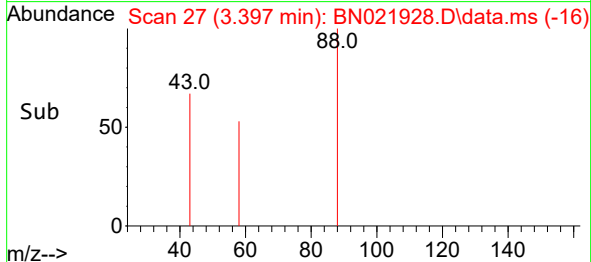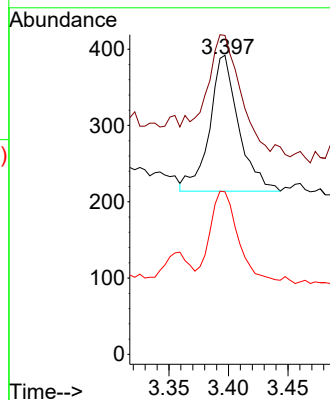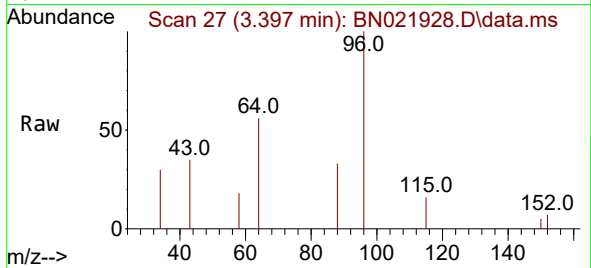

#12
 Fluorene
 Concen: 0.064 ng/ul
 RT: 15.693 min Scan# 2709
 Delta R.T. -0.065 min
 Lab File: BN021928.D
 Acq: 26 Sep 2022 21:33

Tgt Ion: 166 Resp: 3218
 Ion Ratio Lower Upper
 166 100
 165 7.0 78.6 117.8#
 167 33.0 11.8 17.6#


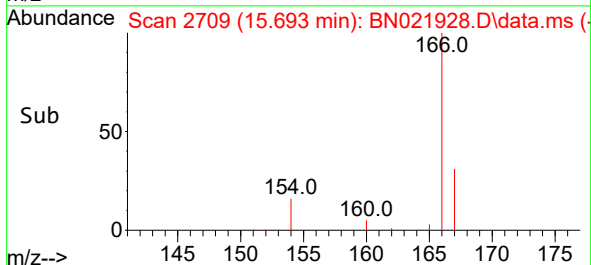
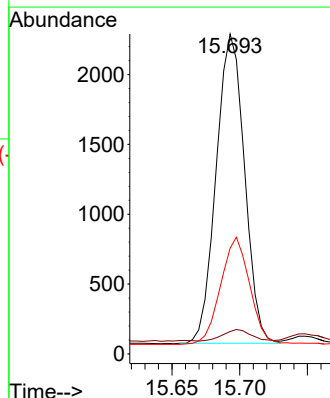
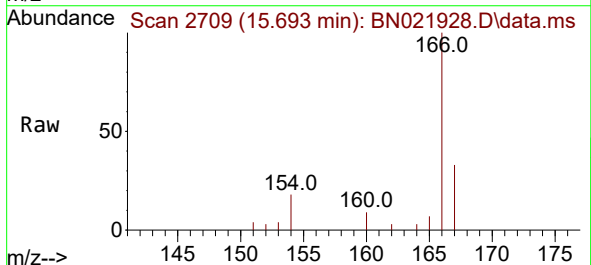


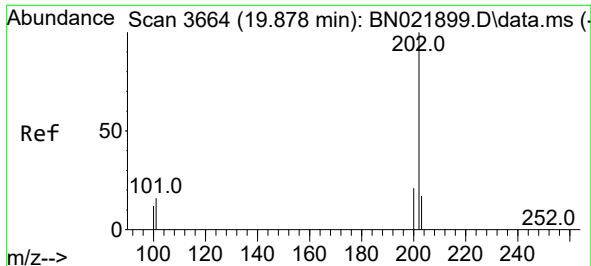

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.845 min Scan# 30
Delta R.T. -0.033 min
Lab File: BN021928.D
Acq: 26 Sep 2022 21:33

Instrument :
BNA_N
ClientSampleId :
EXZ28

Tgt Ion:202 Resp: 2595
Ion Ratio Lower Upper
202 100
101 176.6 11.3 16.9#
100 1287.6 9.0 13.4#

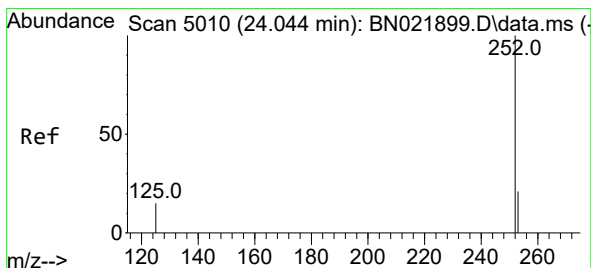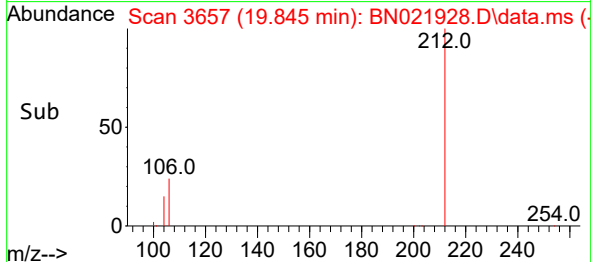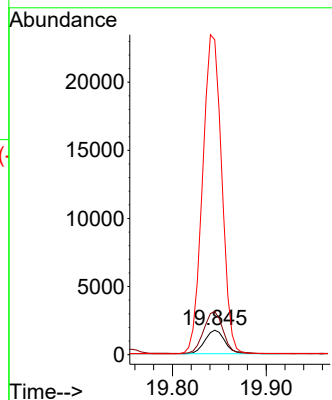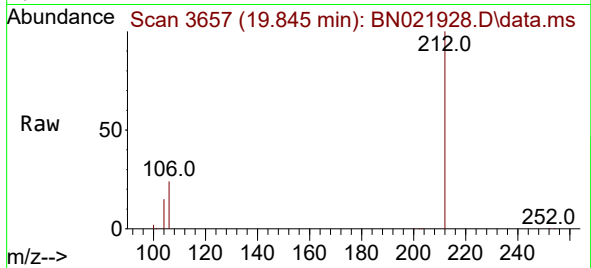

#26
Benzo(a)pyrene
Concen: 0.095 ng/ul
RT: 23.983 min Scan# 4989
Delta R.T. -0.059 min
Lab File: BN021928.D
Acq: 26 Sep 2022 21:33

Tgt Ion:252 Resp: 4165
Ion Ratio Lower Upper
252 100
253 47.7 22.1 33.1#
125 47.6 14.7 22.1#

