

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
 Data File : BN021929.D
 Acq On : 26 Sep 2022 22:12
 Operator : CG/JU
 Sample : N4662-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ33

Quant Time: Sep 27 00:26:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	6252	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	20741	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.698	164	11546	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	22777	0.400	ng/ul	0.00
17) Chrysene-d12	21.647	240	13371	0.400	ng/ul	# 0.00
23) Perylene-d12	24.147	264	11178	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	37286	4.848	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.462	152	10430	0.318	ng/ul	-0.01
18) Fluoranthene-d10	19.483	212	22025	0.443	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.845	202	2493	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.986	252	4003	0.097	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
Data File : BN021929.D
Acq On : 26 Sep 2022 22:12
Operator : CG/JU
Sample : N4662-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ33

Quant Time: Sep 27 00:26:27 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




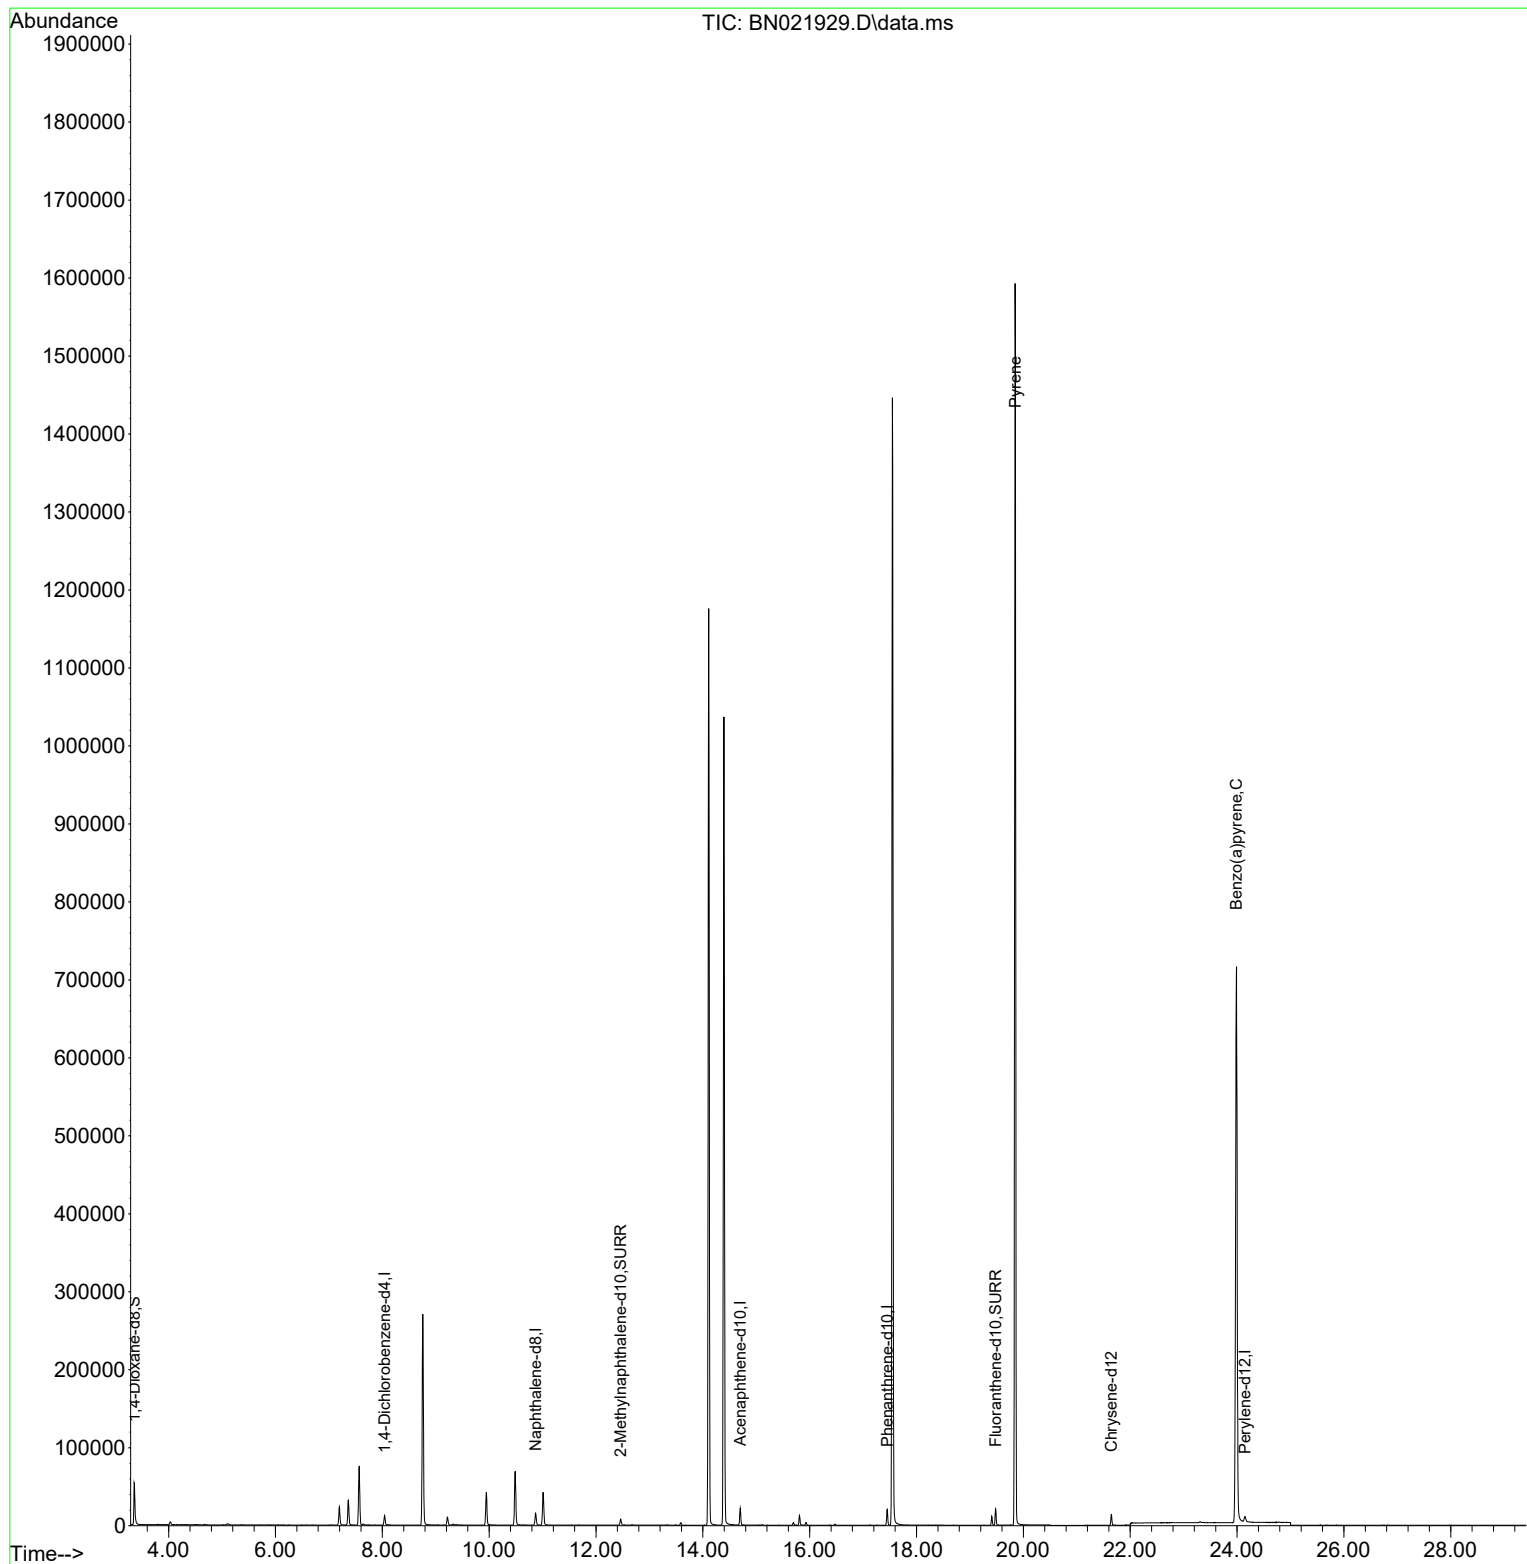


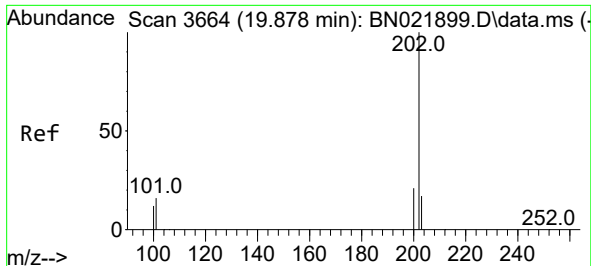

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.845 min Scan# 30
Delta R.T. -0.032 min
Lab File: BN021929.D
Acq: 26 Sep 2022 22:12

Instrument :
BNA_N
ClientSampleId :
EXZ33

Tgt Ion:202 Resp: 2493
Ion Ratio Lower Upper
202 100
101 179.3 11.3 16.9#
100 1336.2 9.0 13.4#

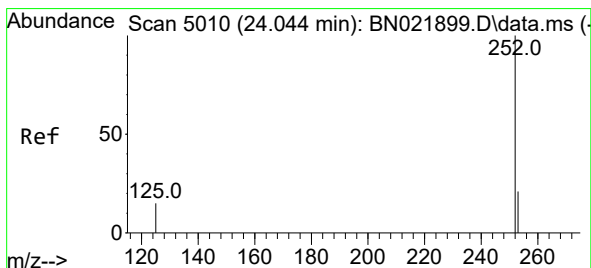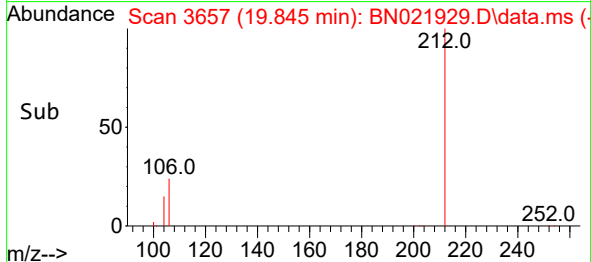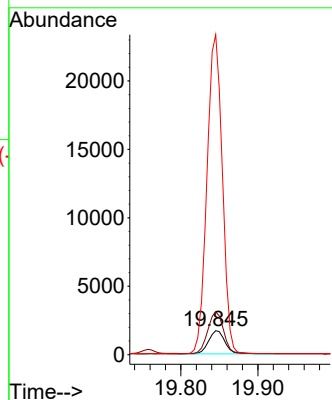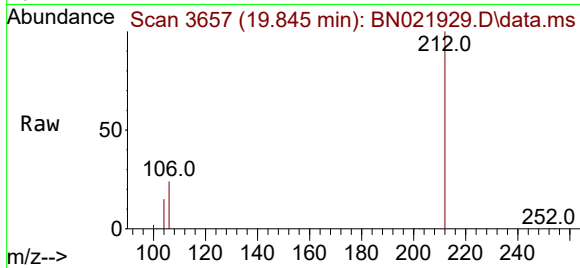

#26
Benzo(a)pyrene
Concen: 0.097 ng/ul
RT: 23.986 min Scan# 4990
Delta R.T. -0.055 min
Lab File: BN021929.D
Acq: 26 Sep 2022 22:12

Tgt Ion:252 Resp: 4003
Ion Ratio Lower Upper
252 100
253 47.5 22.1 33.1#
125 46.2 14.7 22.1#

