

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
 Data File : BN021926.D
 Acq On : 26 Sep 2022 20:15
 Operator : CG/JU
 Sample : N4662-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ26

Quant Time: Sep 27 00:26:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	6225	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	20699	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.703	164	11620	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	22725	0.400	ng/ul	0.00
17) Chrysene-d12	21.647	240	12794	0.400	ng/ul	# 0.00
23) Perylene-d12	24.149	264	10595	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.359	96	37100	4.844	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.462	152	10181	0.311	ng/ul	-0.01
18) Fluoranthene-d10	19.483	212	21031	0.442	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	1037	0.132	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092722\
Data File : BN021926.D
Acq On : 26 Sep 2022 20:15
Operator : CG/JU
Sample : N4662-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ26


Quant Time: Sep 27 00:26:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

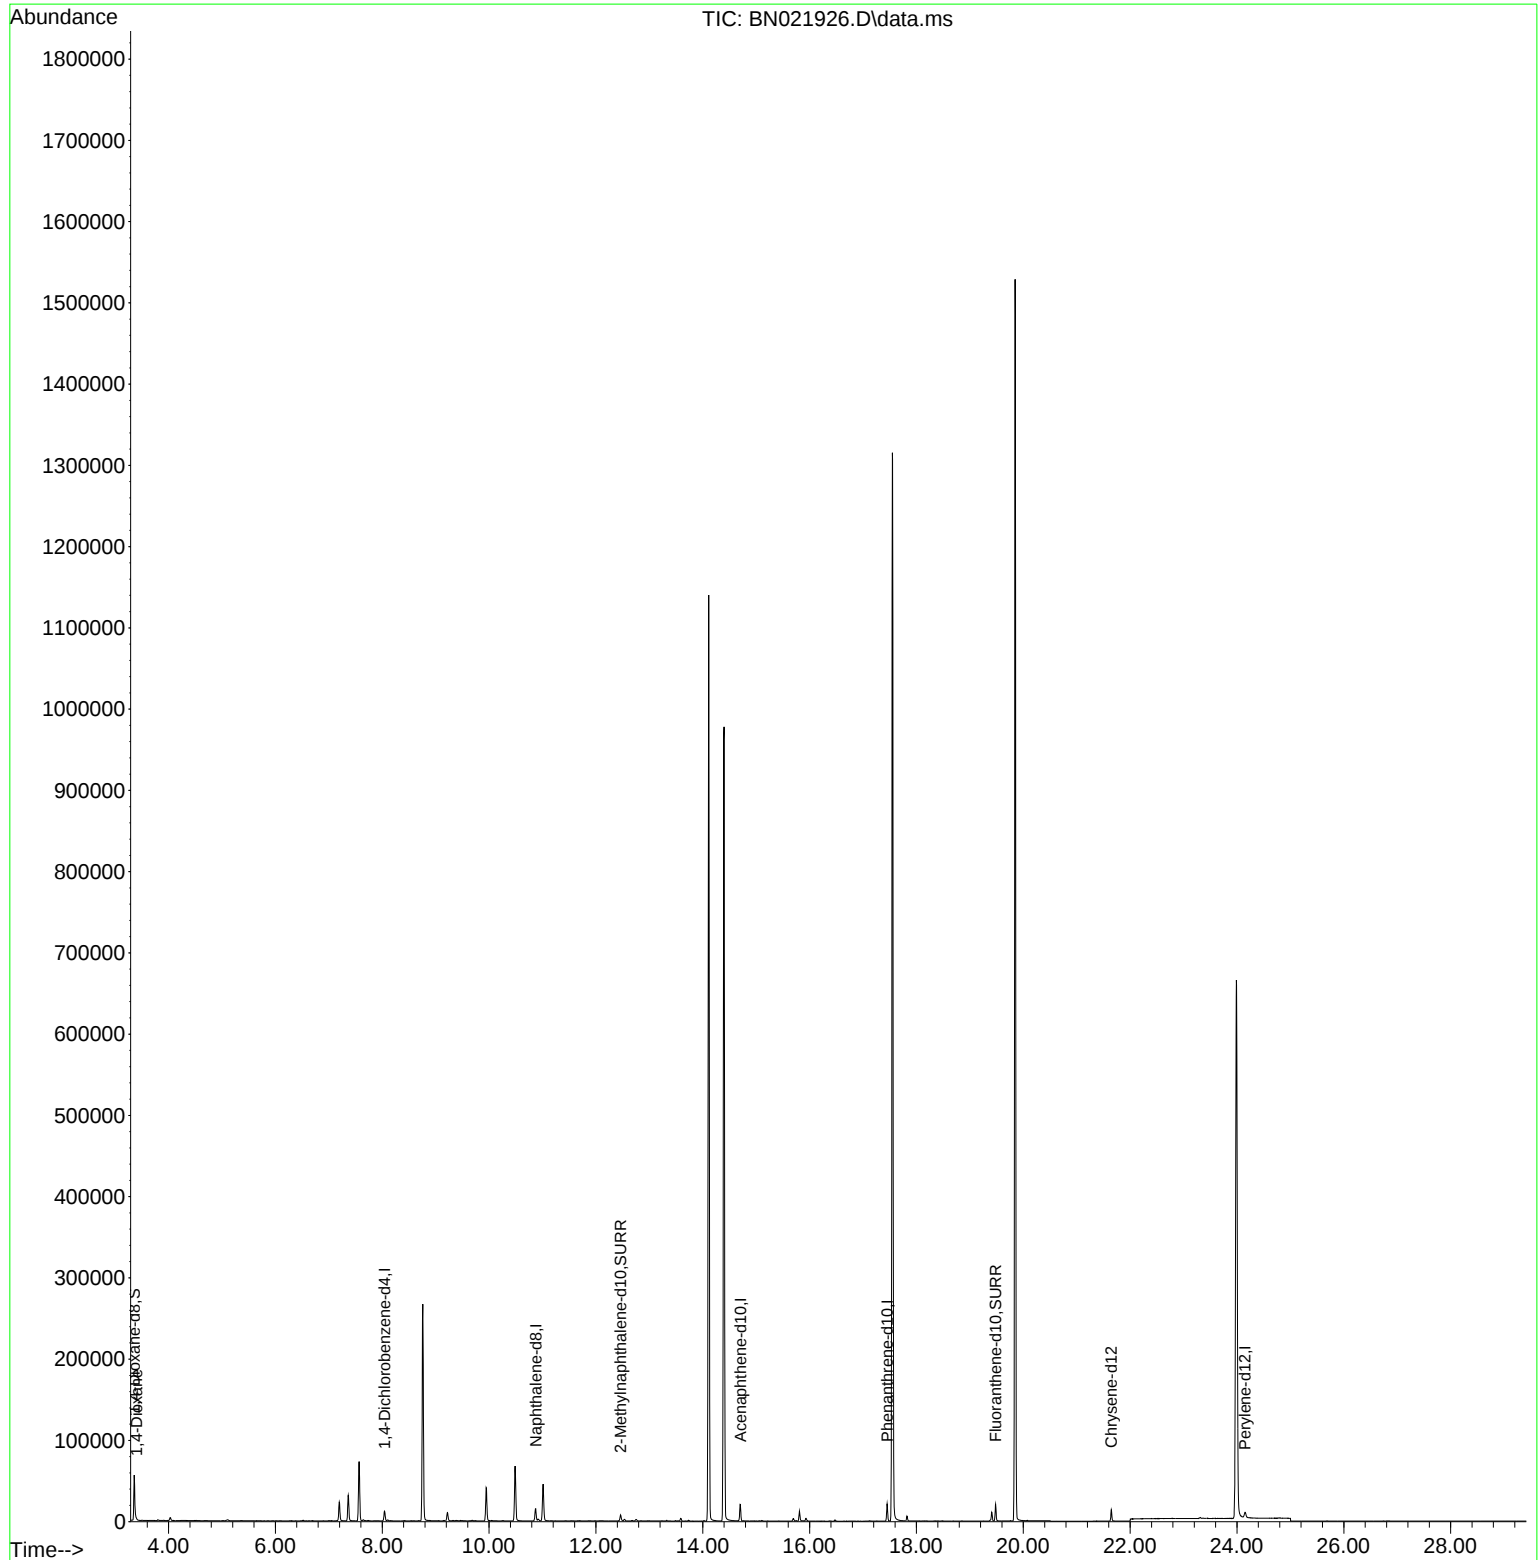

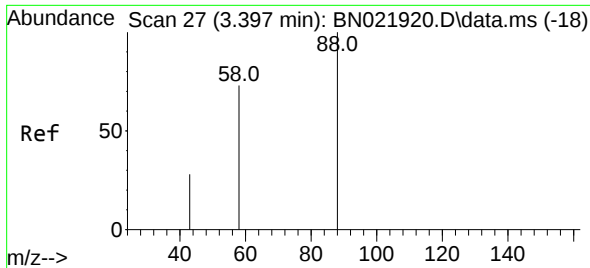

#2
 1,4-Dioxane
 Concen: 0.132 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021926.D
 Acq: 26 Sep 2022 20:15

Instrument :
 BNA_N
 ClientSampleId :
 EXZ26

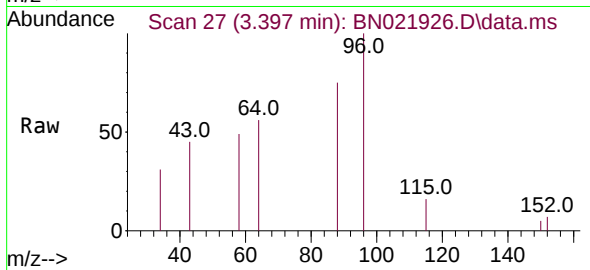

Tgt Ion: 88	Resp: 1037
Ion Ratio	Lower Upper
88	100
43	60.0 31.4 47.0#
58	65.1 49.0 73.6

