
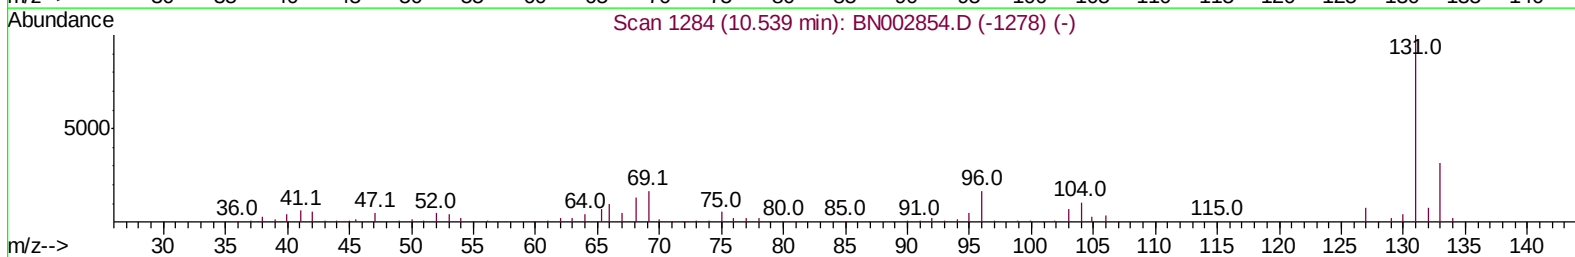
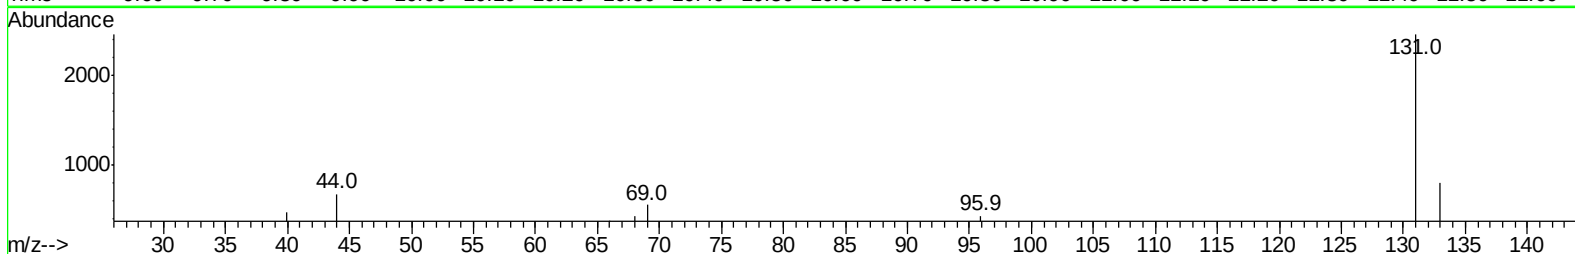


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092818\
Data File : BN002861.D
Acq On : 28 Sep 2018 21:32
Operator : MJ/SJ
Sample : J5117-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Sep 29 06:36:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 29 06:35:10 2018
Response via : Initial Calibration

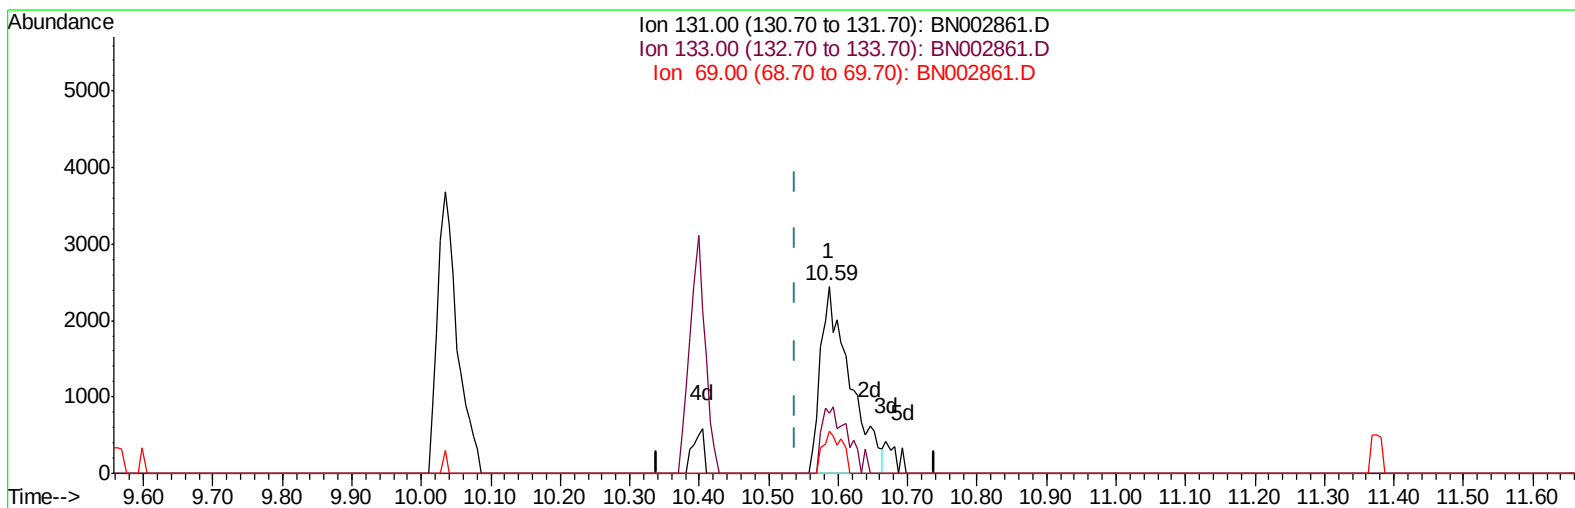

TIC: BN002861.D

(29) 4-Chloroaniline-d4 (S)

10.587min (+0.047) 0.69ng/ul m

response 7227

Ion	Exp%	Act%
131.00	100	100
133.00	32.90	32.45
69.00	16.80	22.61#
0.00	0.00	0.00