

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092818\
 Data File : BN002855.D
 Acq On : 28 Sep 2018 18:02
 Operator : MJ/SJ
 Sample : PB113355BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	47	rVB	30975	46758	1.04%	0.116%
2	6.811	644	650	668	rBV	506770	874969	19.47%	2.167%
3	6.969	671	677	691	rBV	468742	725859	16.15%	1.797%
4	7.163	704	710	724	rVB	555485	913619	20.33%	2.262%
5	7.628	782	789	799	rBV	417354	702466	15.63%	1.739%
6	8.334	903	909	927	rBV	652373	1112371	24.75%	2.754%
7	8.775	975	984	998	rBV	539616	910365	20.25%	2.254%
8	9.493	1099	1106	1122	rBV	437928	769290	17.11%	1.905%
9	10.028	1191	1197	1210	rBV	612750	1126835	25.07%	2.790%
10	10.393	1252	1259	1271	rBV	638769	1097314	24.41%	2.717%
11	10.540	1278	1284	1306	rBV	667973	1270704	28.27%	3.147%
12	13.681	1811	1818	1831	rBV	1516062	2167870	48.23%	5.368%
13	13.951	1858	1864	1877	rBV	1639594	2476022	55.09%	6.131%
14	14.263	1911	1917	1929	rVB2	1027493	1555859	34.61%	3.853%
15	14.498	1951	1957	1977	rBV	380791	824739	18.35%	2.042%
16	15.263	2081	2087	2100	rBV	2284839	3219406	71.62%	7.972%
17	15.410	2106	2112	2123	rBV	509160	824006	18.33%	2.040%
18	17.016	2379	2385	2395	rBV	1422519	1948830	43.36%	4.826%
19	17.116	2395	2402	2419	rVV2	2518428	3635725	80.89%	9.003%
20	19.422	2787	2794	2809	rBV	3108329	4358569	96.97%	10.793%
21	21.221	3094	3100	3112	rBV	1817807	2449792	54.50%	6.066%
22	22.263	3273	3277	3283	rBV	54854	70047	1.56%	0.173%
23	22.757	3356	3361	3366	rBV2	79600	114350	2.54%	0.283%
24	23.286	3443	3451	3463	rBV	2296020	4494838	100.00%	11.130%
25	23.427	3468	3475	3485	rVB	1151150	2208769	49.14%	5.469%
26	23.933	3556	3561	3568	rVB	102432	187224	4.17%	0.464%
27	24.651	3678	3683	3693	rVB2	87297	188947	4.20%	0.468%
28	25.492	3822	3826	3833	rVB2	51791	109032	2.43%	0.270%


Sum of corrected areas: 40384575

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092818\
Data File : BN002855.D
Acq On : 28 Sep 2018 18:02
Operator : MJ/SJ
Sample : PB113355BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

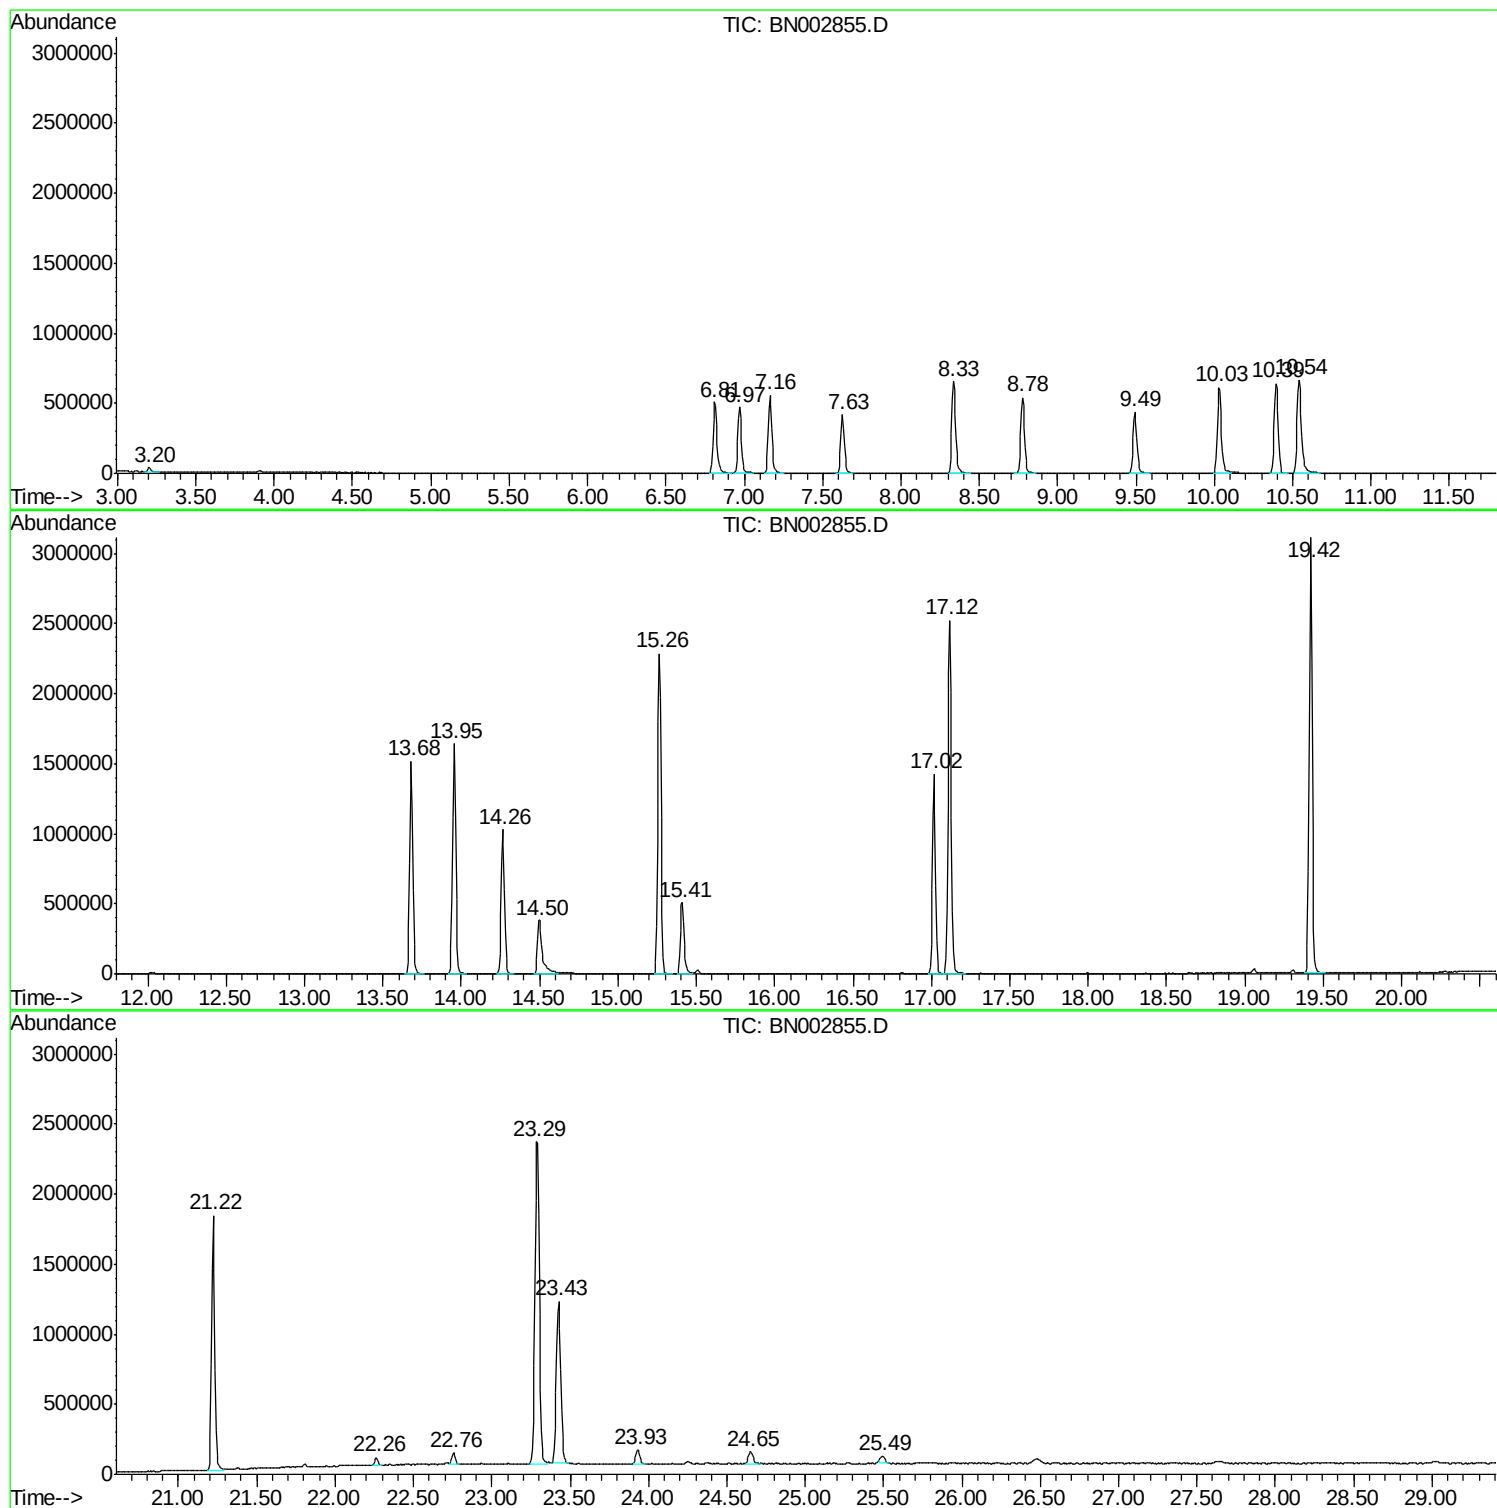

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092818\
Data File : BN002855.D
Acq On : 28 Sep 2018 18:02
Operator : MJ/SJ
Sample : PB113355BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092818\
Data File : BN002855.D
Acq On : 28 Sep 2018 18:02
Operator : MJ/SJ
Sample : PB113355BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc