

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092820\
 Data File : BN012006.D
 Acq On : 29 Sep 2020 05:41
 Operator : CG/JU
 Sample : L4118-14
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW201D1-20200919

Quant Time: Sep 29 07:06:35 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 25 11:18:41 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	1487	0.40	ng	# 0.00
7) Naphthalene-d8	10.440	136	6334	0.40	ng	#-0.01
13) Acenaphthene-d10	14.306	164	3564	0.40	ng	0.00
19) Phenanthrene-d10	17.053	188	6876	0.40	ng	0.00
29) Chrysene-d12	21.248	240	6545	0.40	ng	#-0.01
36) Perylene-d12	23.456	264	6849	0.40	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.283	112	622	0.12	ng	0.00
5) Phenol-d6	6.845	99	401	0.06	ng	0.00
8) Nitrobenzene-d5	8.818	82	2383	0.36	ng	0.00
11) 2-Methylnaphthalene-d10	12.038	152	3456	0.34	ng	0.00
14) 2,4,6-Tribromophenol	15.803	330	764	0.44	ng	0.00
15) 2-Fluorobiphenyl	12.923	172	4525	0.34	ng	-0.01
27) Fluoranthene-d10	19.087	212	8395	0.42	ng	0.00
31) Terphenyl-d14	19.688	244	7251	0.48	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.253	88	160	0.06	ng	# 69
34) Bis(2-ethylhexyl)phtha...	21.163	149	988	0.07	ng	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092820\
Data File : BN012006.D
Acq On : 29 Sep 2020 05:41
Operator : CG/JU
Sample : L4118-14
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW201D1-20200919

Quant Time: Sep 29 07:06:35 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 11:18:41 2020
Response via : Initial Calibration



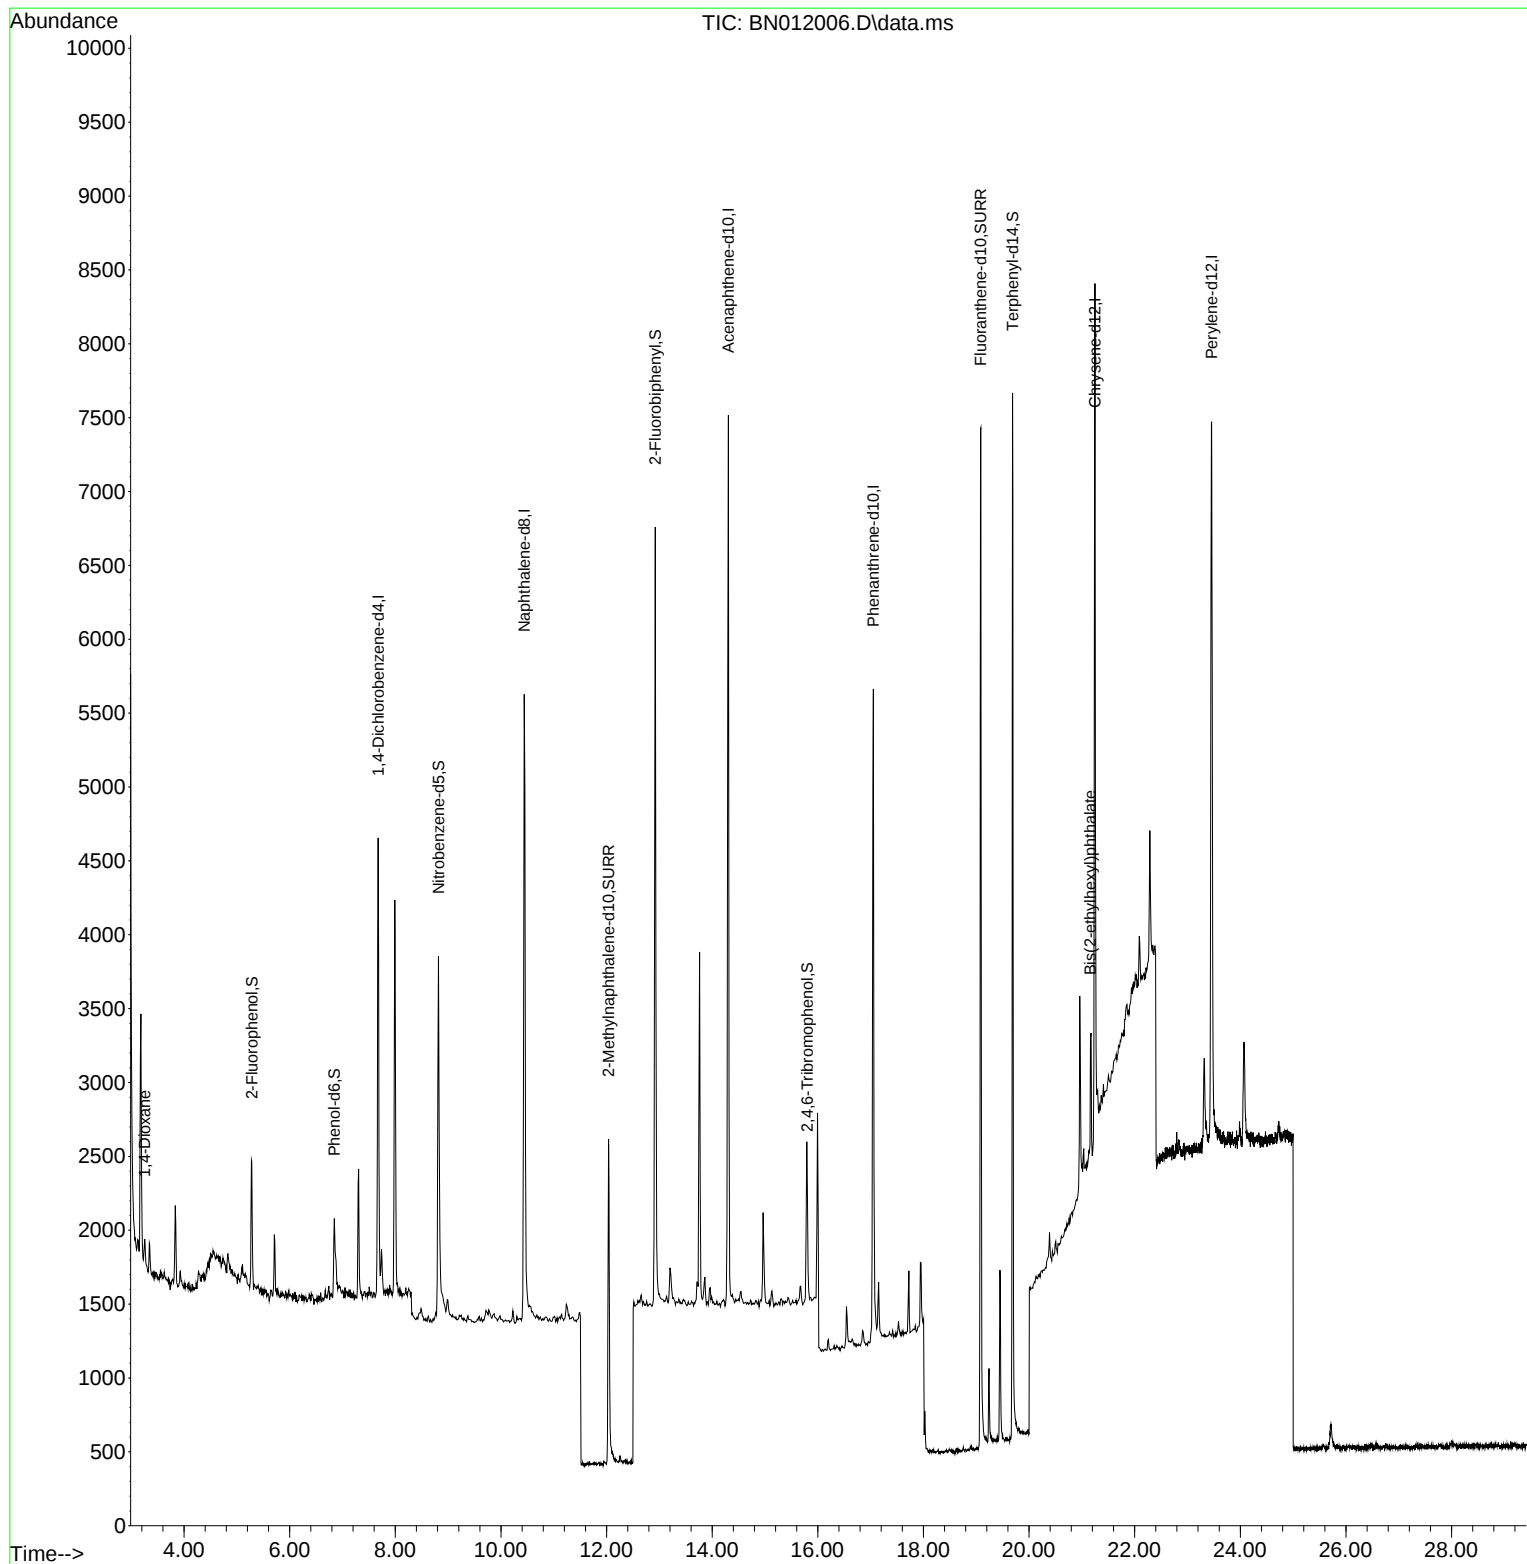




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.675 min Scan# 583
Delta R.T. -0.008 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41




Instrument :
BNA_N
ClientSampleId :
MW201D1-20200919


Tgt Ion:152 Resp: 1487
Ion Ratio Lower Upper
152 100
150 157.2 118.3 177.5
115 77.2 51.3 76.9#

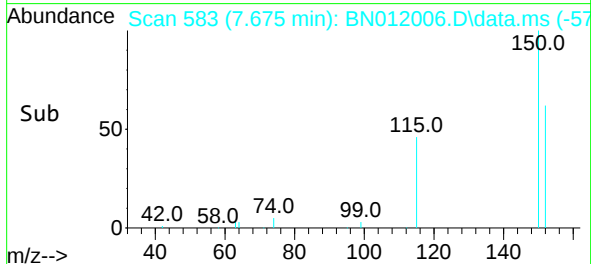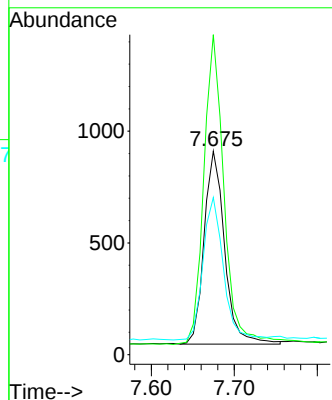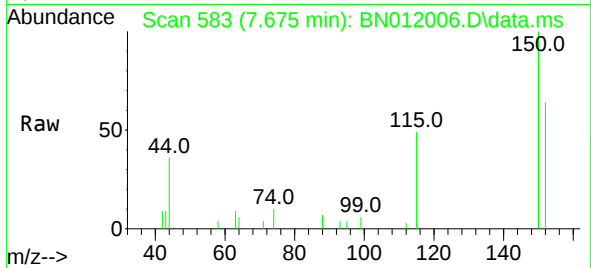

#2
1,4-Dioxane
Concen: 0.06 ng
RT: 3.253 min Scan# 34
Delta R.T. -0.000 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41

Tgt Ion: 88 Resp: 160
Ion Ratio Lower Upper
88 100
58 72.5 63.3 94.9
43 88.8 33.0 49.4#


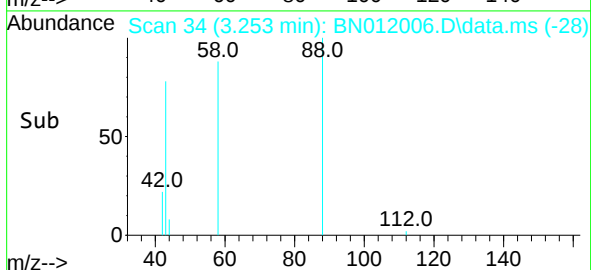
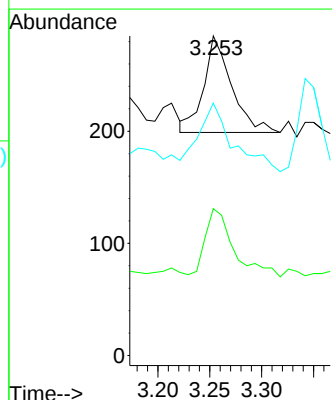
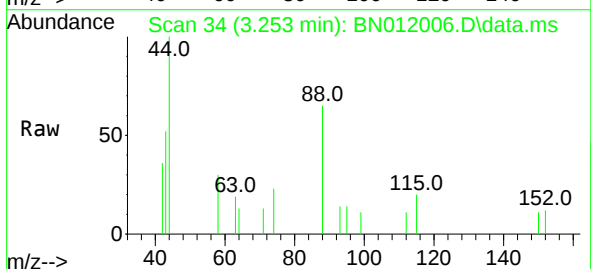


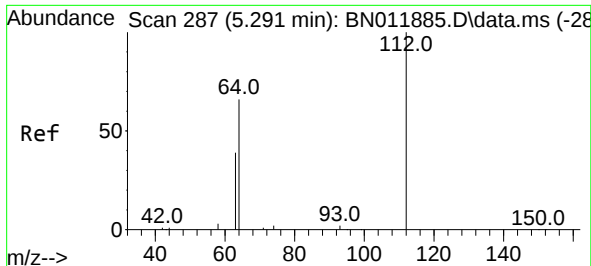

#4
2-Fluorophenol
Concen: 0.12 ng
RT: 5.283 min Scan# 286
Delta R.T. -0.000 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41




Instrument :
BNA_N
ClientSampleId :
MW201D1-20200919


Tgt Ion:112 Resp: 622
Ion Ratio Lower Upper
112 100
64 70.4 49.0 73.6
63 49.7 31.8 47.6#

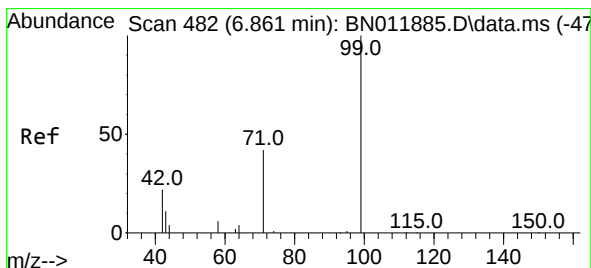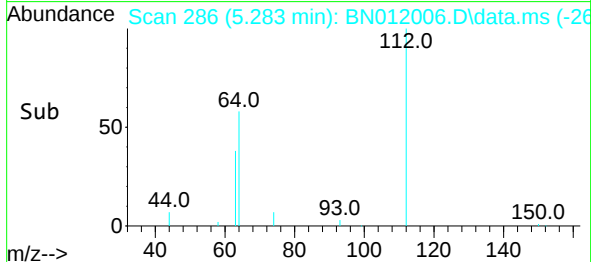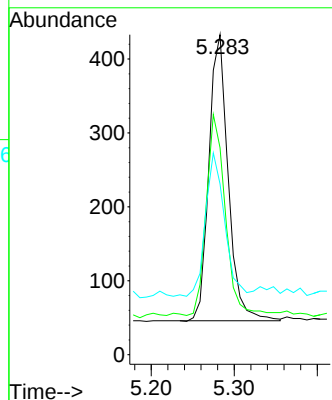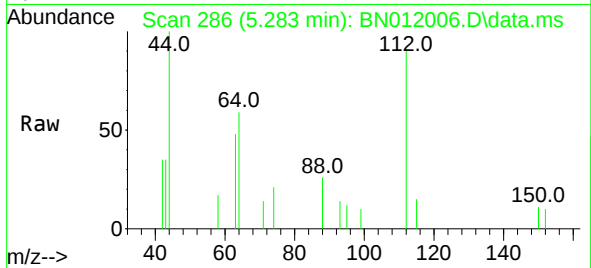

#5
Phenol-d6
Concen: 0.06 ng
RT: 6.845 min Scan# 480
Delta R.T. -0.008 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41

Tgt Ion: 99 Resp: 401
Ion Ratio Lower Upper
99 100
42 48.4 23.4 35.0#
71 64.6 38.1 57.1#


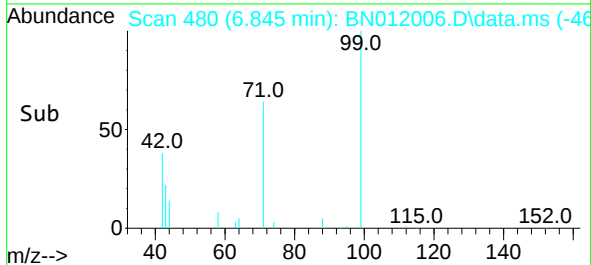
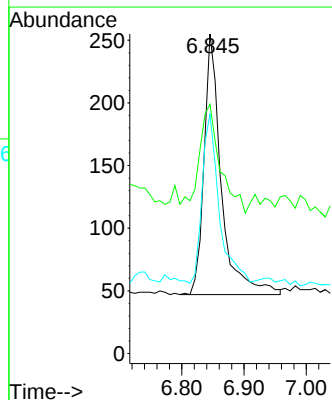
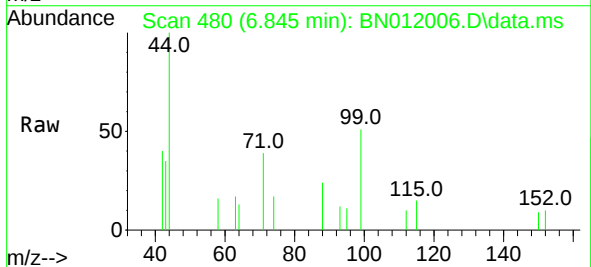


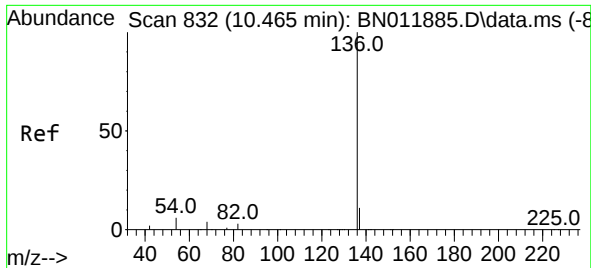

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.440 min Scan# 830
Delta R.T. -0.013 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41




Instrument :
BNA_N
ClientSampleId :
MW201D1-20200919


Tgt Ion:136	Resp:	6334
Ion Ratio	Lower	Upper
136	100	
137	12.3	9.5 14.3
54	14.3	5.6 8.4#
68	7.2	3.2 4.8#

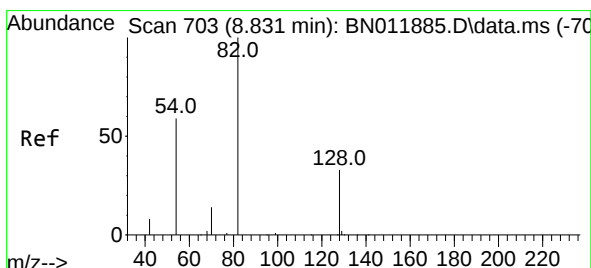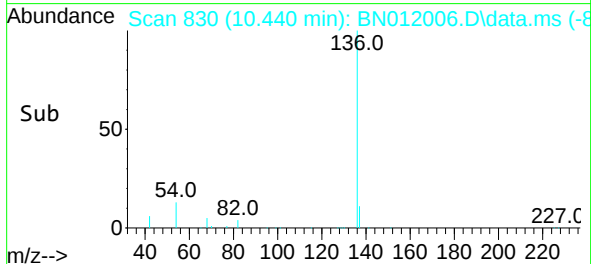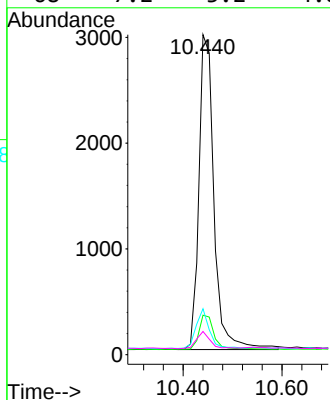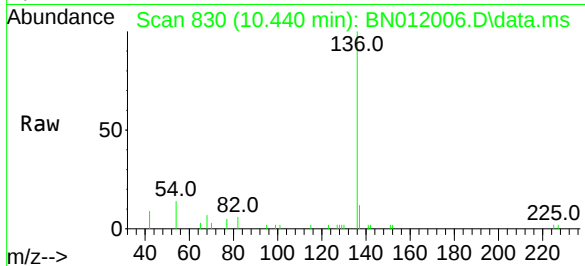

#8
Nitrobenzene-d5
Concen: 0.36 ng
RT: 8.818 min Scan# 702
Delta R.T. -0.000 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41

Tgt Ion: 82	Resp:	2383
Ion Ratio	Lower	Upper
82	100	
128	34.3	34.2 51.2
54	65.7	43.1 64.7#


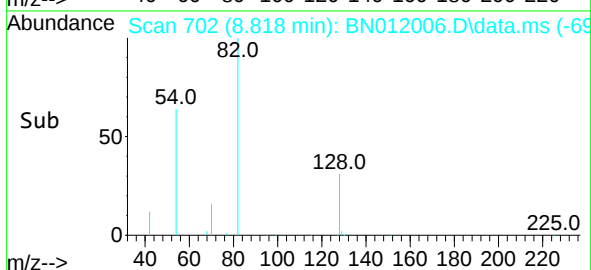
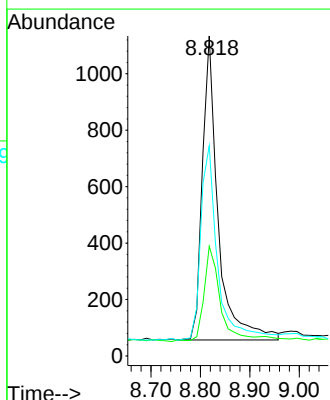
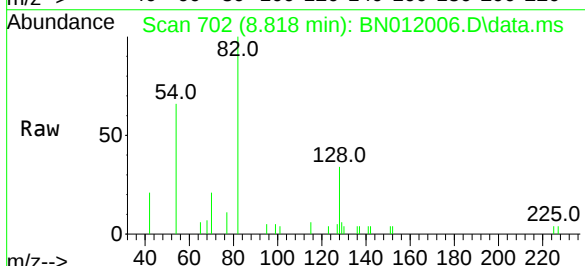


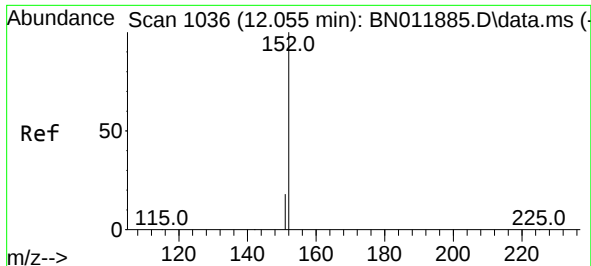

#11
2-Methylnaphthalene-d10
Concen: 0.34 ng
RT: 12.038 min Scan# 1032
Delta R.T. -0.009 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41




Instrument :
BNA_N
ClientSampleId :
MW201D1-20200919


Tgt Ion:152 Resp: 3456
Ion Ratio Lower Upper
152 100
151 20.2 16.7 25.1

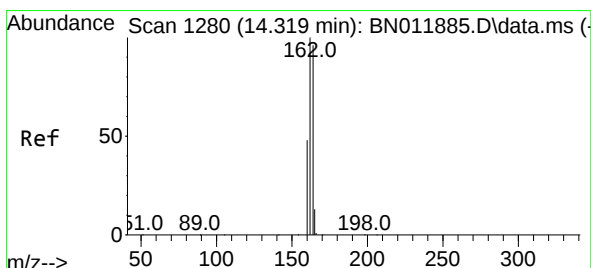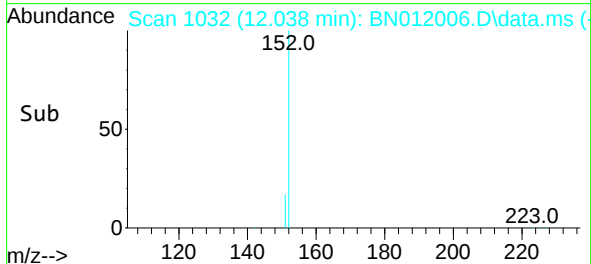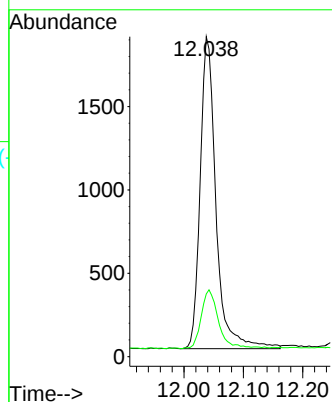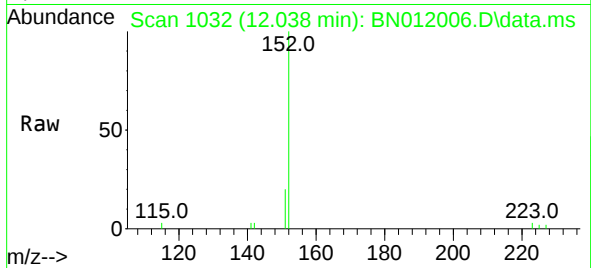

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.306 min Scan# 1279
Delta R.T. -0.000 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41

Tgt Ion:164 Resp: 3564
Ion Ratio Lower Upper
164 100
162 98.6 83.6 125.4
160 46.4 41.2 61.8


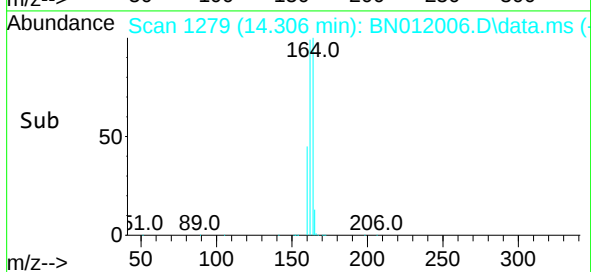
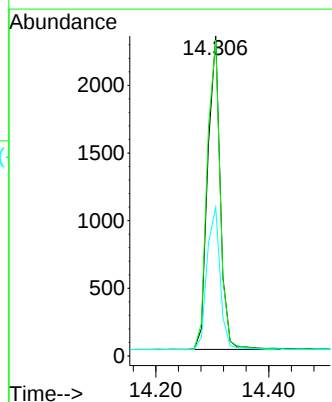
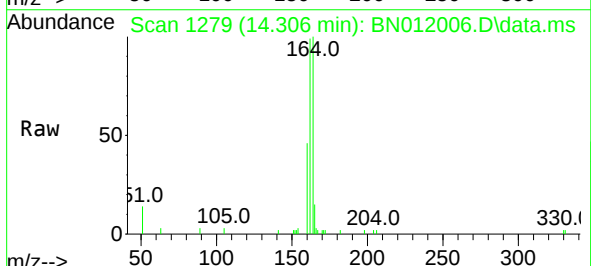


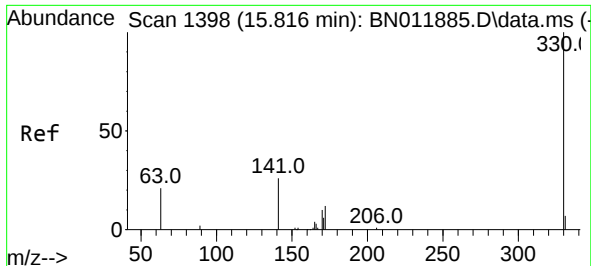

#14
2,4,6-Tribromophenol
Concen: 0.44 ng
RT: 15.803 min Scan# 1397
Delta R.T. -0.000 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41




Instrument :
BNA_N
ClientSampleId :
MW201D1-20200919


Tgt Ion:330 Resp: 764
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 57.3 33.7 50.5#

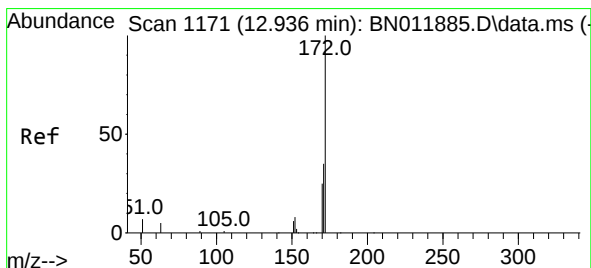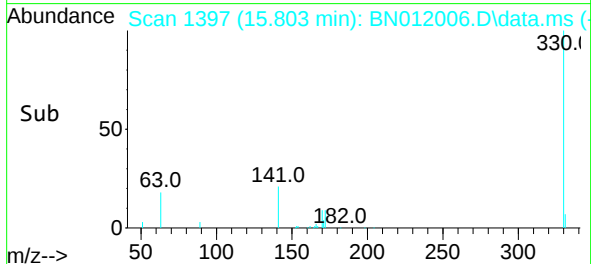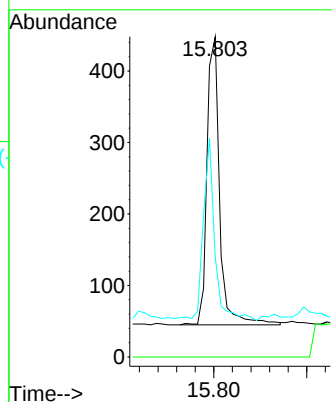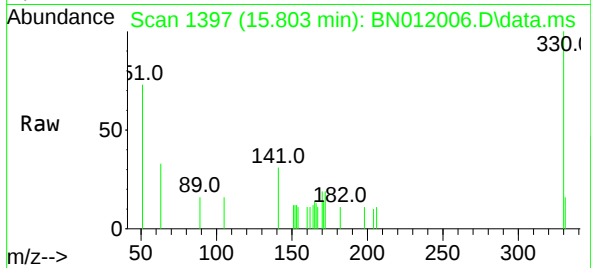

#15
2-Fluorobiphenyl
Concen: 0.34 ng
RT: 12.923 min Scan# 1170
Delta R.T. -0.013 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41

Tgt Ion:172 Resp: 4525
Ion Ratio Lower Upper
172 100
171 35.5 27.4 41.2
170 24.3 17.8 26.6


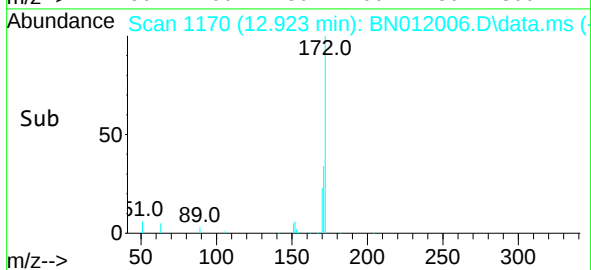
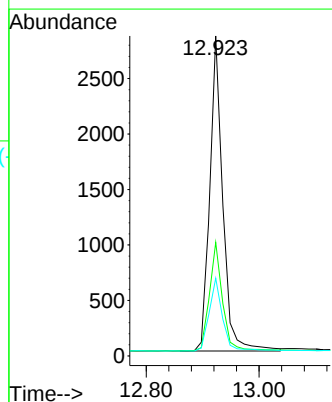
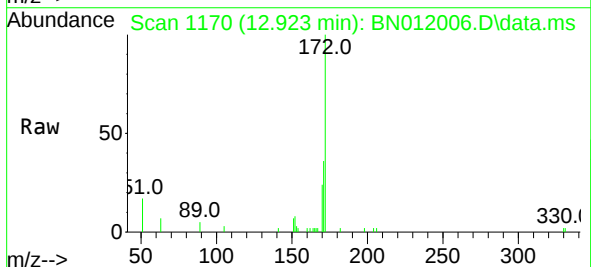


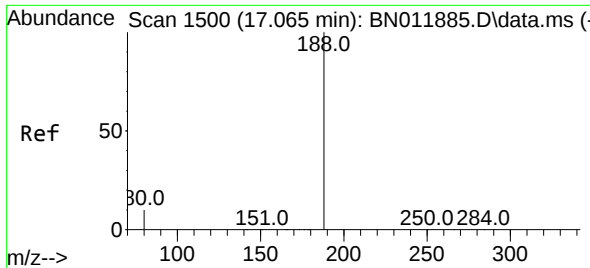

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.053 min Scan# 1499
Delta R.T. -0.000 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41




Instrument :
BNA_N
ClientSampleId :
MW201D1-20200919


Tgt Ion:188 Resp: 6876
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.2 7.7 11.5

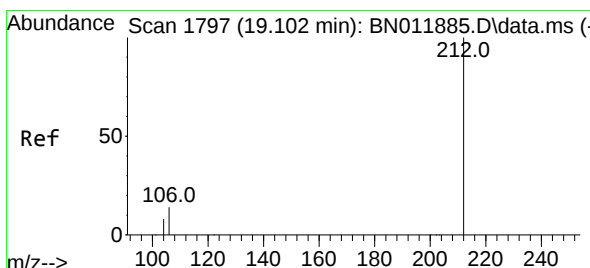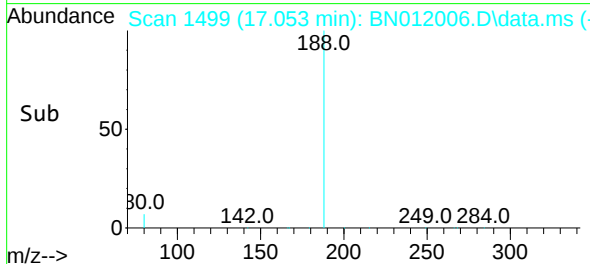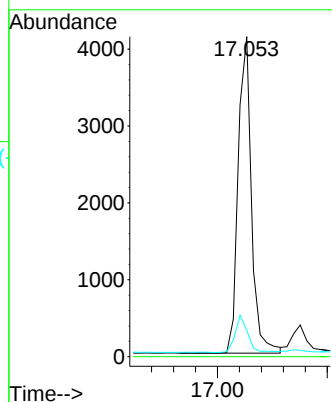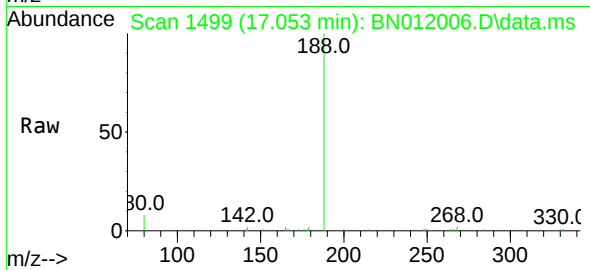

#27
Fluoranthene-d10
Concen: 0.42 ng
RT: 19.087 min Scan# 1794
Delta R.T. -0.005 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41

Tgt Ion:212 Resp: 8395
Ion Ratio Lower Upper
212 100
106 11.4 6.4 9.6#
104 7.1 3.9 5.9#


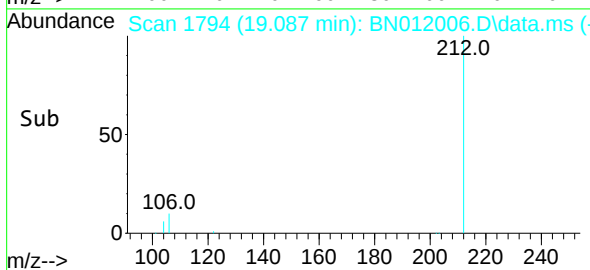
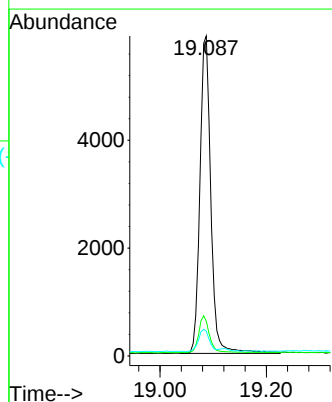
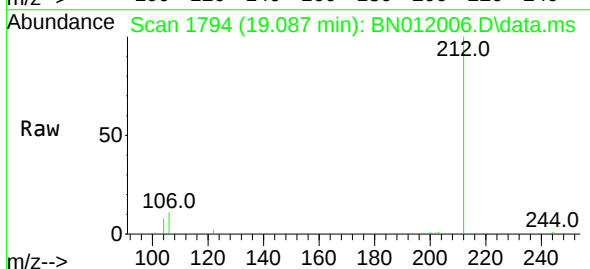


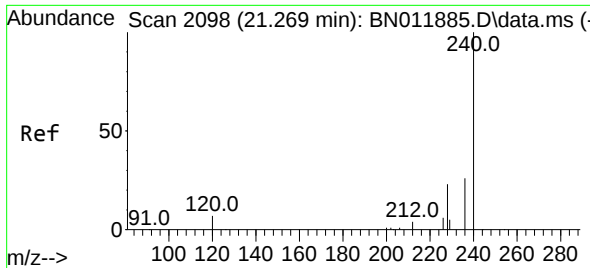

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.248 min Scan# 2096
Delta R.T. -0.011 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41




Instrument :
BNA_N
ClientSampleId :
MW201D1-20200919


Tgt Ion:240 Resp: 6545
Ion Ratio Lower Upper
240 100
120 10.7 3.5 5.3#
236 26.9 20.5 30.7

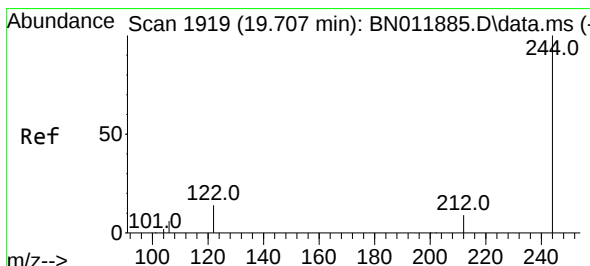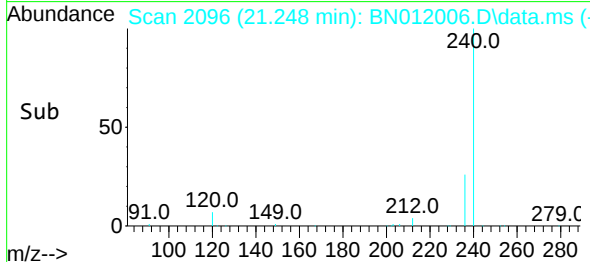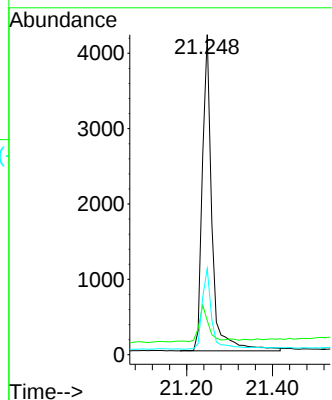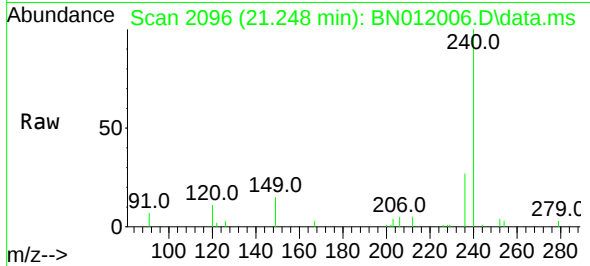

#31
Terphenyl-d14
Concen: 0.48 ng
RT: 19.688 min Scan# 1915
Delta R.T. -0.010 min
Lab File: BN012006.D
Acq: 29 Sep 2020 05:41

Tgt Ion:244 Resp: 7251
Ion Ratio Lower Upper
244 100
212 10.3 7.3 10.9
122 13.7 7.8 11.6#


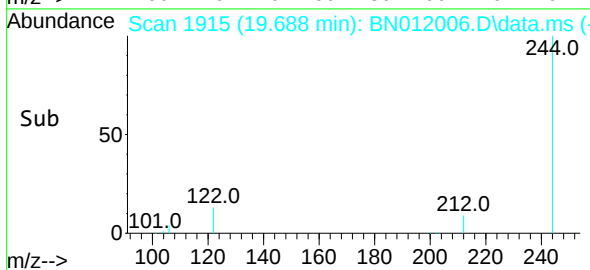
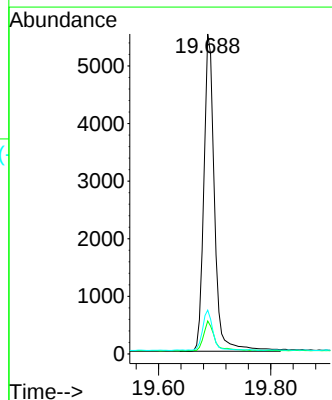
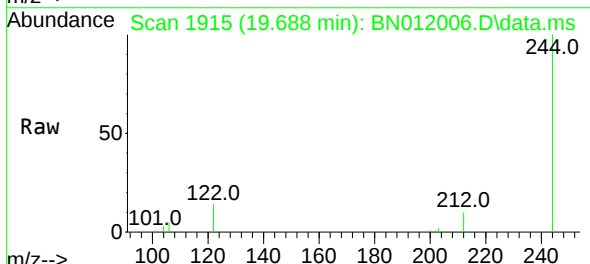


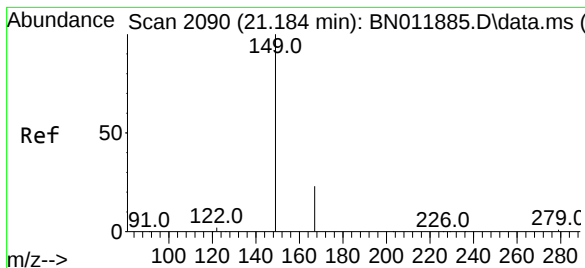

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.07 ng
 RT: 21.163 min Scan# 2088
 Delta R.T. -0.011 min
 Lab File: BN012006.D
 Acq: 29 Sep 2020 05:41

Instrument :
 BNA_N
 ClientSampleId :
 MW201D1-20200919

Tgt Ion:149 Resp: 988
 Ion Ratio Lower Upper
 149 100
 167 23.8 23.6 35.4
 279 5.8 4.0 6.0

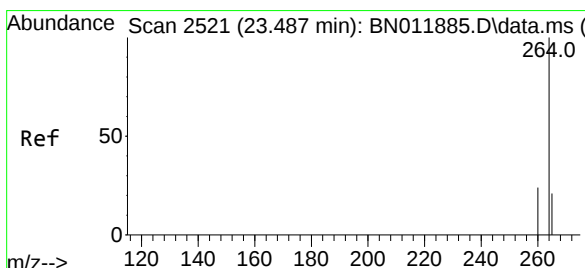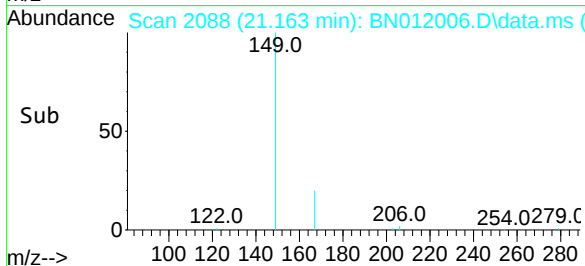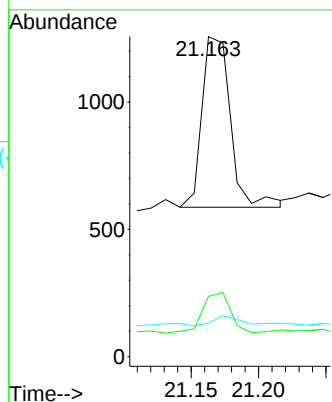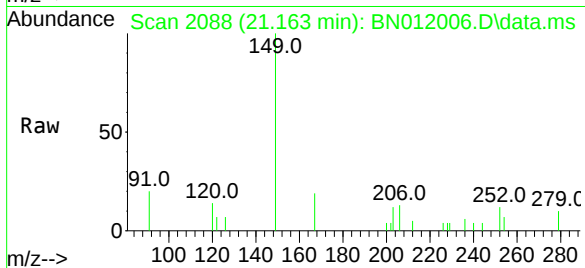

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.456 min Scan# 2512
 Delta R.T. -0.014 min
 Lab File: BN012006.D
 Acq: 29 Sep 2020 05:41

Tgt Ion:264 Resp: 6849
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.6 29.4
 265 61.1 38.6 58.0#

