
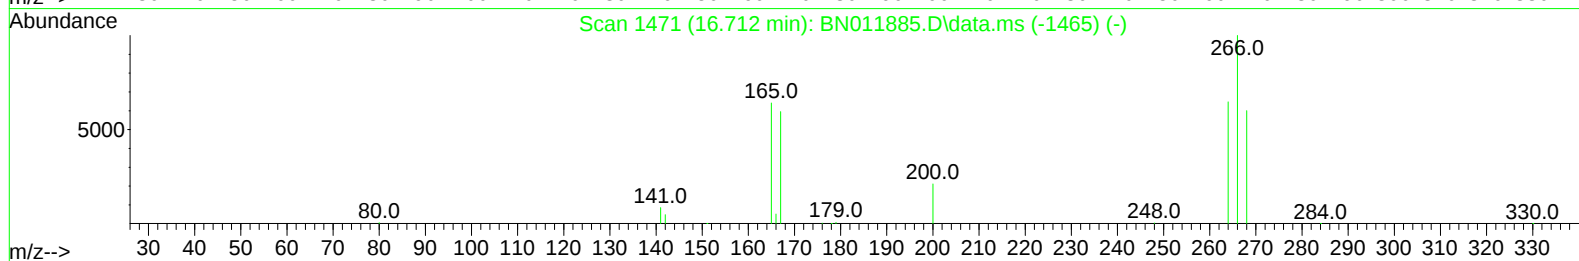
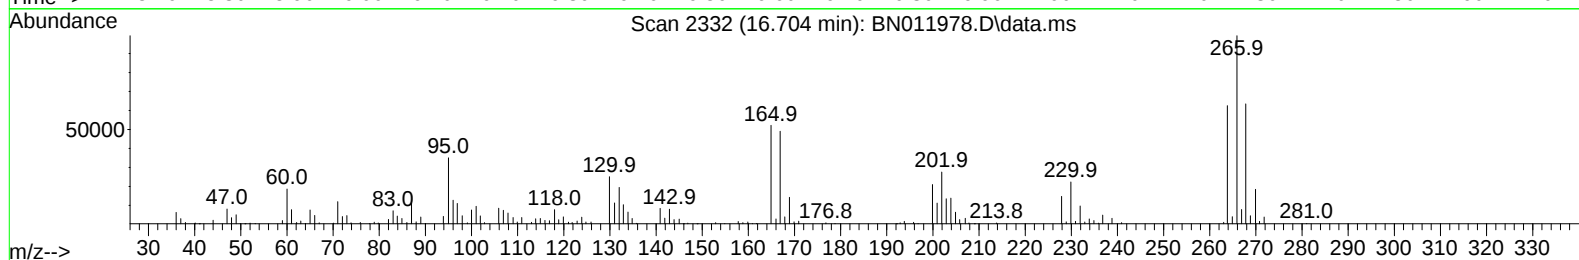


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092820\
Data File : BN011978.D
Acq On : 28 Sep 2020 09:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 04:57:53 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 11:18:41 2020
Response via : Initial Calibration

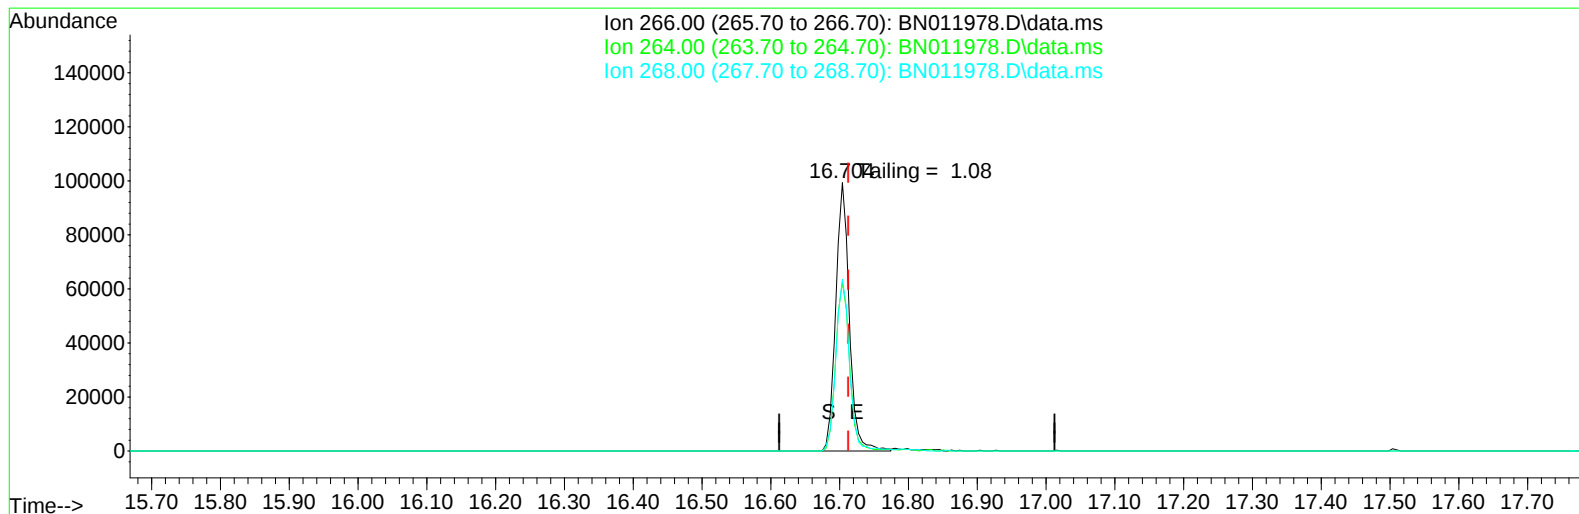

TIC: BN011978.D\data.ms

(24) Pentachlorophenol

16.704min (-0.009) 0.00 ng

response 136021

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.00	64.82
268.00	65.50	64.95
0.00	0.00	0.00