

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092820\
 Data File : BN012011.D
 Acq On : 29 Sep 2020 08:42
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Sep 29 09:17:36 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 25 11:18:41 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	1852	0.40	ng	0.00
7) Naphthalene-d8	10.440	136	7763	0.40	ng	#-0.01
13) Acenaphthene-d10	14.306	164	4000	0.40	ng	0.00
19) Phenanthrene-d10	17.053	188	7693	0.40	ng	0.00
29) Chrysene-d12	21.248	240	6969	0.40	ng	#-0.01
36) Perylene-d12	23.460	264	7328	0.40	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.275	112	2567	0.40	ng	0.00
5) Phenol-d6	6.845	99	3255	0.40	ng	0.00
8) Nitrobenzene-d5	8.818	82	3234	0.40	ng	0.00
11) 2-Methylnaphthalene-d10	12.038	152	4628	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.790	330	843	0.43	ng	-0.01
15) 2-Fluorobiphenyl	12.923	172	5805	0.38	ng	-0.01
27) Fluoranthene-d10	19.087	212	8429	0.37	ng	0.00
31) Terphenyl-d14	19.693	244	6187	0.39	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.253	88	1346	0.42	ng	91
3) n-Nitrosodimethylamine	3.559	42	2166	0.47	ng	92
6) bis(2-Chloroethyl)ether	7.103	93	2701	0.39	ng	92
9) Naphthalene	10.491	128	8371	0.38	ng	99
10) Hexachlorobutadiene	10.782	225	1528	0.42	ng	# 96
12) 2-Methylnaphthalene	12.113	142	5306	0.38	ng	95
16) Acenaphthylene	14.014	152	7210	0.37	ng	99
17) Acenaphthene	14.369	154	4912	0.37	ng	93
18) Fluorene	15.359	166	5920	0.37	ng	100
20) 4,6-Dinitro-2-methylph...	15.435	198	584	0.40	ng	# 1
21) 4-Bromophenyl-phenylether	16.250	248	1628	0.40	ng	# 82
22) Hexachlorobenzene	16.360	284	1950	0.41	ng	# 81
23) Atrazine	16.518	200	1574	0.40	ng	96
24) Pentachlorophenol	16.700	266	872	0.38	ng	98
25) Phenanthrene	17.090	178	8650	0.37	ng	99
26) Anthracene	17.175	178	7813	0.38	ng	99
28) Fluoranthene	19.117	202	9623	0.36	ng	# 96
30) Pyrene	19.479	202	9797	0.38	ng	100
32) Benzo(a)anthracene	21.237	228	7965	0.36	ng	98
33) Chrysene	21.280	228	9143	0.38	ng	98
34) Bis(2-ethylhexyl)phtha...	21.174	149	5963	0.38	ng	92
35) Indeno(1,2,3-cd)pyrene	25.667	276	10865	0.40	ng	# 95
37) Benzo(b)fluoranthene	22.799	252	8736	0.35	ng	# 83
38) Benzo(k)fluoranthene	22.844	252	9635	0.35	ng	# 85
39) Benzo(a)pyrene	23.364	252	8388	0.36	ng	# 77
40) Dibenzo(a,h)anthracene	25.685	278	8978	0.38	ng	# 87
41) Benzo(g,h,i)perylene	26.342	276	9629	0.37	ng	# 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092820\
Data File : BN012011.D
Acq On : 29 Sep 2020 08:42
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Sep 29 09:17:36 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 11:18:41 2020
Response via : Initial Calibration

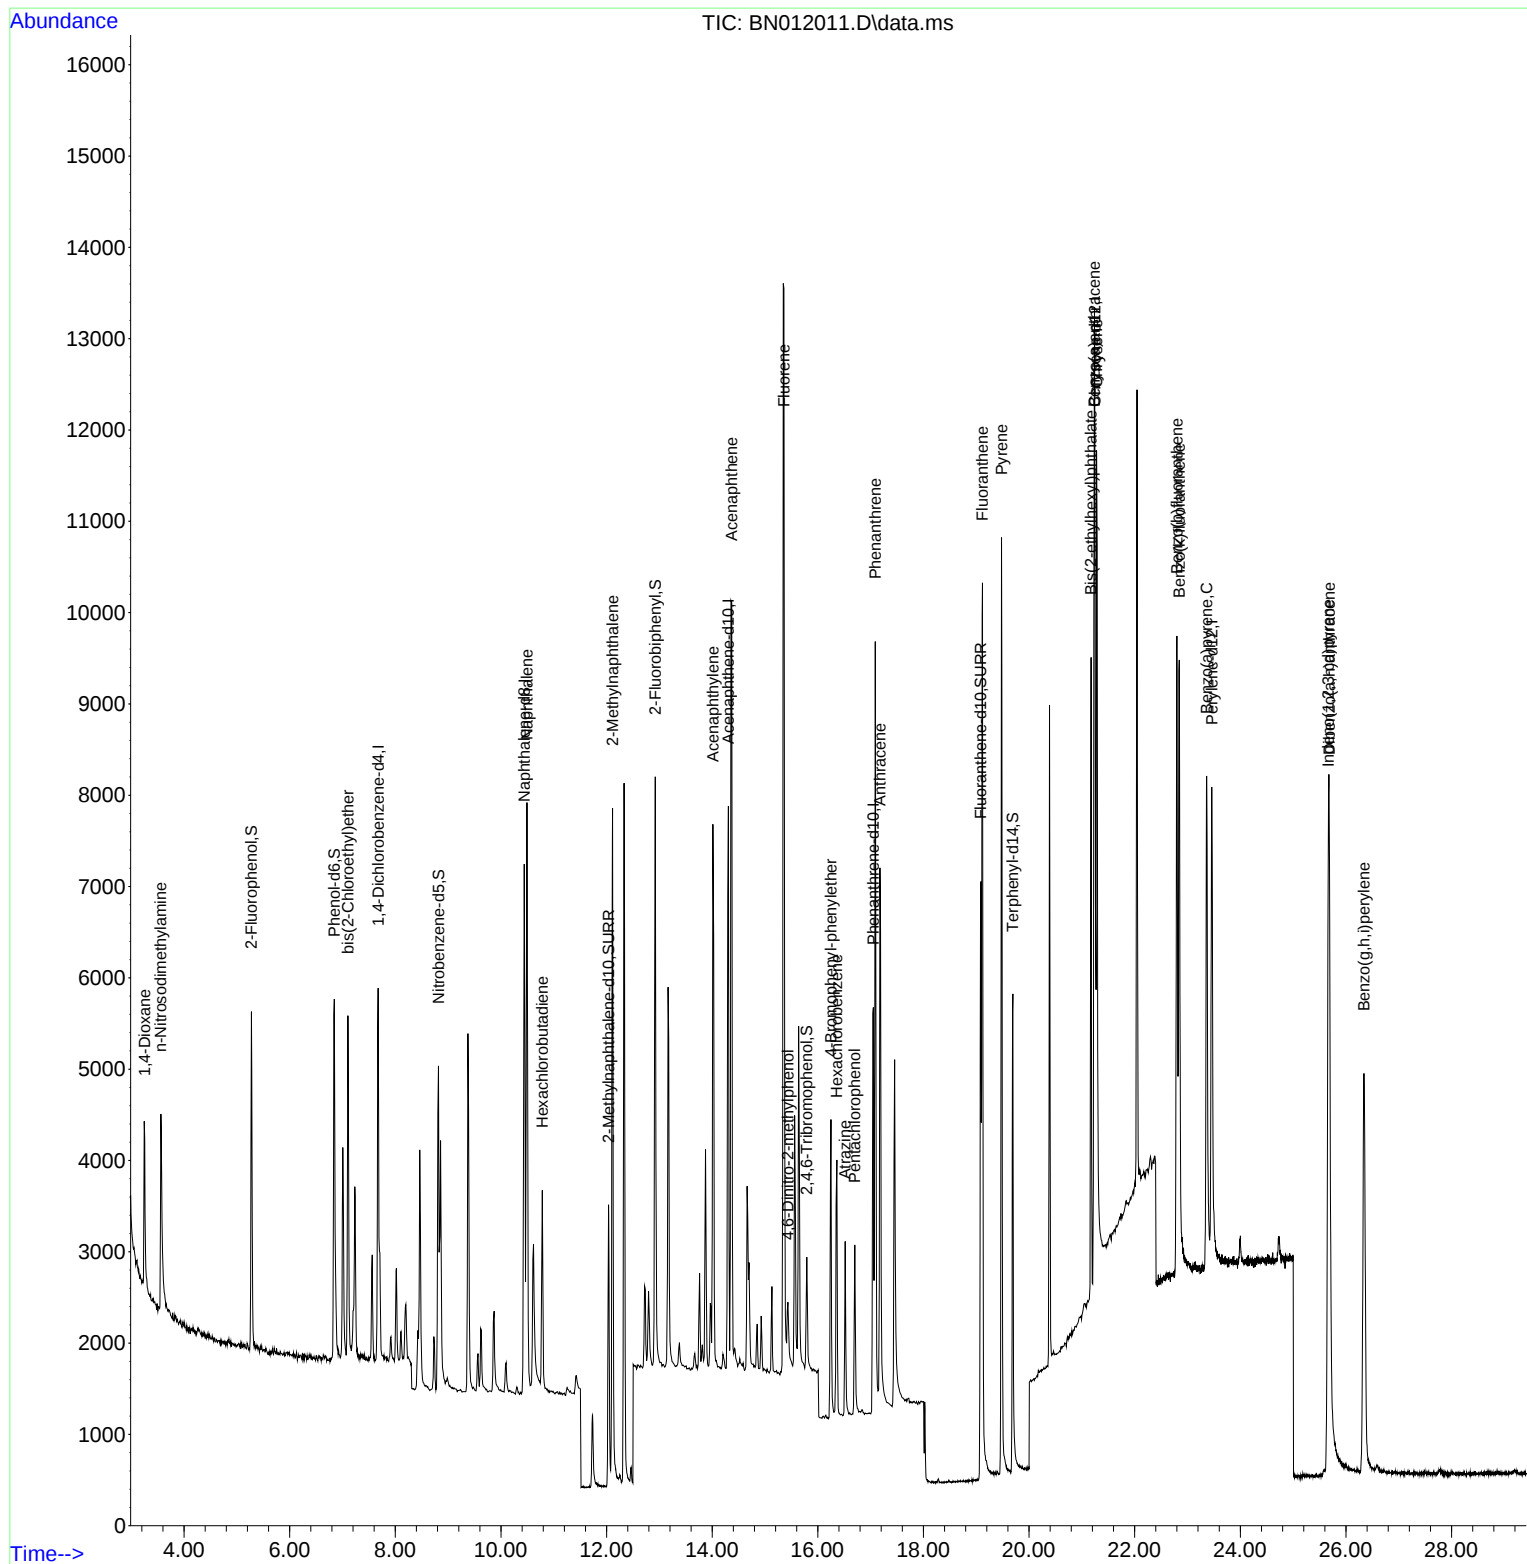






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.675 min Scan# 583
 Delta R.T. -0.008 min
 Lab File: BN012011.D
 Acq: 29 Sep 2020 08:42

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:152 Resp: 1852




Ion	Ratio	Lower	Upper
152	100		
150	156.6	118.3	177.5
115	76.2	51.3	76.9

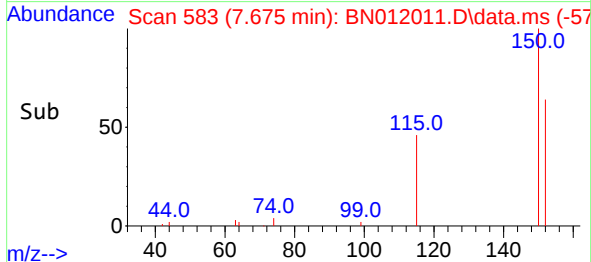


#2
 1,4-Dioxane
 Concen: 0.42 ng
 RT: 3.253 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: BN012011.D
 Acq: 29 Sep 2020 08:42

Tgt Ion: 88 Resp: 1346

Ion	Ratio	Lower	Upper
88	100		
58	70.7	63.3	94.9
43	46.1	33.0	49.4






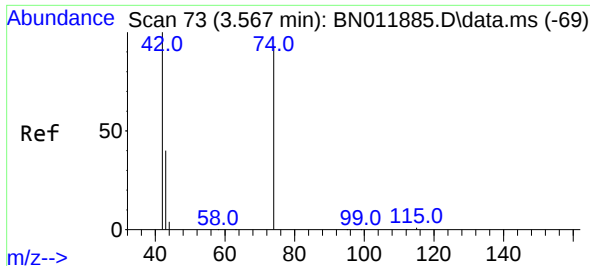


#3
n-Nitrosodimethylamine
Concen: 0.47 ng
RT: 3.559 min Scan# 72
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 42 Resp: 2166




Ion	Ratio	Lower	Upper
42	100		
74	73.1	64.4	96.6
44	7.7	6.7	10.1

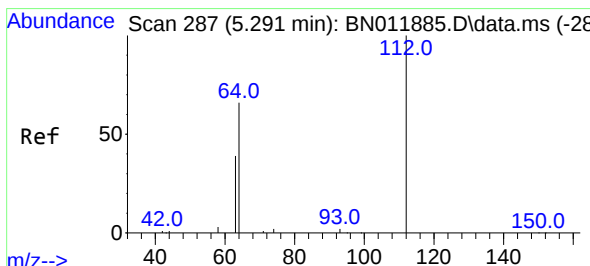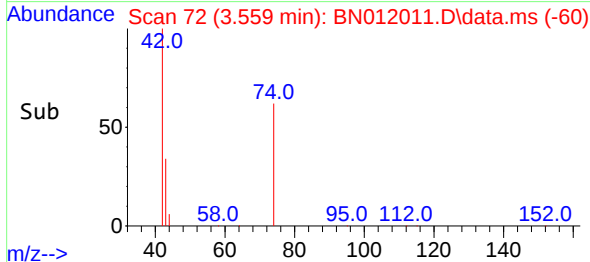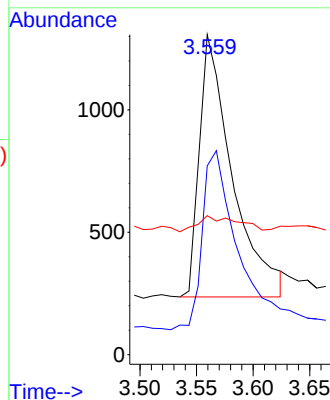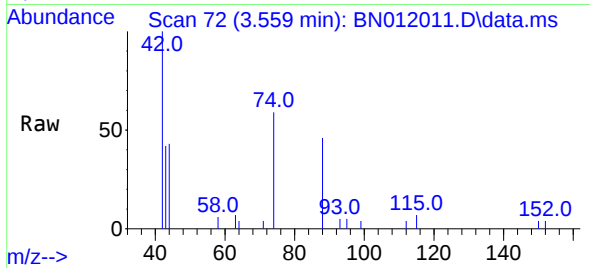

#4
2-Fluorophenol
Concen: 0.40 ng
RT: 5.275 min Scan# 285
Delta R.T. -0.008 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion: 112 Resp: 2567

Ion	Ratio	Lower	Upper
112	100		
64	71.6	49.0	73.6
63	46.4	31.8	47.6

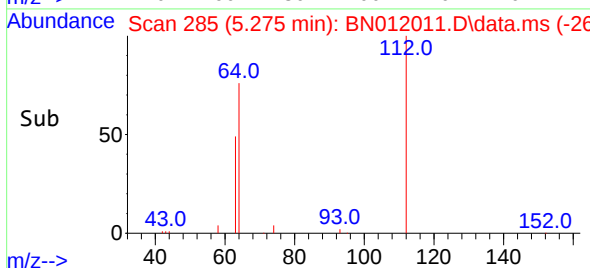
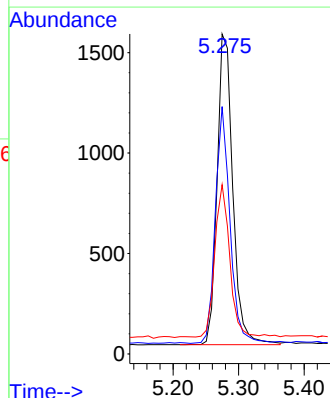
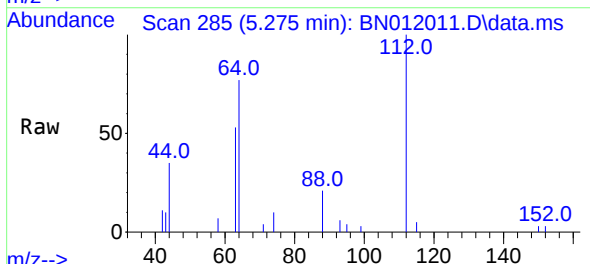




#5
Phenol-d6
Concen: 0.40 ng
RT: 6.845 min Scan# 480
Delta R.T. -0.008 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 3255
Ion Ratio Lower Upper
99 100
42 36.0 23.4 35.0#
71 53.8 38.1 57.1

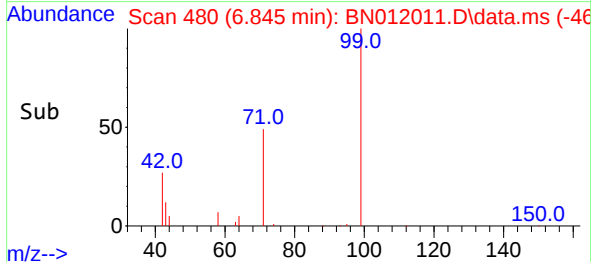

#6
bis(2-Chloroethyl)ether
Concen: 0.39 ng
RT: 7.103 min Scan# 512
Delta R.T. -0.008 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion: 93 Resp: 2701
Ion Ratio Lower Upper
93 100
63 85.1 61.1 91.7
95 30.6 25.5 38.3









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.440 min Scan# 830
Delta R.T. -0.013 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	7763
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.5	14.3
54	11.4	5.6	8.4#
68	6.7	3.2	4.8#

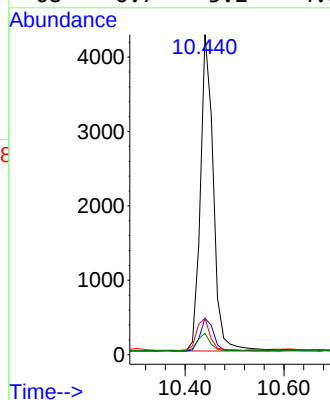

#8
Nitrobenzene-d5
Concen: 0.40 ng
RT: 8.818 min Scan# 702
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:	82	Resp:	3234
Ion	Ratio	Lower	Upper
82	100		
128	36.8	34.2	51.2
54	59.1	43.1	64.7



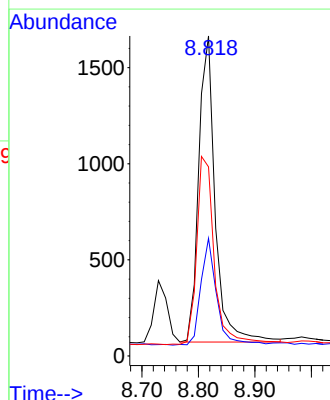



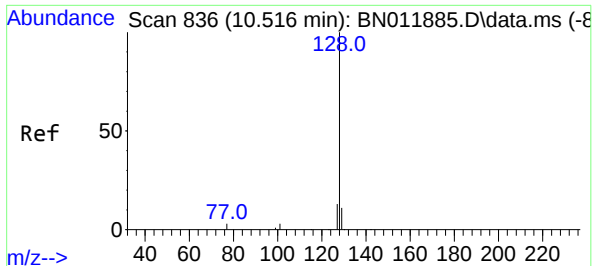

#9
Naphthalene
Concen: 0.38 ng
RT: 10.491 min Scan# 834
Delta R.T. -0.013 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	128	Resp:	8371
Ion	Ratio	Lower	Upper
128	100		
129	11.4	9.7	14.5
127	13.5	11.0	16.4

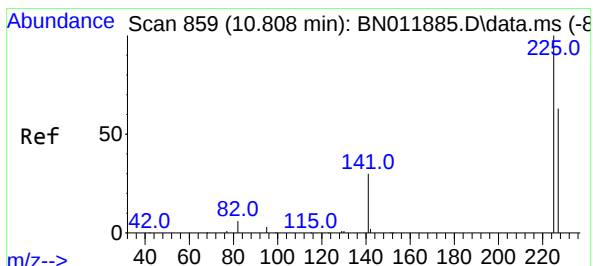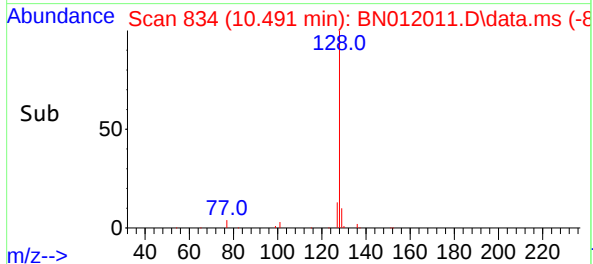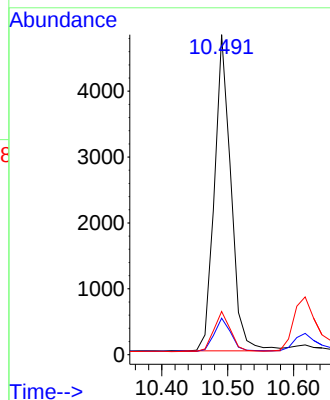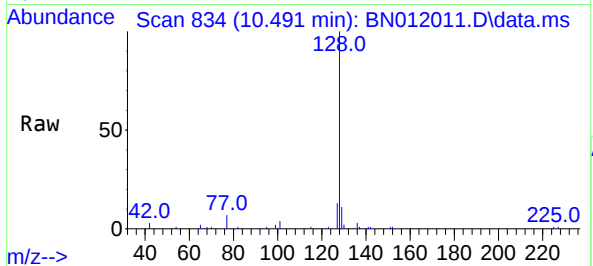

#10
Hexachlorobutadiene
Concen: 0.42 ng
RT: 10.782 min Scan# 857
Delta R.T. -0.013 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:	225	Resp:	1528
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	62.0	51.9	77.9


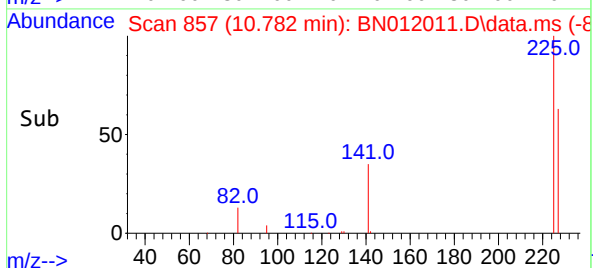
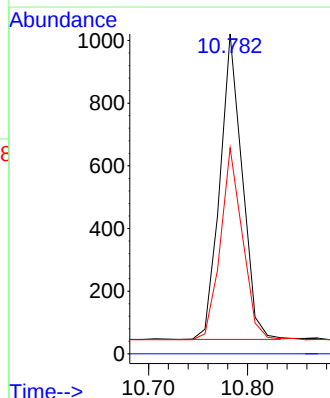
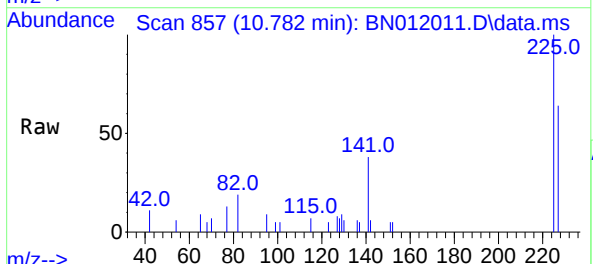




#11
2-Methylnaphthalene-d10
Concen: 0.38 ng
RT: 12.038 min Scan# 1032
Delta R.T. -0.009 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 4628
Ion Ratio Lower Upper
152 100
151 20.1 16.7 25.1

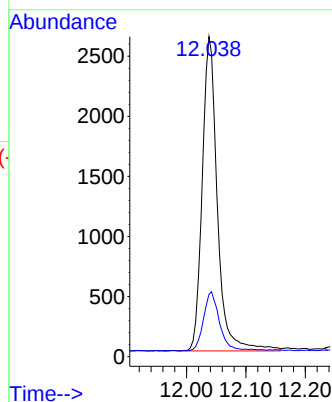

#12
2-Methylnaphthalene
Concen: 0.38 ng
RT: 12.113 min Scan# 1049
Delta R.T. -0.009 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:142 Resp: 5306
Ion Ratio Lower Upper
142 100
141 88.6 70.0 105.0
115 52.6 35.8 53.6









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.306 min Scan# 1279
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:164 Resp: 4000
Ion Ratio Lower Upper
164 100
162 99.3 83.6 125.4
160 46.5 41.2 61.8

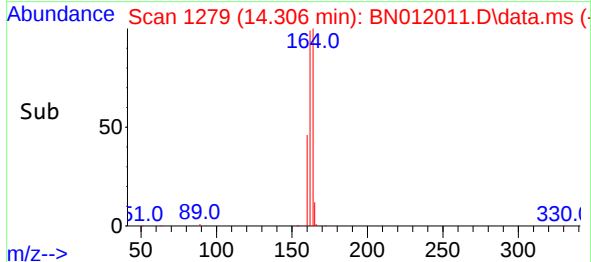

#14
2,4,6-Tribromophenol
Concen: 0.43 ng
RT: 15.790 min Scan# 1396
Delta R.T. -0.013 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:330 Resp: 843
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 49.0 33.7 50.5


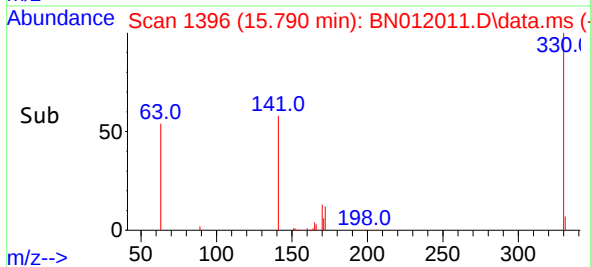

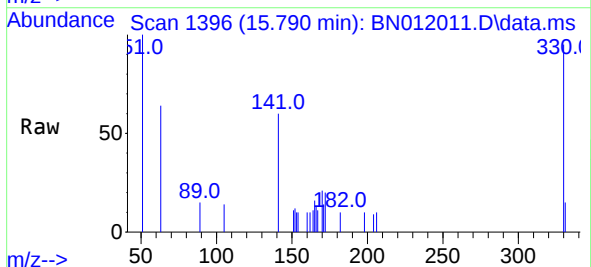




#15
2-Fluorobiphenyl
Concen: 0.38 ng
RT: 12.923 min Scan# 1170
Delta R.T. -0.013 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	172	Resp:	5805
Ion Ratio	Lower	Upper	
172	100		
171	35.0	27.4	41.2
170	24.1	17.8	26.6

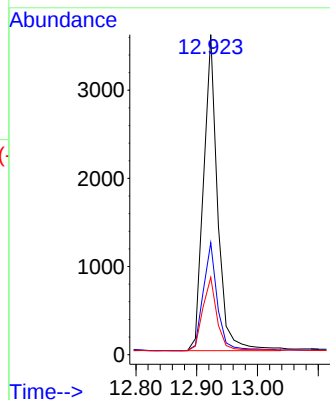

#16
Acenaphthylene
Concen: 0.37 ng
RT: 14.014 min Scan# 1256
Delta R.T. -0.013 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:	152	Resp:	7210
Ion Ratio	Lower	Upper	
152	100		
151	19.7	15.9	23.9
153	12.7	10.5	15.7



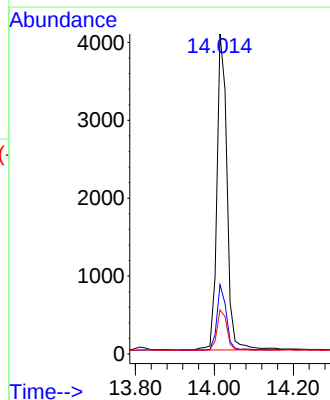





#17
Acenaphthene
Concen: 0.37 ng
RT: 14.369 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:154 Resp: 4912
Ion Ratio Lower Upper
154 100
153 112.9 83.4 125.2
152 56.6 42.8 64.2

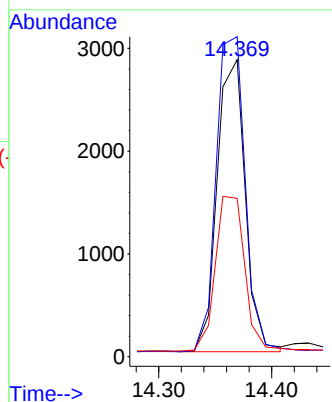

#18
Fluorene
Concen: 0.37 ng
RT: 15.359 min Scan# 1362
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:166 Resp: 5920
Ion Ratio Lower Upper
166 100
165 98.7 78.8 118.2
167 13.2 11.2 16.8









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.053 min Scan# 1499
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:188 Resp: 7693
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.9 7.7 11.5



#20
4,6-Dinitro-2-methylphenol
Concen: 0.40 ng
RT: 15.435 min Scan# 1368
Delta R.T. -0.013 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:198 Resp: 584
Ion Ratio Lower Upper
198 100
51 190.5 45.0 67.4#
105 57.1 30.4 45.6#









#21
4-Bromophenyl-phenylether
Concen: 0.40 ng
RT: 16.250 min Scan# 1433
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 1628
Ion Ratio Lower Upper
248 100
250 98.8 82.7 124.1
141 75.0 33.7 50.5#



#22
Hexachlorobenzene
Concen: 0.41 ng
RT: 16.360 min Scan# 1442
Delta R.T. -0.012 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:284 Resp: 1950
Ion Ratio Lower Upper
284 100
142 62.0 32.4 48.6#
249 33.0 26.8 40.2







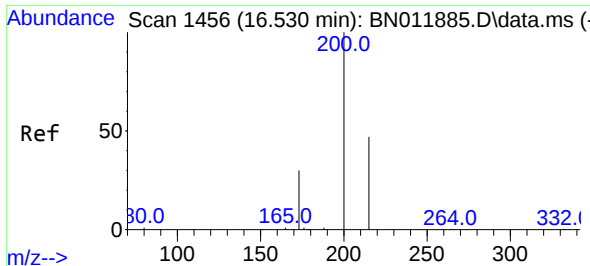

#23
Atrazine
Concen: 0.40 ng
RT: 16.518 min Scan# 1455
Delta R.T. -0.012 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:200 Resp: 1574
Ion Ratio Lower Upper
200 100
173 27.6 18.7 28.1
215 49.2 40.2 60.4

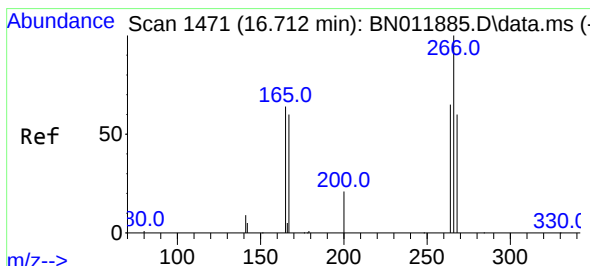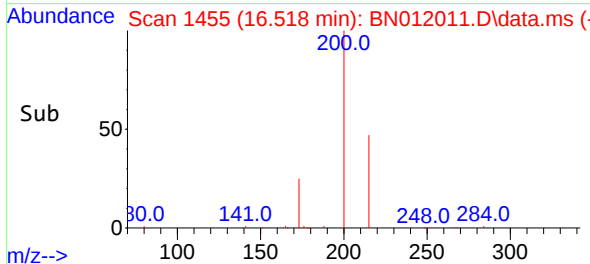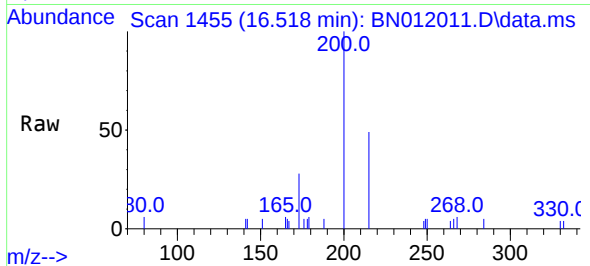

#24
Pentachlorophenol
Concen: 0.38 ng
RT: 16.700 min Scan# 1470
Delta R.T. -0.012 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:266 Resp: 872
Ion Ratio Lower Upper
266 100
264 66.6 51.2 76.8
268 65.8 52.4 78.6

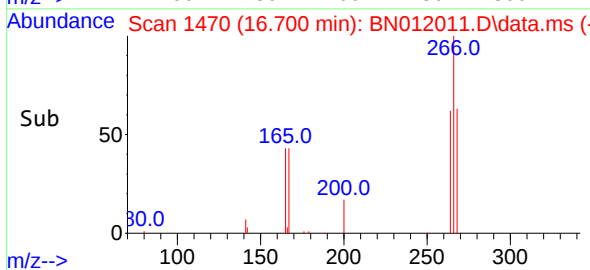

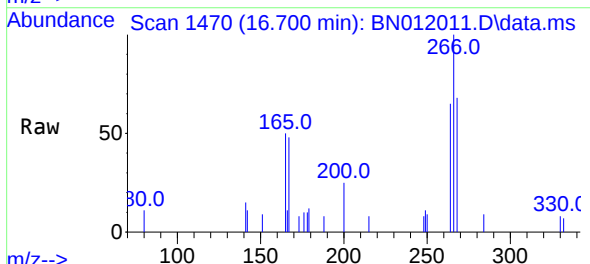




#25
Phenanthrene
Concen: 0.37 ng
RT: 17.090 min Scan# 1502
Delta R.T. -0.012 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:178 Resp: 8650
Ion Ratio Lower Upper
178 100
176 19.3 15.1 22.7
179 15.4 12.3 18.5

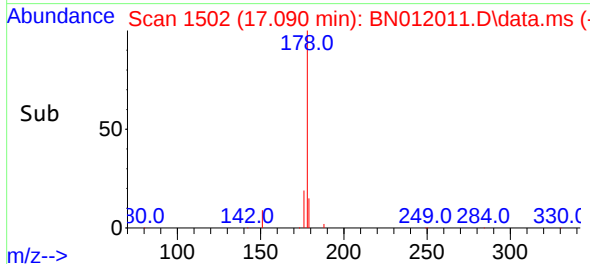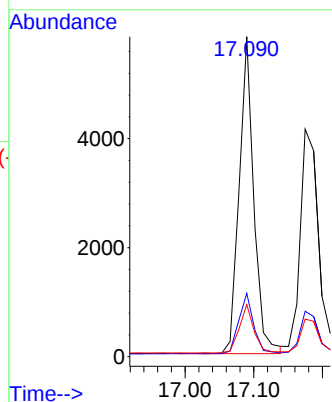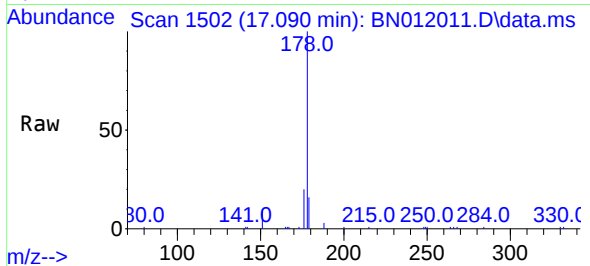

#26
Anthracene
Concen: 0.38 ng
RT: 17.175 min Scan# 1509
Delta R.T. -0.012 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:178 Resp: 7813
Ion Ratio Lower Upper
178 100
176 18.4 14.6 21.8
179 15.2 12.4 18.6


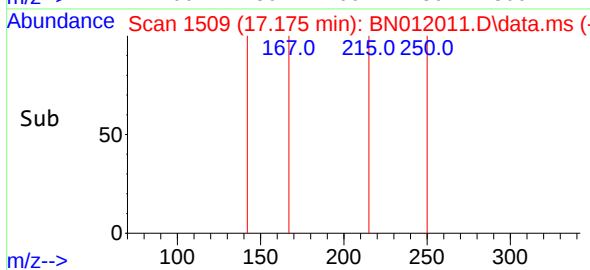
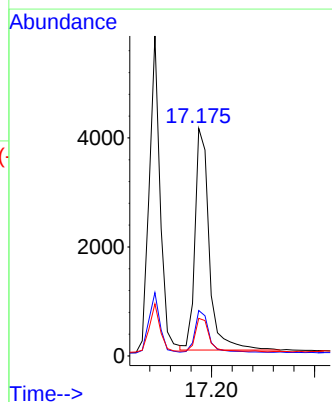
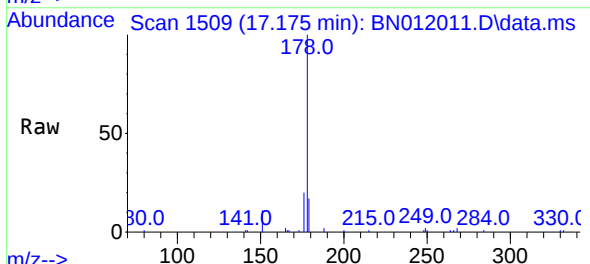




#27
Fluoranthene-d10
Concen: 0.37 ng
RT: 19.087 min Scan# 1794
Delta R.T. -0.005 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:212 Resp: 8429
Ion Ratio Lower Upper
212 100
106 10.9 6.4 9.6#
104 7.0 3.9 5.9#

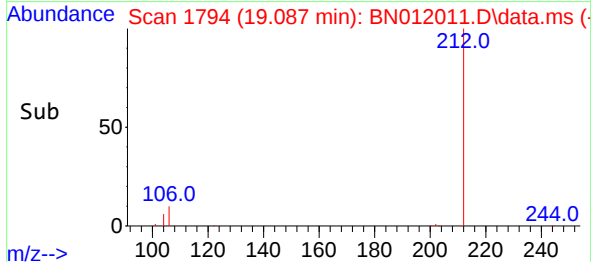

#28
Fluoranthene
Concen: 0.36 ng
RT: 19.117 min Scan# 1800
Delta R.T. -0.005 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:202 Resp: 9623
Ion Ratio Lower Upper
202 100
101 10.0 5.4 8.2#
203 16.5 13.8 20.6

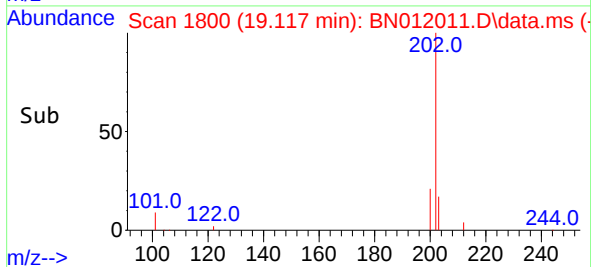

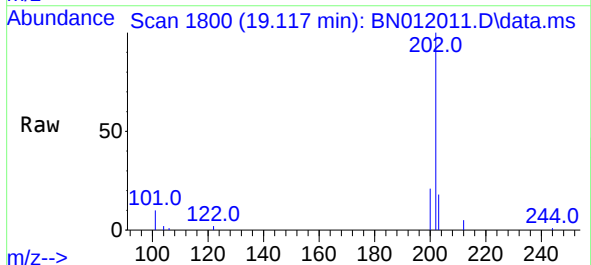




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.248 min Scan# 2096
Delta R.T. -0.011 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 6969
Ion Ratio Lower Upper
240 100
120 10.9 3.5 5.3#
236 26.0 20.5 30.7



#30
Pyrene
Concen: 0.38 ng
RT: 19.479 min Scan# 1873
Delta R.T. -0.005 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:202 Resp: 9797
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.7 13.9 20.9









#31
Terphenyl-d14
Concen: 0.39 ng
RT: 19.693 min Scan# 1916
Delta R.T. -0.005 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:244 Resp: 6187
Ion Ratio Lower Upper
244 100
212 9.9 7.3 10.9
122 12.6 7.8 11.6#

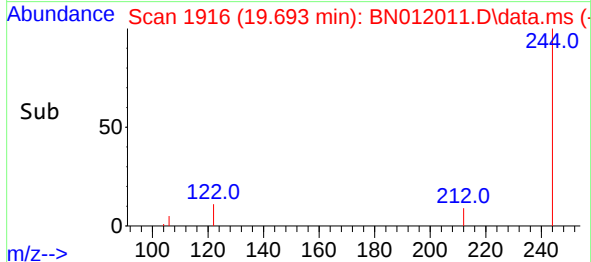

#32
Benzo(a)anthracene
Concen: 0.36 ng
RT: 21.237 min Scan# 2095
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:228 Resp: 7965
Ion Ratio Lower Upper
228 100
226 26.7 21.0 31.4
229 21.1 16.0 24.0


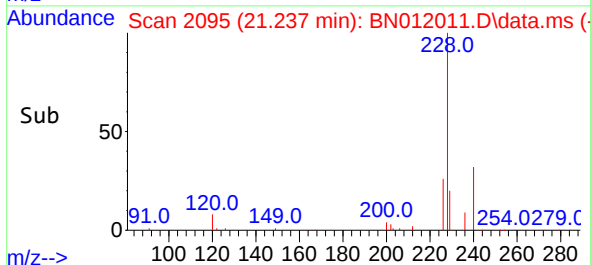
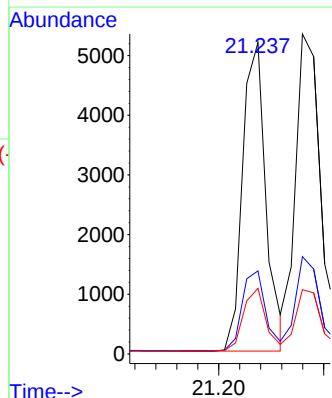
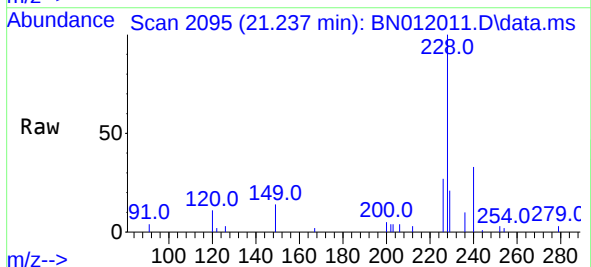




#33
Chrysene
Concen: 0.38 ng
RT: 21.280 min Scan# 2099
Delta R.T. -0.011 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	228	Resp:	9143
Ion Ratio	Lower	Upper	
228	100		
226	30.4	23.3	34.9
229	20.1	15.8	23.8

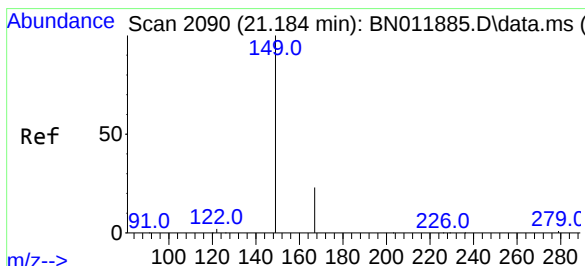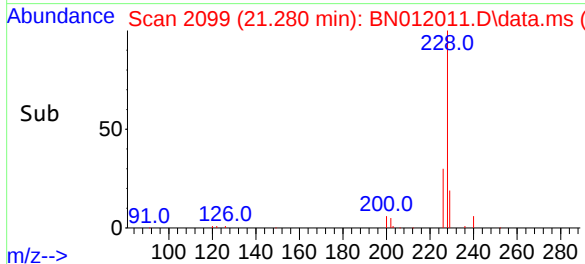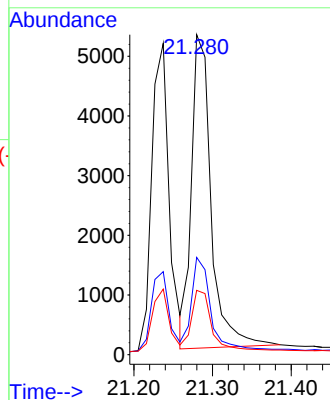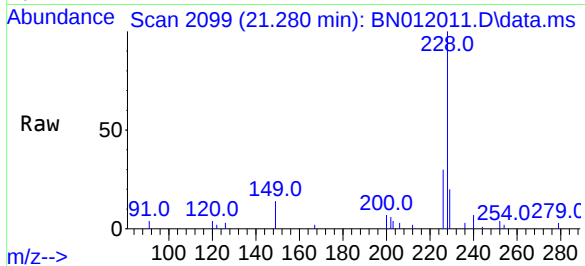

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.38 ng
RT: 21.174 min Scan# 2089
Delta R.T. -0.000 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:	149	Resp:	5963
Ion Ratio	Lower	Upper	
149	100		
167	24.8	23.6	35.4
279	4.6	4.0	6.0


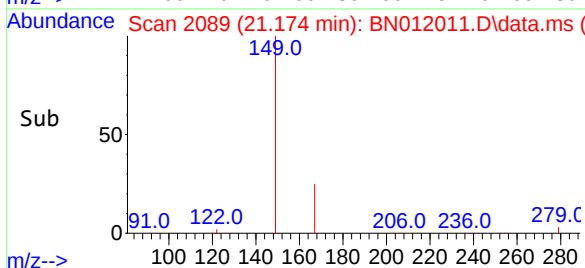
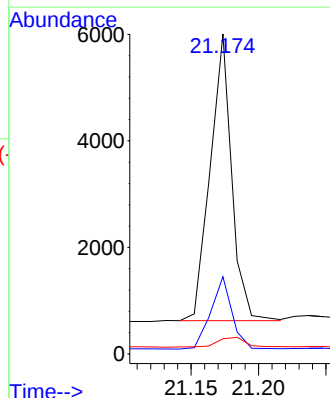
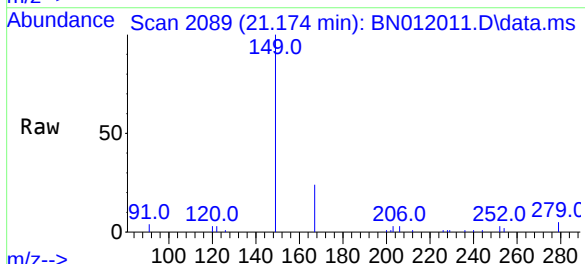




#35
Indeno(1,2,3-cd)pyrene
Concen: 0.40 ng
RT: 25.667 min Scan# 3158
Delta R.T. -0.014 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:276 Resp: 10865
Ion Ratio Lower Upper
276 100
138 20.6 13.0 19.4#
277 24.4 20.0 30.0



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.460 min Scan# 2513
Delta R.T. -0.010 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:264 Resp: 7328
Ion Ratio Lower Upper
264 100
260 23.8 19.6 29.4
265 63.9 38.6 58.0#





#37

Benzo(b)fluoranthene

Concen: 0.35 ng

RT: 22.799 min Scan# 2320

Delta R.T. -0.007 min

Lab File: BN012011.D

Acq: 29 Sep 2020 08:42





Tgt Ion:252 Resp: 8736

Ion Ratio Lower Upper

252 100

253 30.6 19.1 28.7#

125 16.8 6.2 9.2#

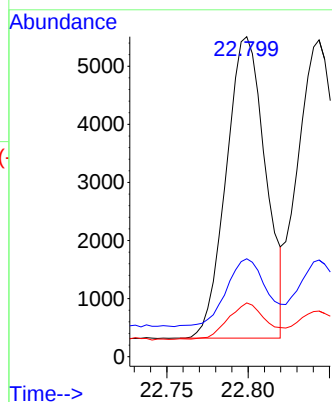

#38

Benzo(k)fluoranthene

Concen: 0.35 ng

RT: 22.844 min Scan# 2333

Delta R.T. -0.003 min

Lab File: BN012011.D

Acq: 29 Sep 2020 08:42




Tgt Ion:252 Resp: 9635

Ion Ratio Lower Upper

252 100

253 30.5 19.3 28.9#

125 14.4 6.0 9.0#




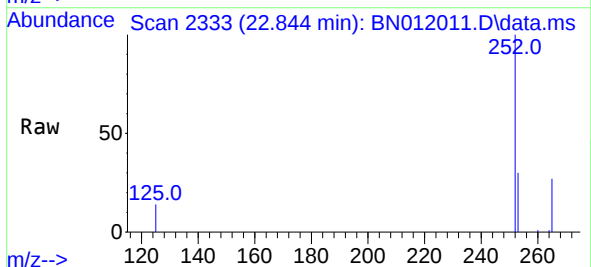




#39
Benzo(a)pyrene
Concen: 0.36 ng
RT: 23.364 min Scan# 2485
Delta R.T. -0.007 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 8388
Ion Ratio Lower Upper
252 100
253 34.3 19.8 29.6#
125 21.1 7.3 10.9#

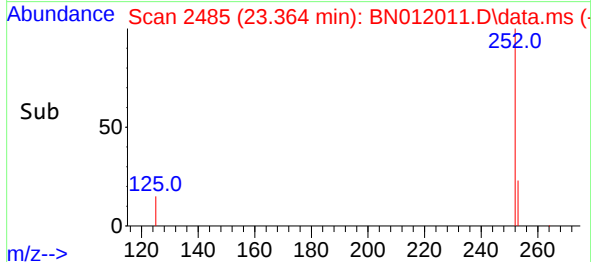

#40
Dibenzo(a,h)anthracene
Concen: 0.38 ng
RT: 25.685 min Scan# 3163
Delta R.T. -0.014 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Tgt Ion:278 Resp: 8978
Ion Ratio Lower Upper
278 100
139 15.8 8.6 13.0#
279 31.3 19.8 29.8#

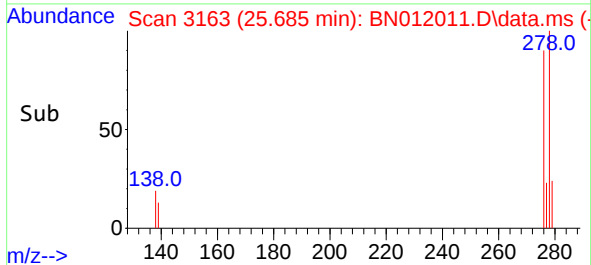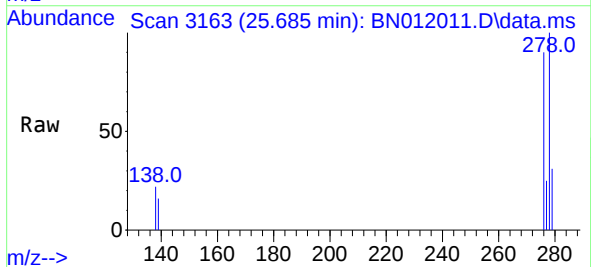

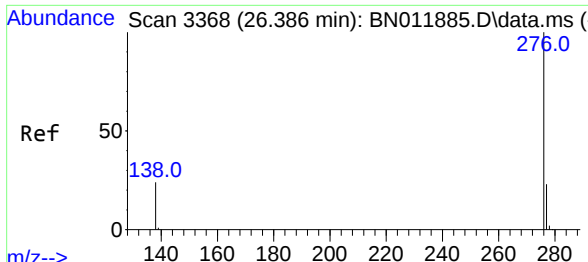

#41
Benzo(g,h,i)perylene
Concen: 0.37 ng
RT: 26.342 min Scan# 3355
Delta R.T. -0.017 min
Lab File: BN012011.D
Acq: 29 Sep 2020 08:42

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:276 Resp: 9629
Ion Ratio Lower Upper
276 100
277 25.5 19.4 29.0
138 20.9 11.3 16.9#

