
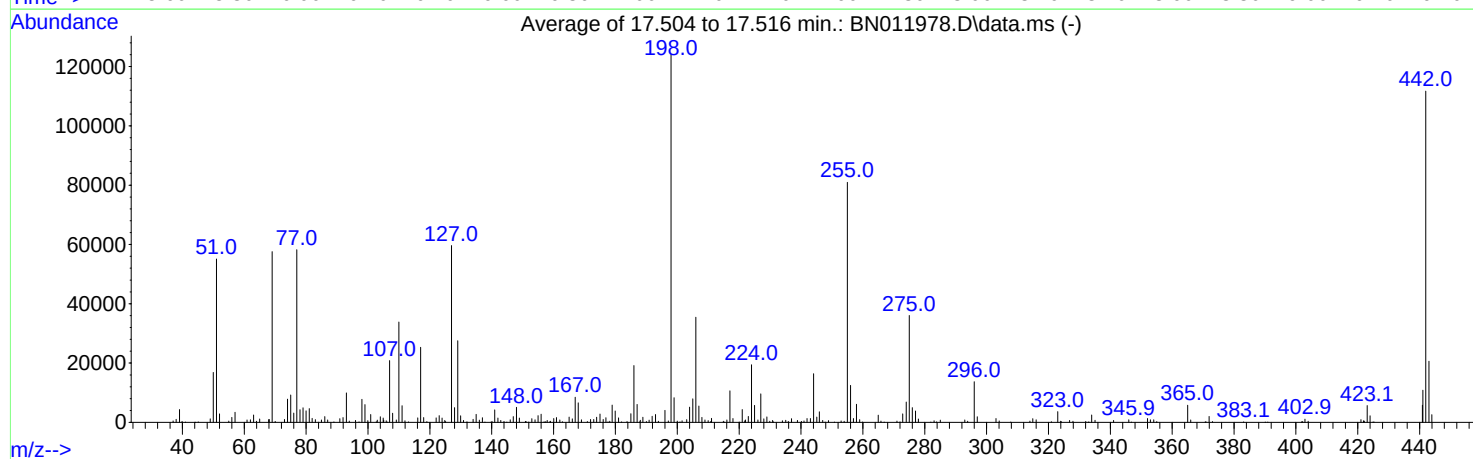


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092820\
 Data File : BN011978.D
 Acq On : 28 Sep 2020 09:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 29 10:58:58 2020

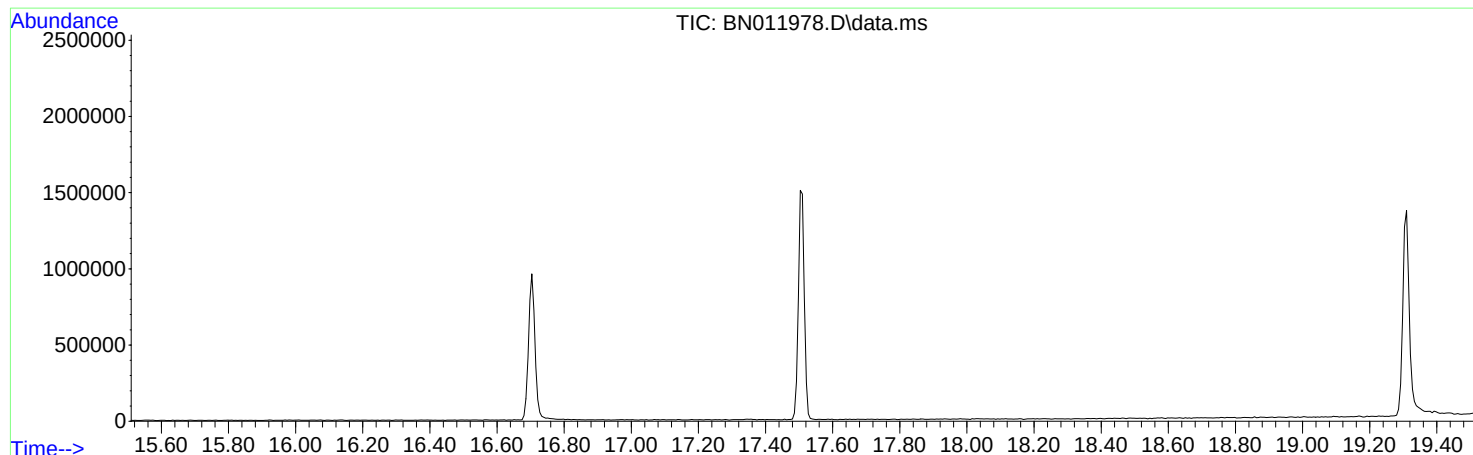

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	55096	PASS
68	69	0.00	2	1.7	995	PASS
69	198	0.00	100	46.4	57595	PASS
70	69	0.00	2	0.6	346	PASS
127	198	10	80	48.1	59640	PASS
197	198	0.00	2	0.4	471	PASS
198	198	100	100	100.0	124064	PASS
199	198	5	9	6.7	8325	PASS
275	198	10	60	29.1	36059	PASS
365	198	1	100	4.6	5768	PASS
441	198	0.01	100	8.8	10858	PASS
442	198	50	100	90.0	111709	PASS
443	442	15	24	18.5	20629	PASS