
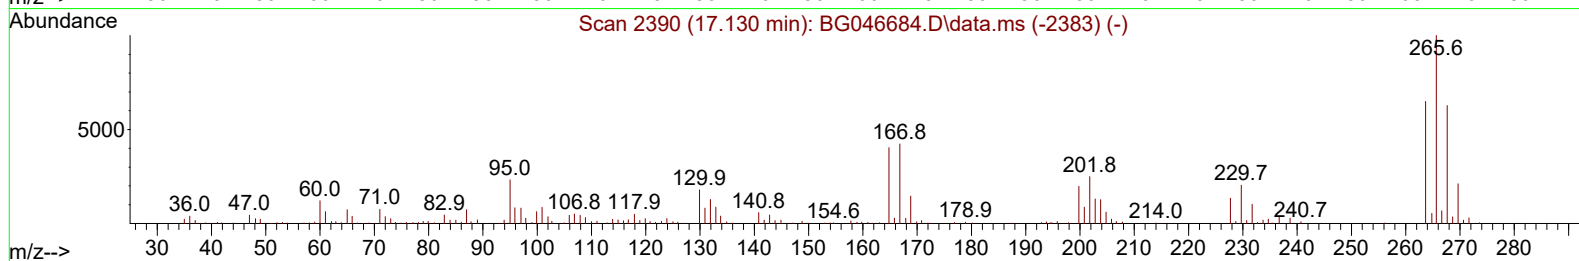
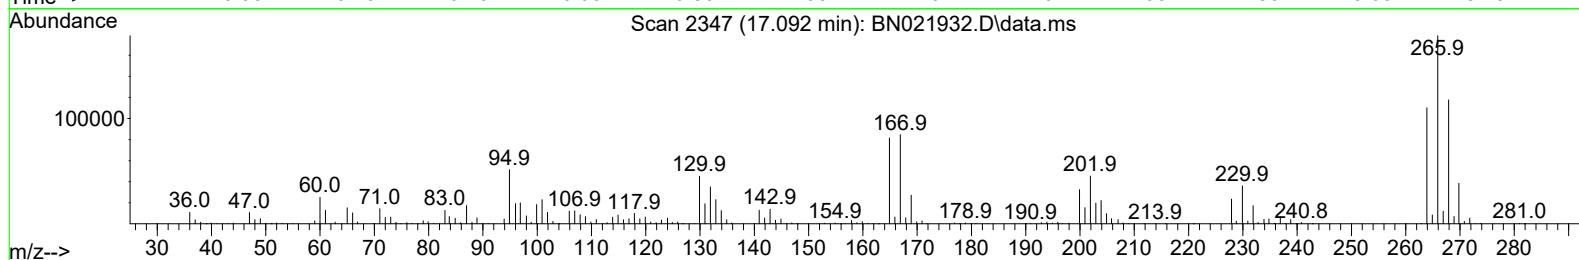


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN092822\  
Data File : BN021932.D  
Acq On : 27 Sep 2022 13:04  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 07:03:57 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 28 07:03:52 2022  
Response via : Initial Calibration

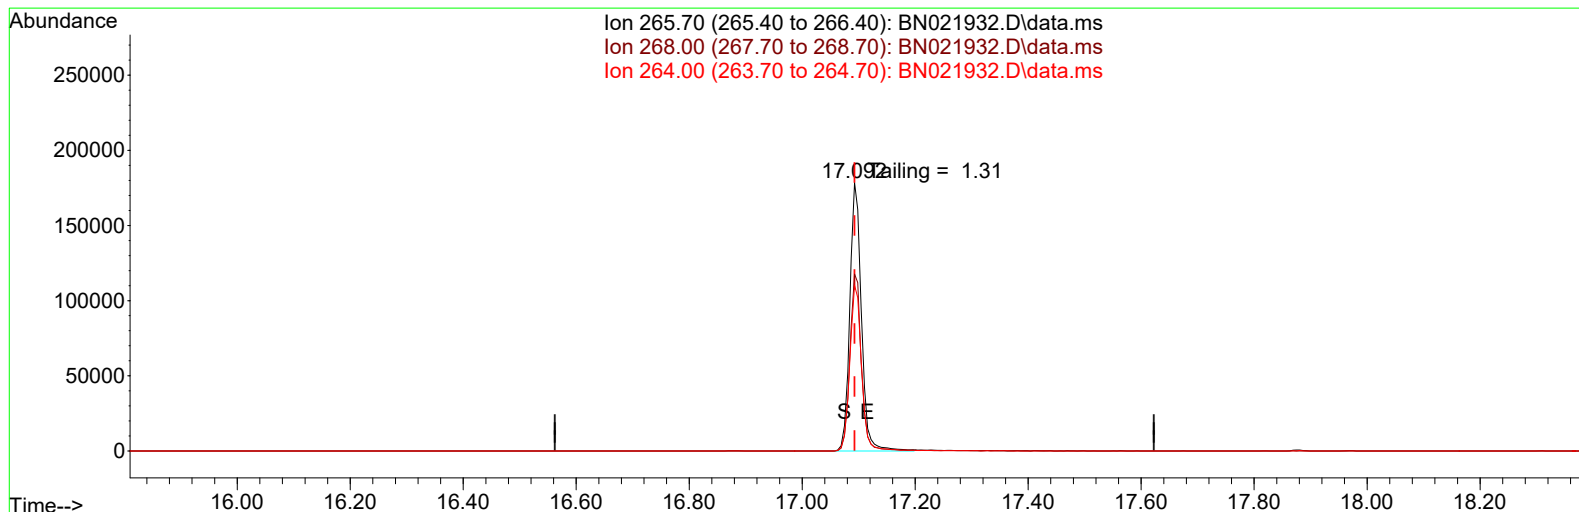

TIC: BN021932.D\data.ms

**(70) Pentachlorophenol (C)**




17.092min ( 0.000) 41659.27 ng

response 257622

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 65.92  |
| 264.00 | 61.60  | 61.73  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN092822\  
Data File : BN021932.D  
Acq On : 27 Sep 2022 13:04  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 07:03:57 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 28 07:03:52 2022  
Response via : Initial Calibration

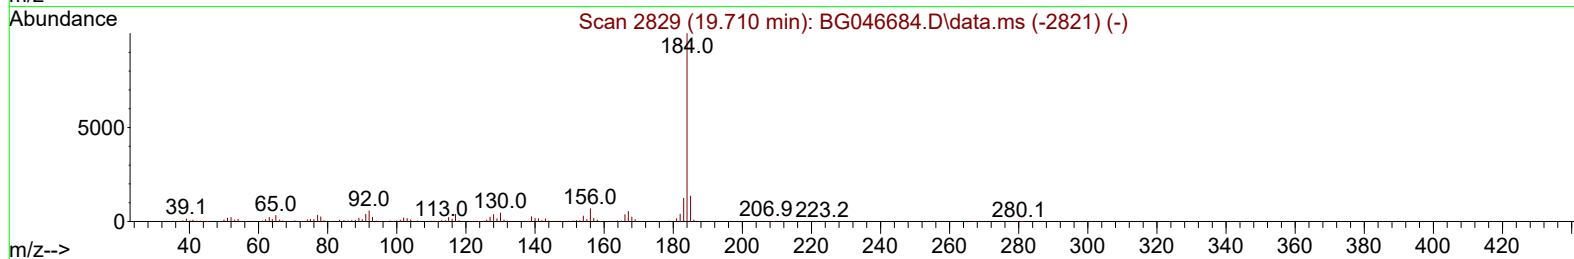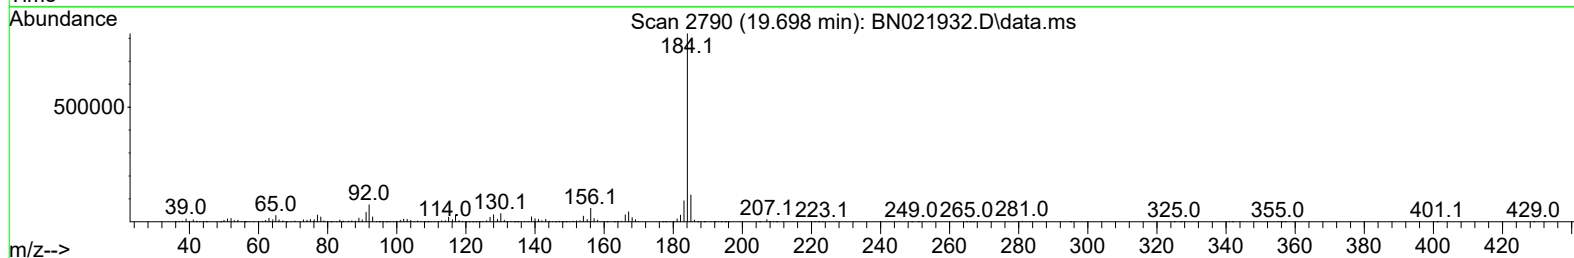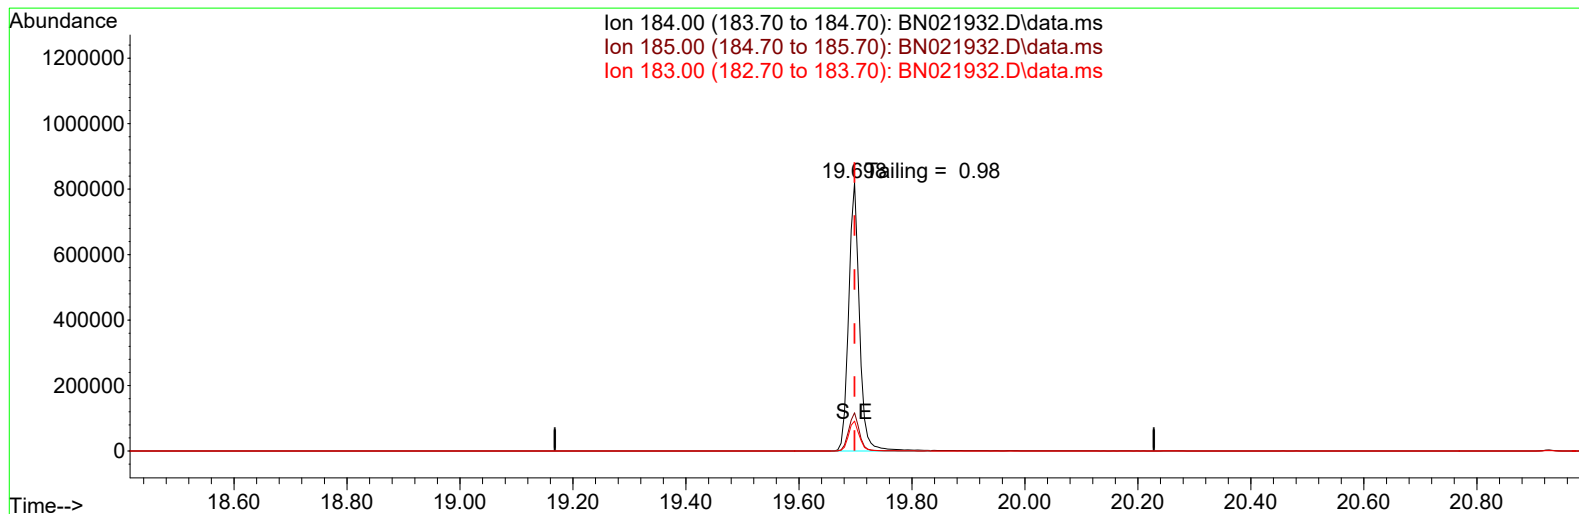

TIC: BN021932.D\data.ms

**(77) Benzidine****19.698min ( 0.000) 62954.60 ng****response 1098379**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.26  |
| 183.00 | 13.20  | 11.18  |
| 0.00   | 0.00   | 0.00   |